

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102419\
 Data File : FB022821.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2019 12:27
 Operator : DD/AJ
 Sample : BSF1024S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 25 00:28:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	515690	20.380 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	1006142	29.606 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	1118685	30.744 ng/ml
3) t n-Heptane	7.752	365034	10.004 ng/ml
4) t Benzene	7.887	437182	9.902 ng/ml
6) t Toluene	10.625	1271157	29.493 ng/ml
7) t Ethylbenzene	13.065	407454	10.032 ng/ml
8) t m-Xylene	13.199	763748	19.850 ng/ml
9) t O-Xylene	13.926	722021	19.824 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	567239	19.906 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102419\
Data File : FB022821.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2019 12:27
Operator : DD/AJ
Sample : BSF1024S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 00:28:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

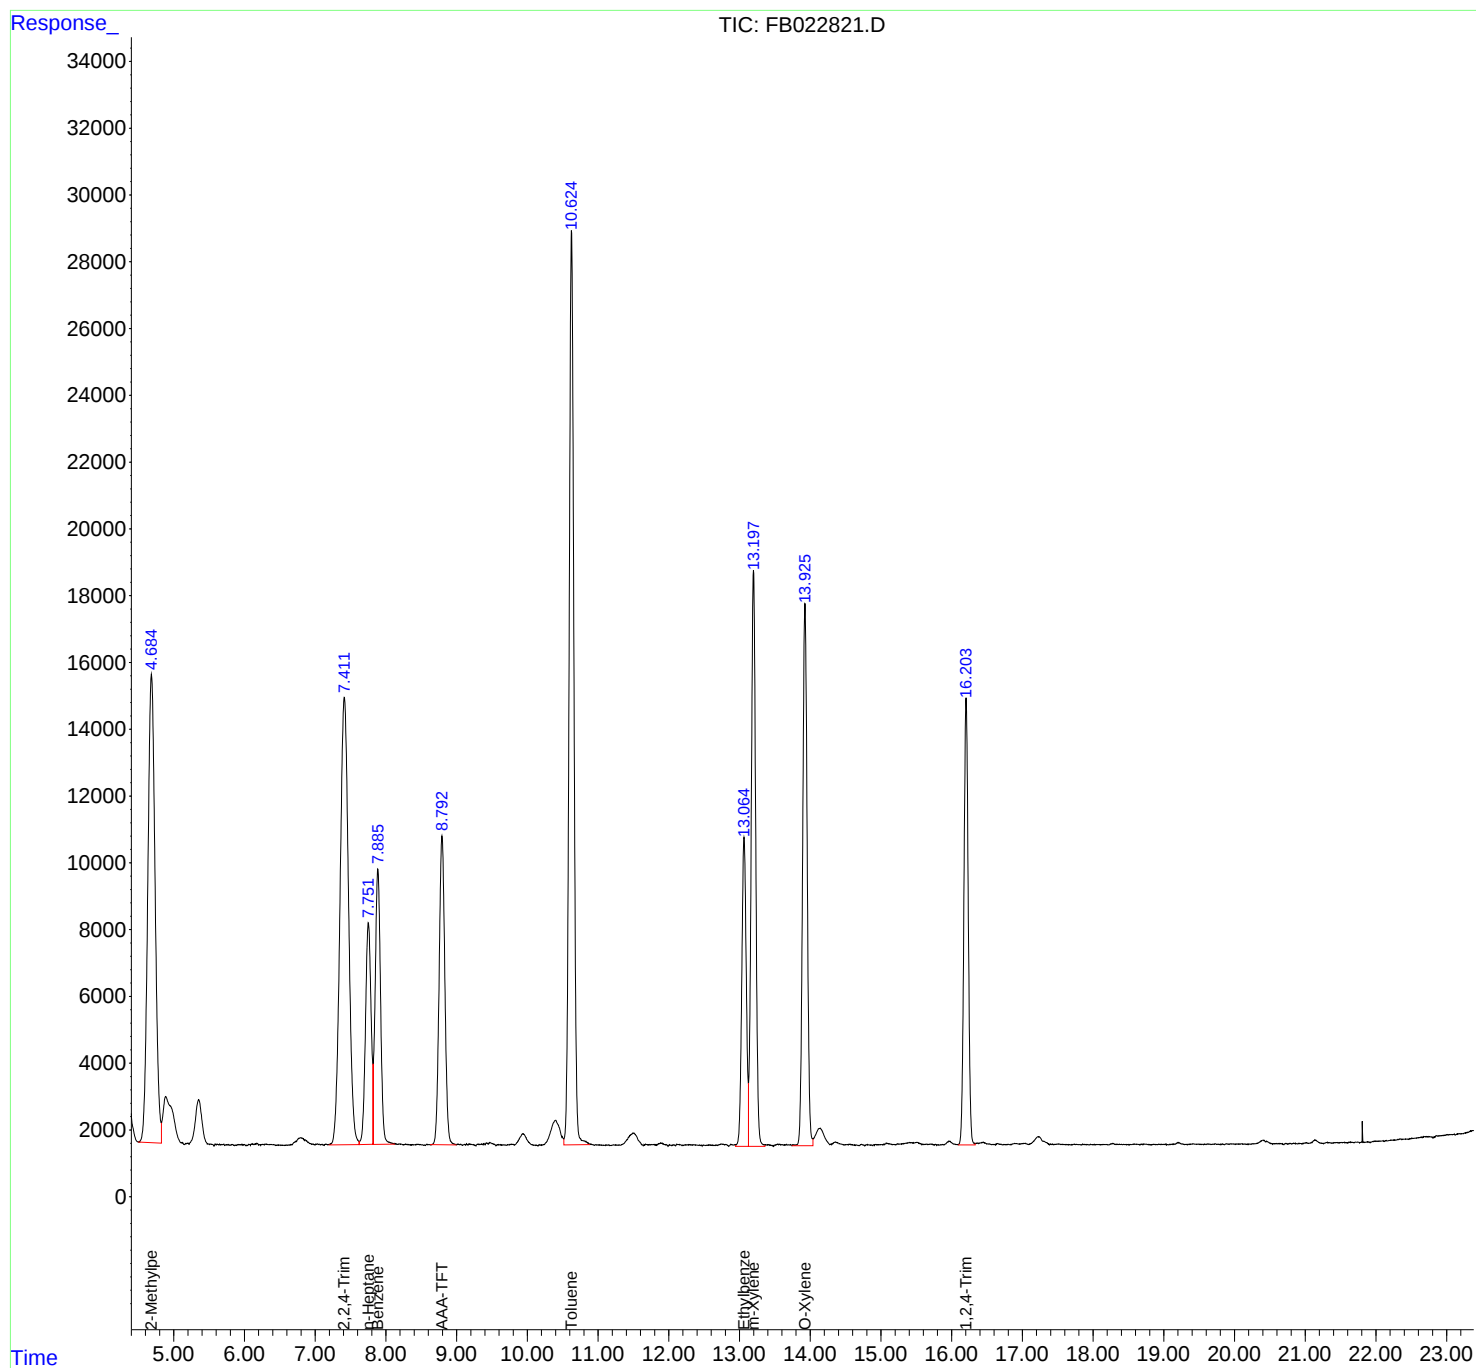

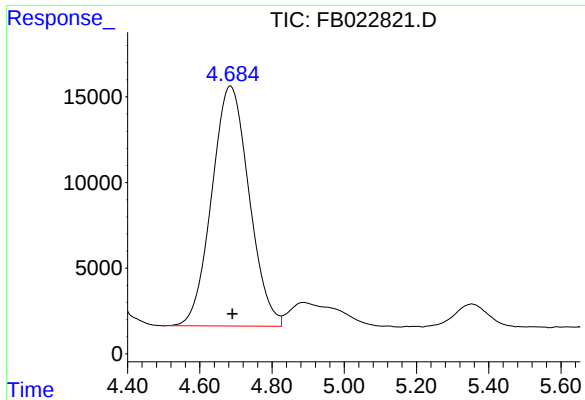


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.005 min
Response: 1006142
Conc: 29.61 ng/ml

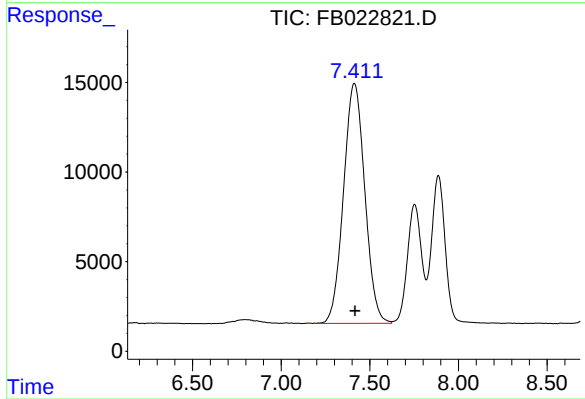


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 1118685
Conc: 30.74 ng/ml

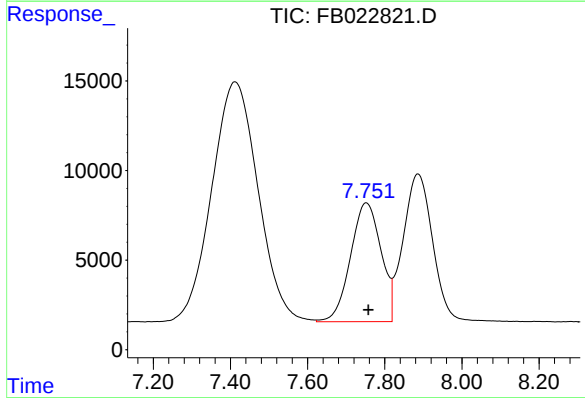


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.005 min
Response: 365034
Conc: 10.00 ng/ml

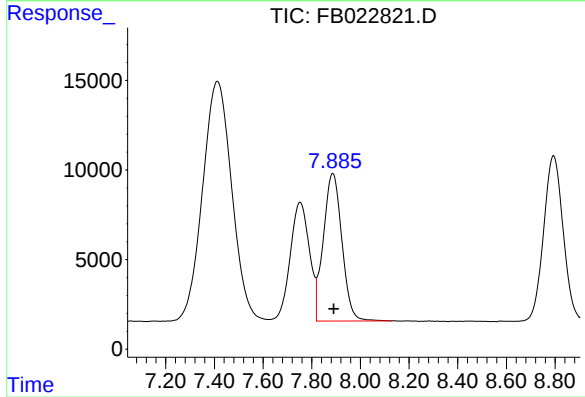


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.005 min
Response: 437182
Conc: 9.90 ng/ml

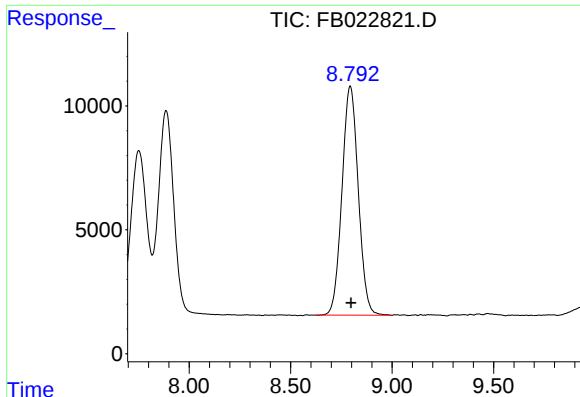


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.004 min
Response: 515690
Conc: 20.38 ng/ml

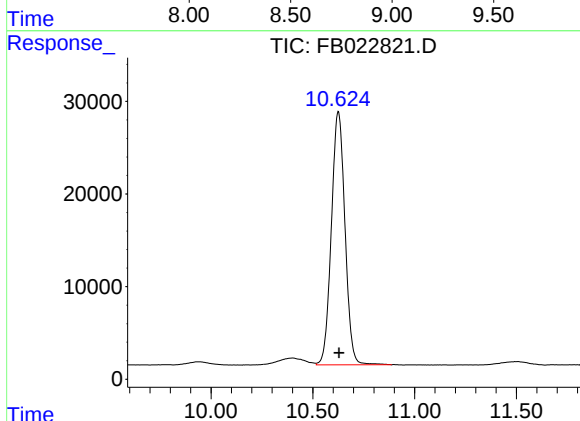


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.004 min
Response: 1271157
Conc: 29.49 ng/ml

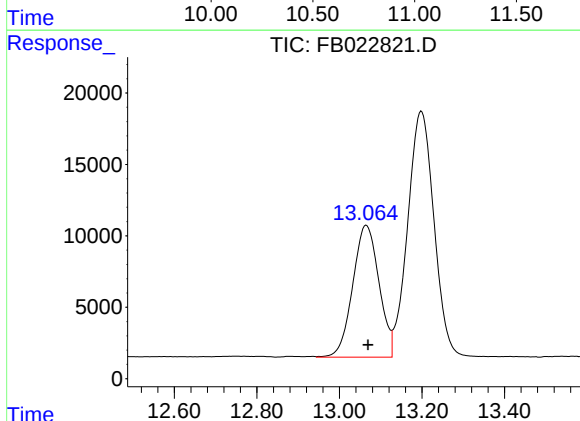


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.005 min
Response: 407454
Conc: 10.03 ng/ml

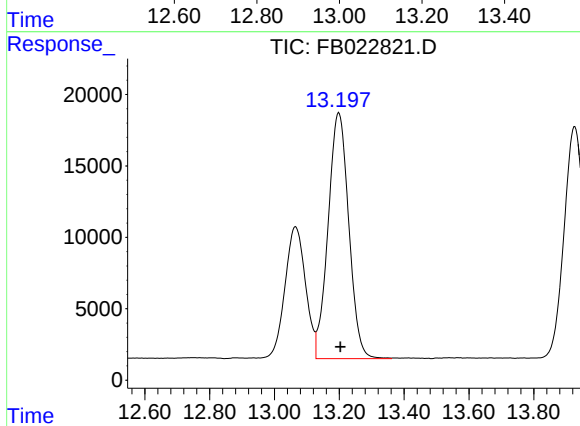


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.004 min
Response: 763748
Conc: 19.85 ng/ml

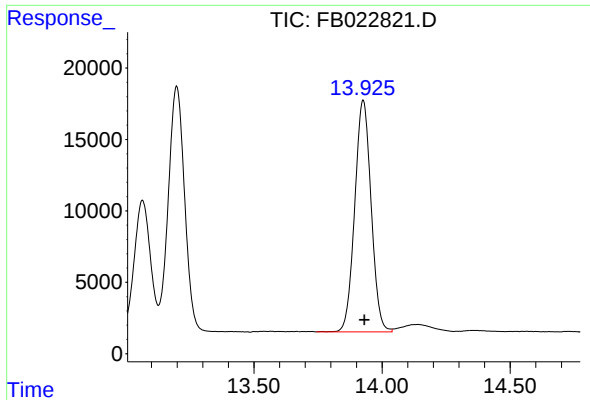

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.004 min
Response: 722021
Conc: 19.82 ng/ml

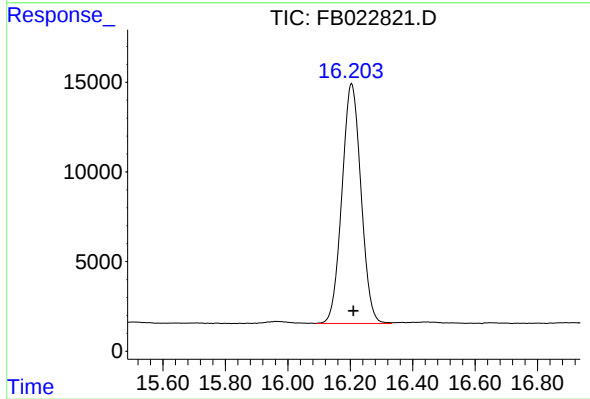

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.005 min
Response: 567239
Conc: 19.91 ng/ml