

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102419\
 Data File : FB022825.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2019 14:26
 Operator : DD/AJ
 Sample : K5145-05MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 25 00:28:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	511186	20.202 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	926762	27.270 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	956251	26.280 ng/ml
3) t n-Heptane	7.756	257085	7.046 ng/ml
4) t Benzene	7.890	413394	9.363 ng/ml
6) t Toluene	10.628	1193998	27.703 ng/ml
7) t Ethylbenzene	13.068	359683	8.856 ng/ml
8) t m-Xylene	13.201	672446	17.477 ng/ml
9) t O-Xylene	13.929	644139	17.686 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	476683	16.728 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102419\
Data File : FB022825.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2019 14:26
Operator : DD/AJ
Sample : K5145-05MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 00:28:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

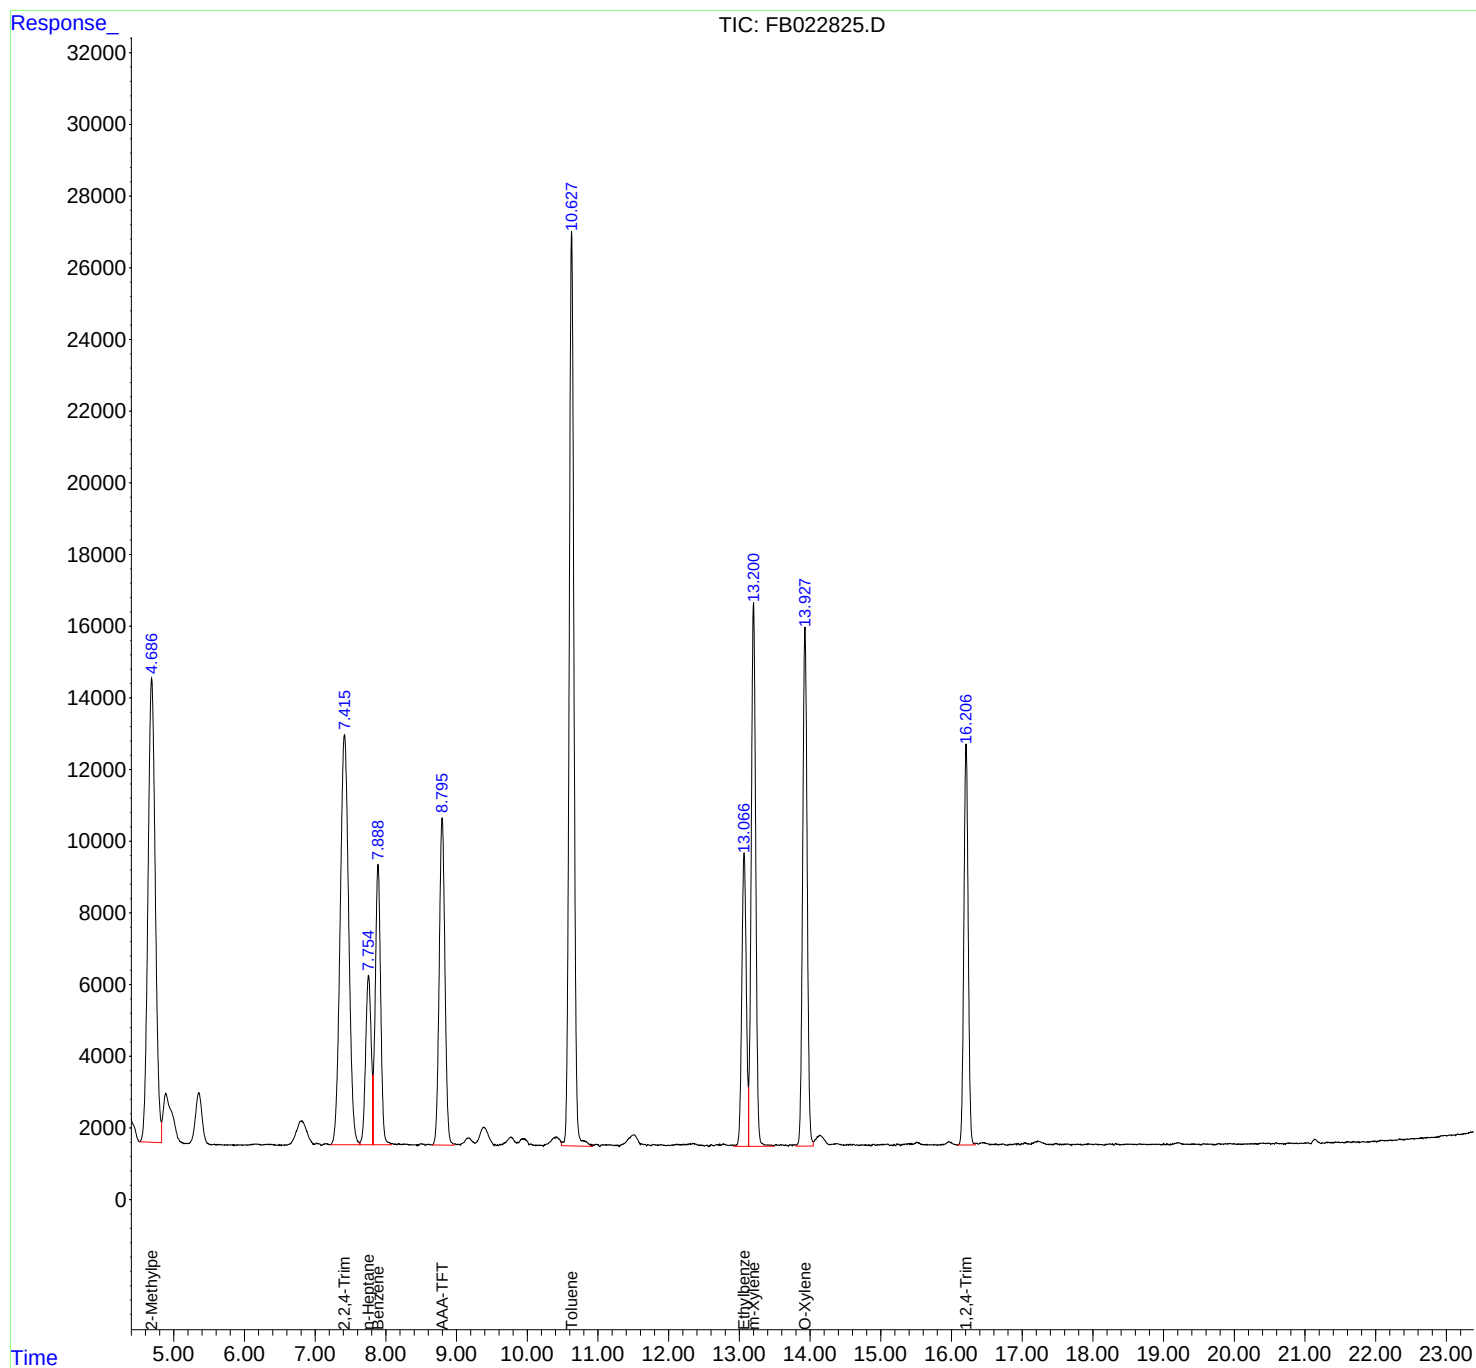

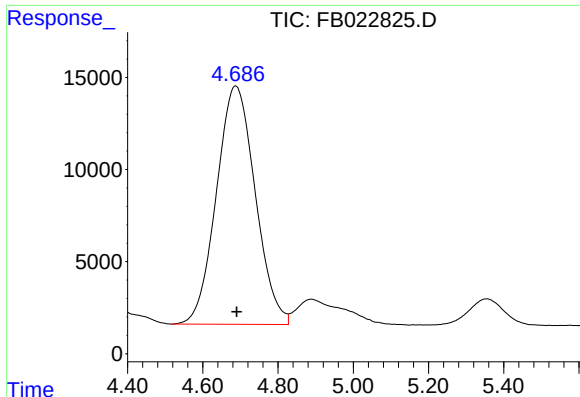


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 926762
Conc: 27.27 ng/ml

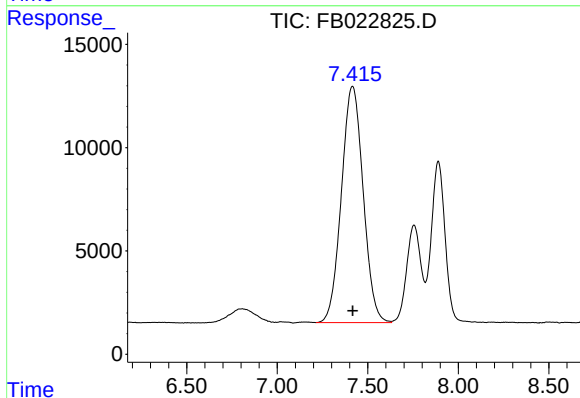


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 956251
Conc: 26.28 ng/ml

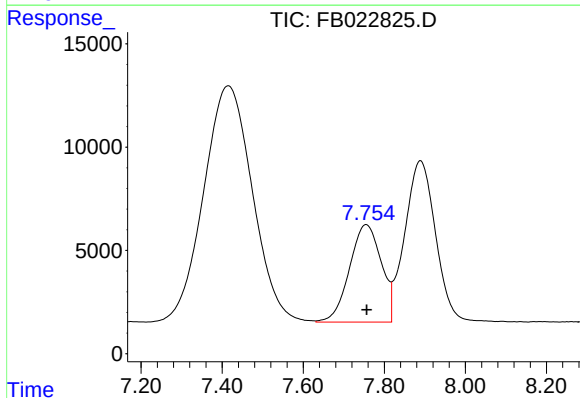


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.001 min
Response: 257085
Conc: 7.05 ng/ml

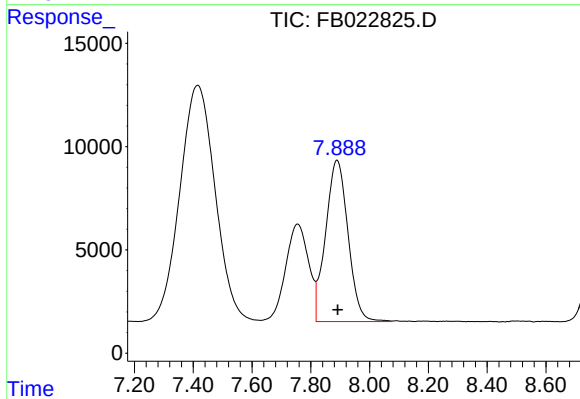


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 413394
Conc: 9.36 ng/ml

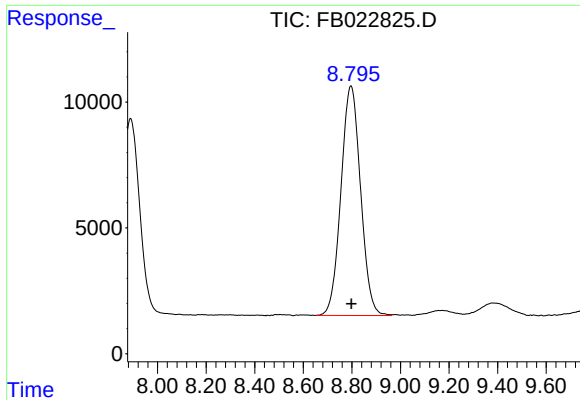


#5 AAA-TFT

R.T.: 8.797 min
 Delta R.T.: -0.002 min
 Response: 511186
 Conc: 20.20 ng/ml

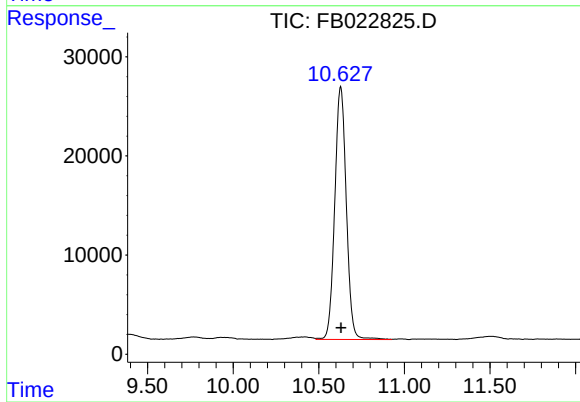


#6 Toluene

R.T.: 10.628 min
 Delta R.T.: -0.002 min
 Response: 1193998
 Conc: 27.70 ng/ml

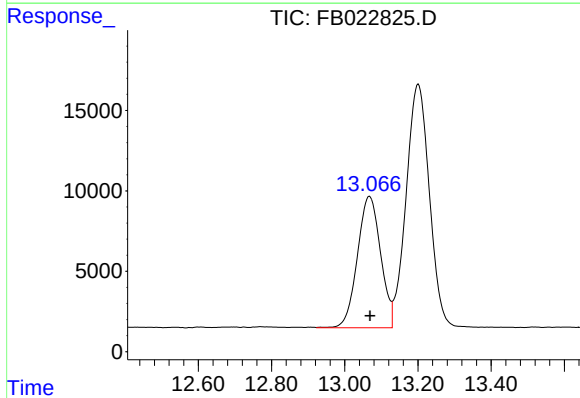


#7 Ethylbenzene

R.T.: 13.068 min
 Delta R.T.: -0.002 min
 Response: 359683
 Conc: 8.86 ng/ml

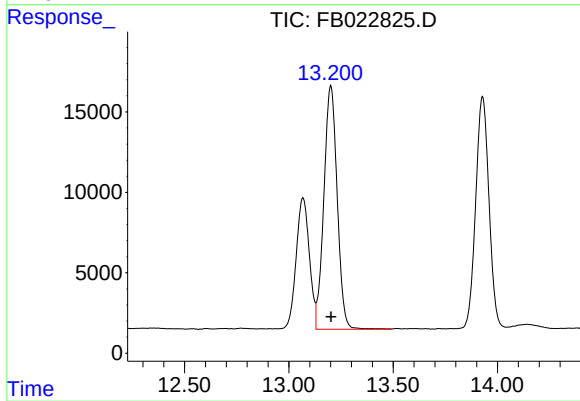


#8 m-Xylene

R.T.: 13.201 min
 Delta R.T.: -0.002 min
 Response: 672446
 Conc: 17.48 ng/ml

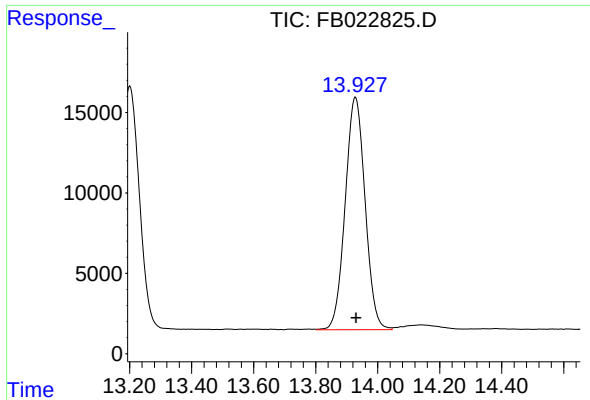

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 644139
Conc: 17.69 ng/ml

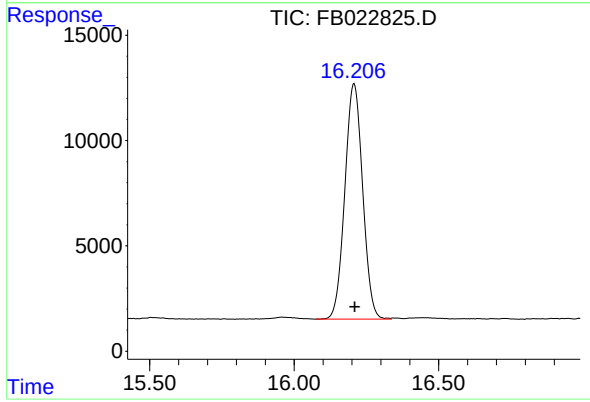

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 476683
Conc: 16.73 ng/ml