

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
 Data File : FB028696.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2022 13:06
 Operator : AJ/MA
 Sample : BSF1024S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 25 08:32:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	242803	18.768 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	472431	28.879 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	528495	29.244 ng/ml
3) t n-Heptane	7.751	159896	9.440 ng/ml
4) t Benzene	7.887	201180	9.159 ng/ml
6) t Toluene	10.621	571329	27.258 ng/ml
7) t Ethylbenzene	13.057	179725	9.056 ng/ml
8) t m-Xylene	13.190	357116	18.127 ng/ml
9) t O-Xylene	13.917	356875	18.344 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	358477	18.517 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
Data File : FB028696.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2022 13:06
Operator : AJ/MA
Sample : BSF1024S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 08:32:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

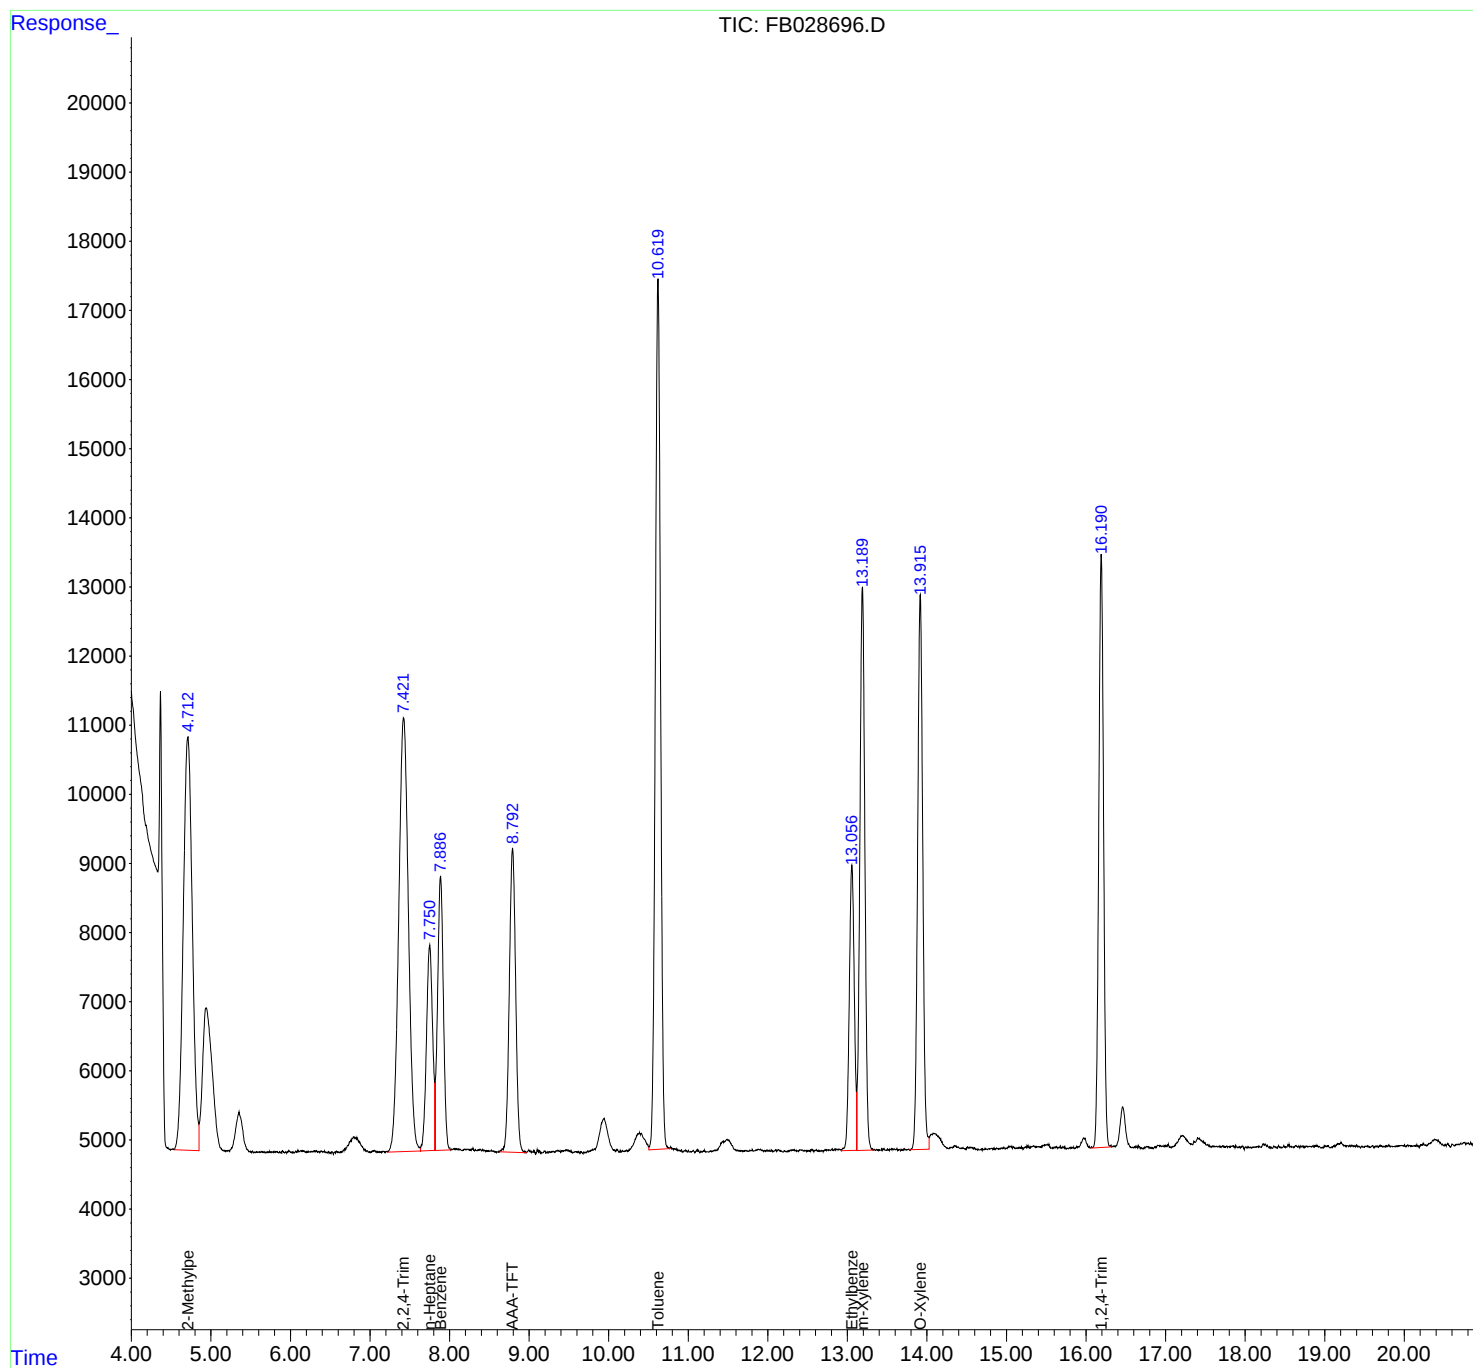


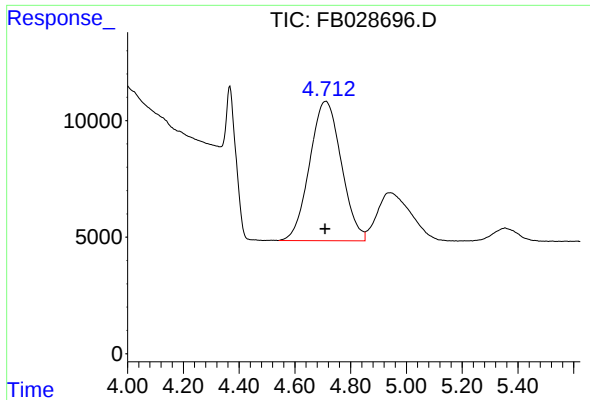

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.004 min
Response: 472431
Conc: 28.88 ng/ml

Instrument :
FID_B
ClientSampleId :

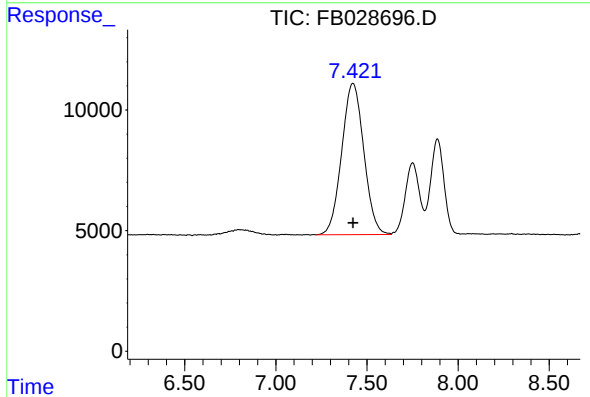


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 528495
Conc: 29.24 ng/ml

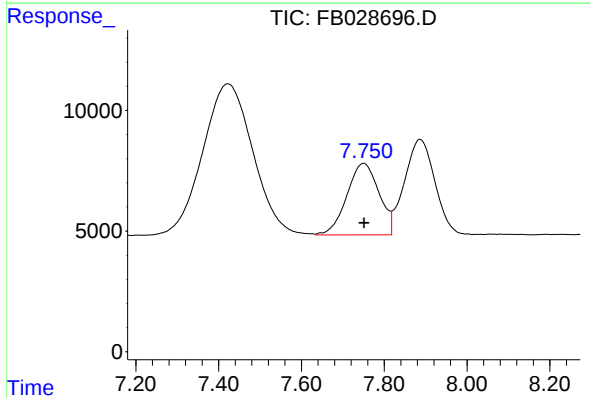


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 159896
Conc: 9.44 ng/ml

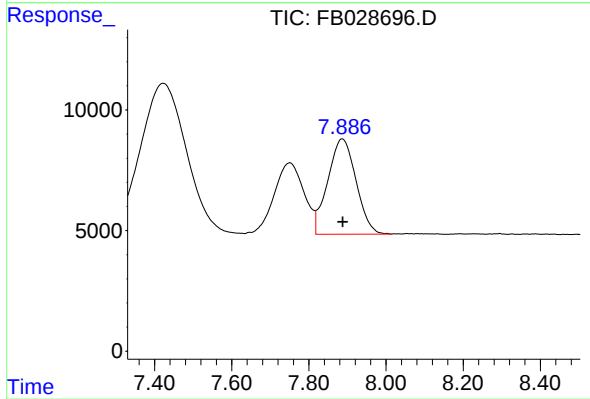

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 201180
Conc: 9.16 ng/ml

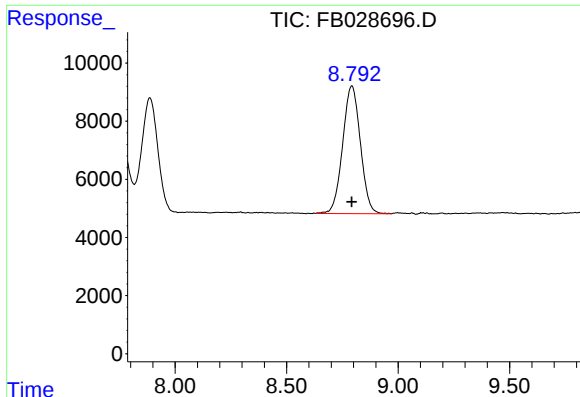

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 242803
Conc: 18.77 ng/ml

Instrument :
FID_B
ClientSampleId :

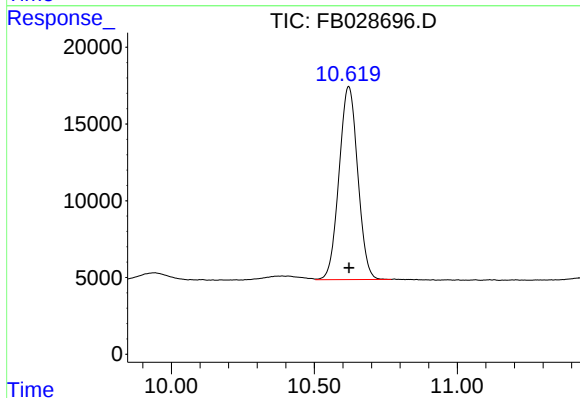


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 571329
Conc: 27.26 ng/ml

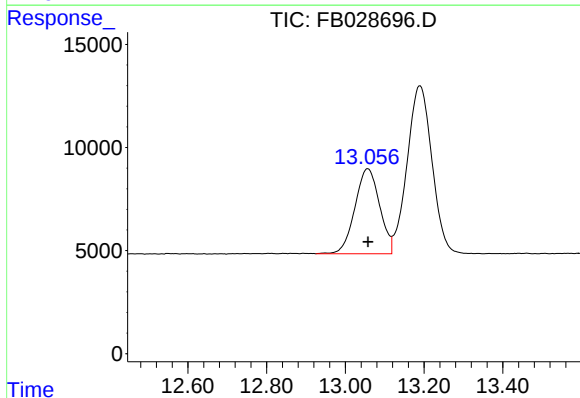


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 179725
Conc: 9.06 ng/ml

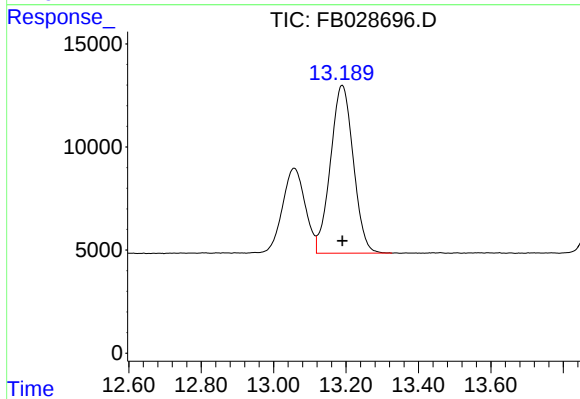

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 357116
Conc: 18.13 ng/ml

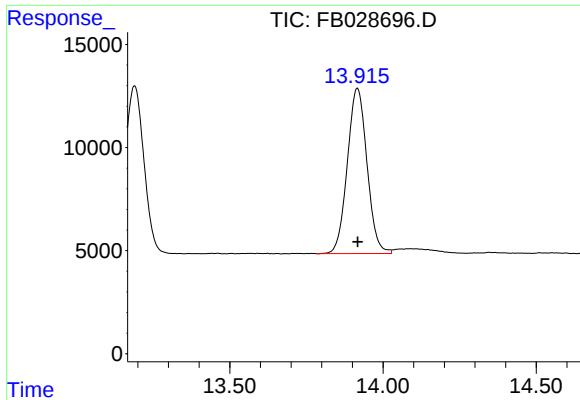

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 356875
Conc: 18.34 ng/ml

Instrument :
FID_B
ClientSampleId :

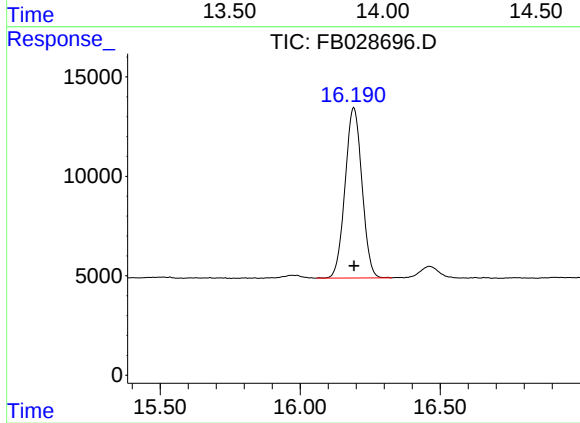

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.001 min
Response: 358477
Conc: 18.52 ng/ml