

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
Data File : FB028700.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2022 15:49
Operator : AJ/MA
Sample : N5193-11 50X
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 08:32:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

1) t	2-Methylpentane	4.703	498051	30.445 ng/ml
2) t	2,2,4-Trimethylpentane	7.411	2171044	120.132 ng/ml
3) t	n-Heptane	7.755	4885192	288.411 ng/ml
6) t	Toluene	10.678	2457836	117.263 ng/ml
7) t	Ethylbenzene	13.021	13812722	695.981 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
Data File : FB028700.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2022 15:49
Operator : AJ/MA
Sample : N5193-11 50X
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 08:32:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

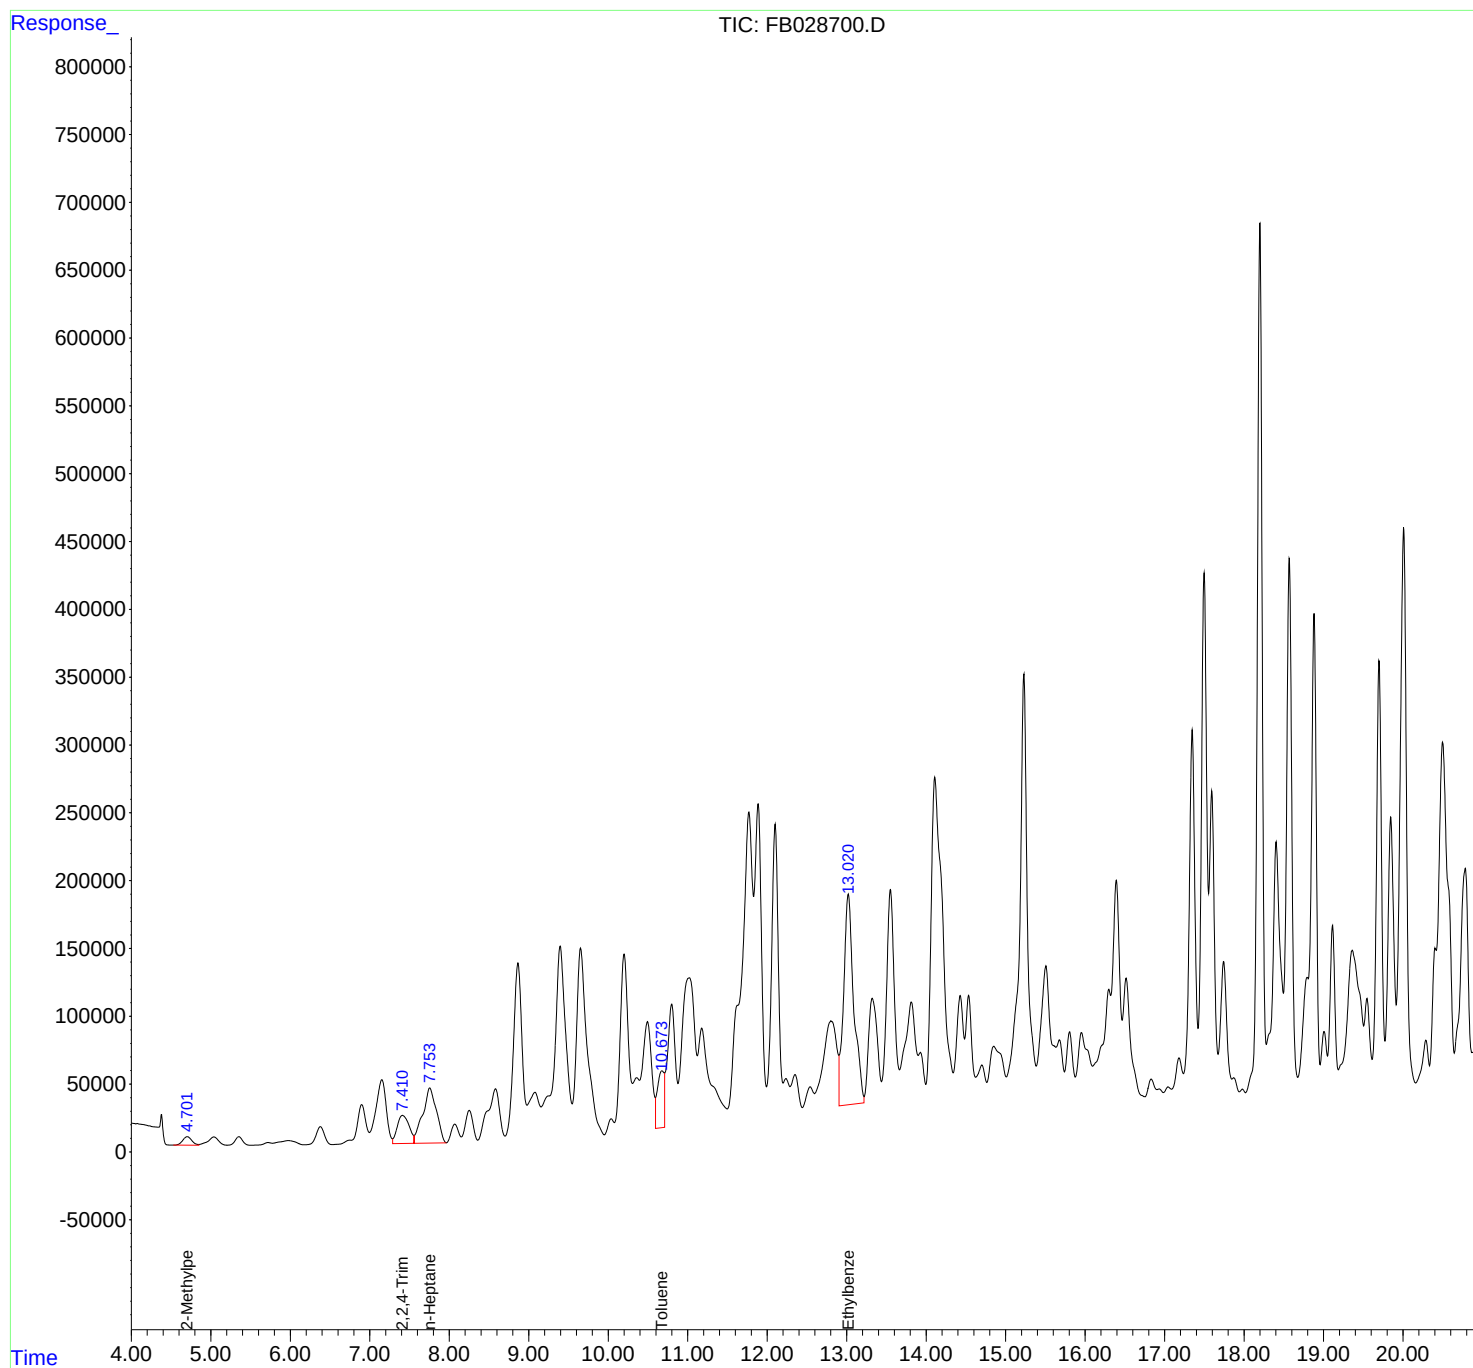


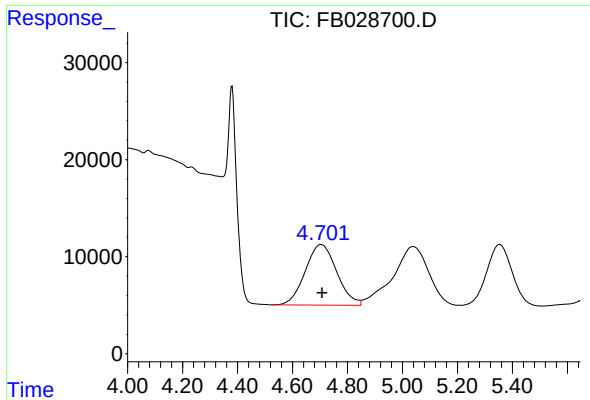

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.005 min
Response: 498051
Conc: 30.45 ng/ml

Instrument :
FID_B
ClientSampleId :

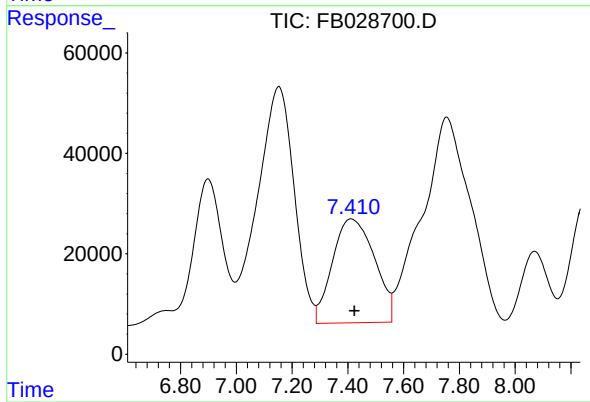


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.012 min
Response: 2171044
Conc: 120.13 ng/ml

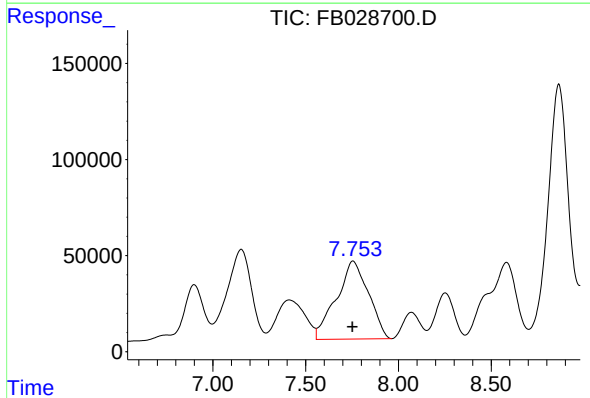


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.003 min
Response: 4885192
Conc: 288.41 ng/ml

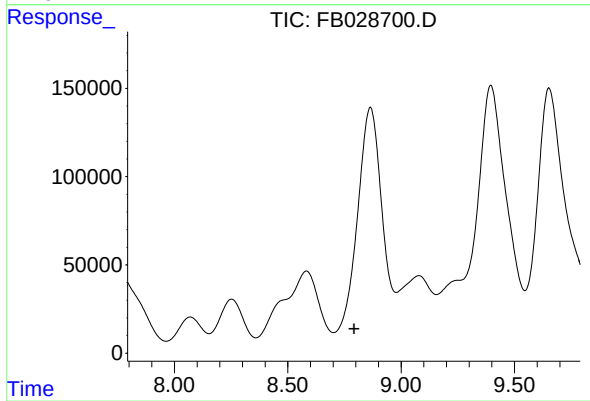

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T.: 8.793 min
Response: 0
Conc: N.D.

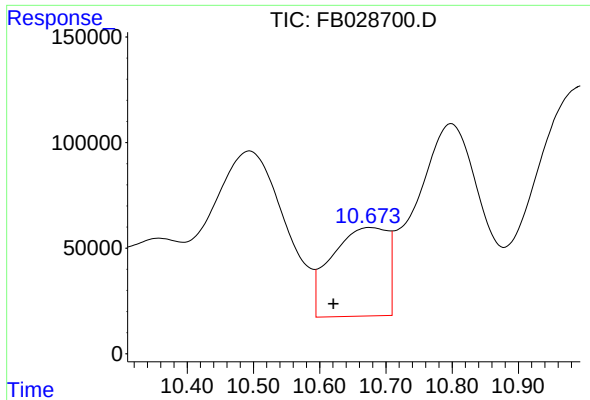

#6 Toluene

R.T.: 10.678 min
Delta R.T.: 0.057 min
Response: 2457836
Conc: 117.26 ng/ml

Instrument :
FID_B
ClientSampleId :

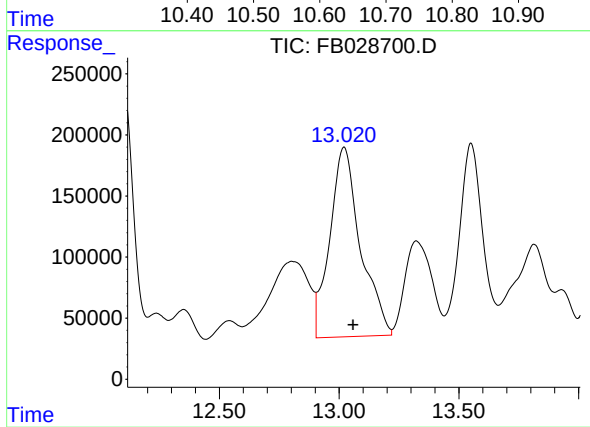

#7 Ethylbenzene

R.T.: 13.021 min
Delta R.T.: -0.037 min
Response: 13812722
Conc: 695.98 ng/ml