

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
Data File : FB028701.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2022 16:28
Operator : AJ/MA
Sample : N5193-13 50X
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 08:32:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

1) t	2-Methylpentane	4.705	222244	13.585 ng/ml
2) t	2,2,4-Trimethylpentane	7.388	1184771	65.558 ng/ml
3) t	n-Heptane	7.804	1683644	99.399 ng/ml
7) t	Ethylbenzene	13.030	6034634	304.067 ng/ml
9) t	O-Xylene	13.923	1738644	89.369 ng/ml
10) t	1,2,4-Trimethylbenzene	16.195	1089747	56.291 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
Data File : FB028701.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2022 16:28
Operator : AJ/MA
Sample : N5193-13 50X
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 08:32:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

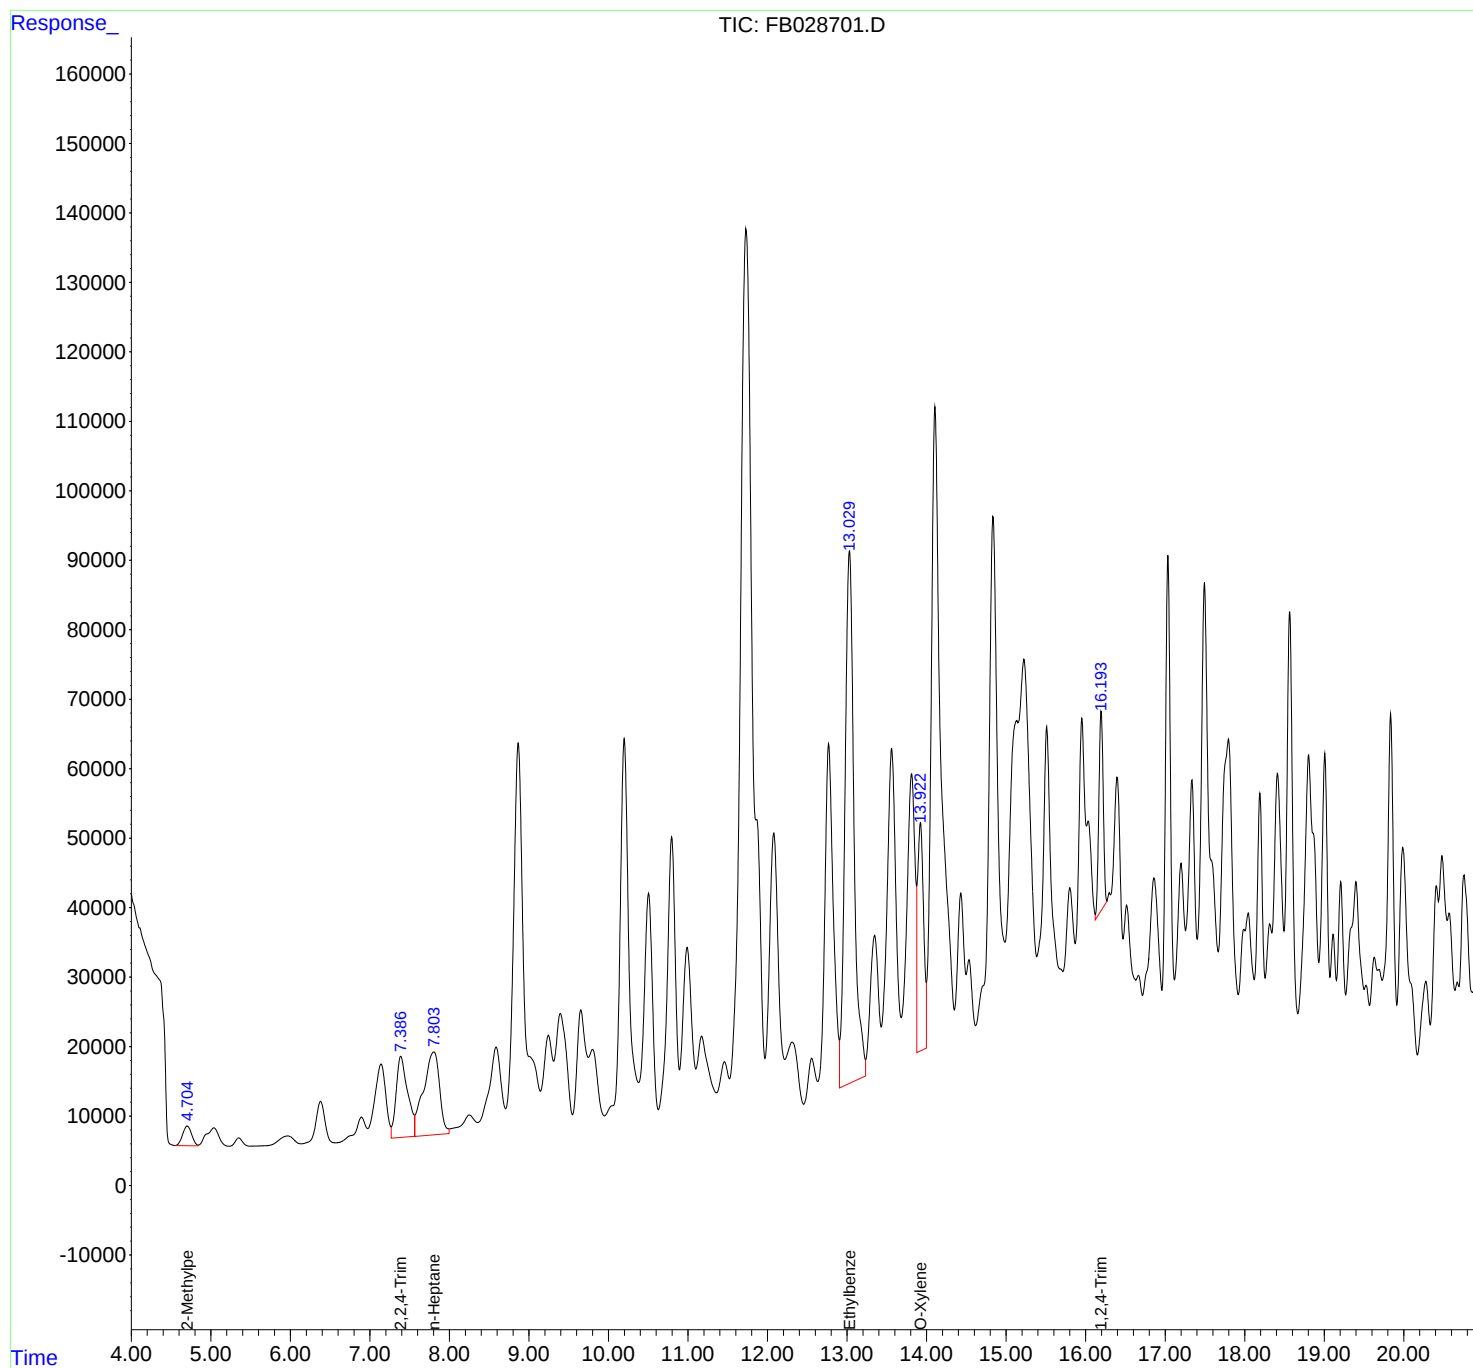


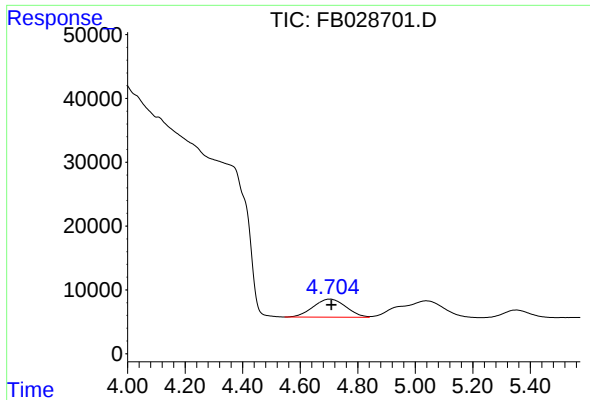

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.003 min
Response: 222244
Conc: 13.59 ng/ml

Instrument :
FID_B
ClientSampleId :

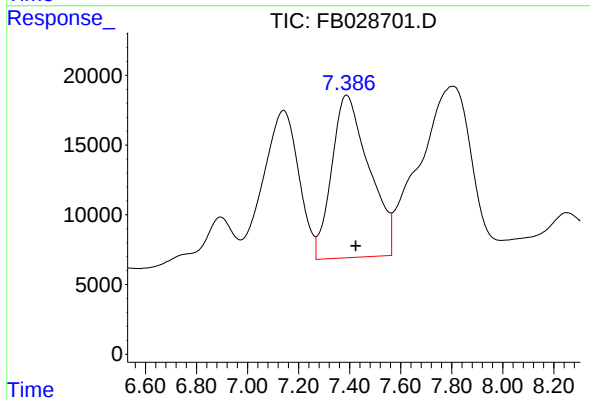


#2 2,2,4-Trimethylpentane

R.T.: 7.388 min
Delta R.T.: -0.036 min
Response: 1184771
Conc: 65.56 ng/ml

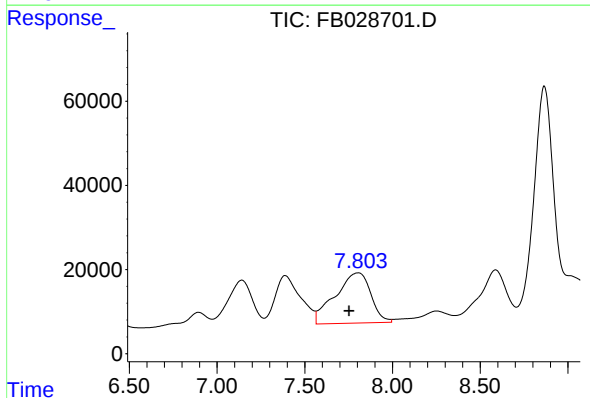


#3 n-Heptane

R.T.: 7.804 min
Delta R.T.: 0.053 min
Response: 1683644
Conc: 99.40 ng/ml

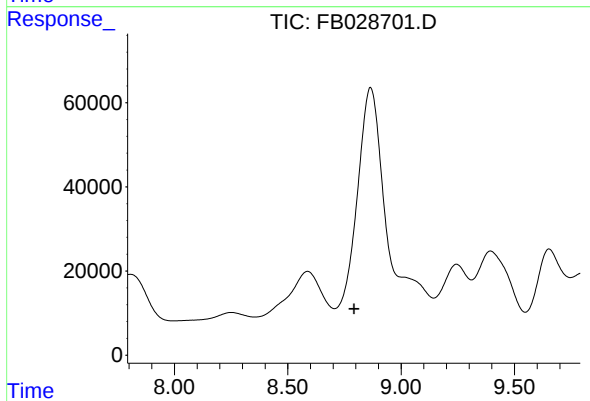

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T.: 8.793 min
Response: 0
Conc: N.D.

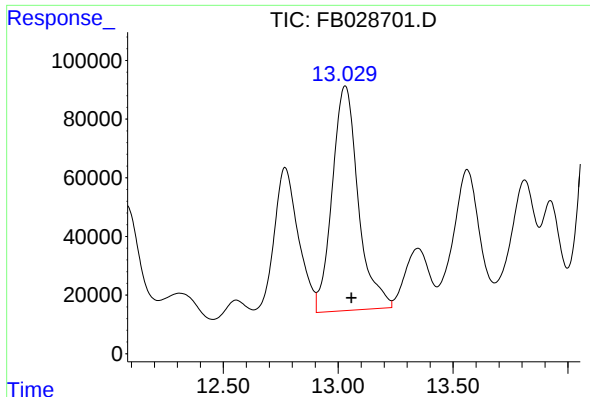

#7 Ethylbenzene


R.T.: 13.030 min
Delta R.T.: -0.028 min
Response: 6034634
Conc: 304.07 ng/ml

Instrument :
FID_B
ClientSampleId :

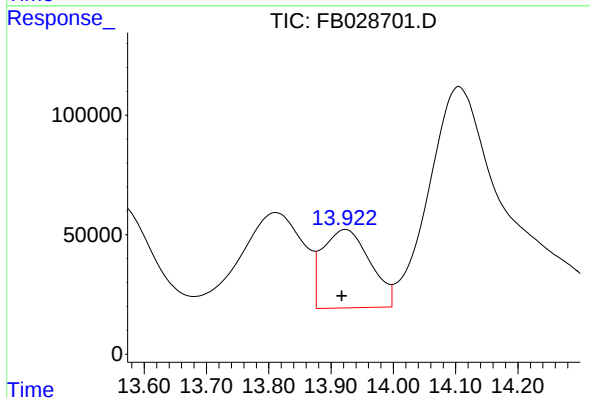

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.005 min
Response: 1738644
Conc: 89.37 ng/ml

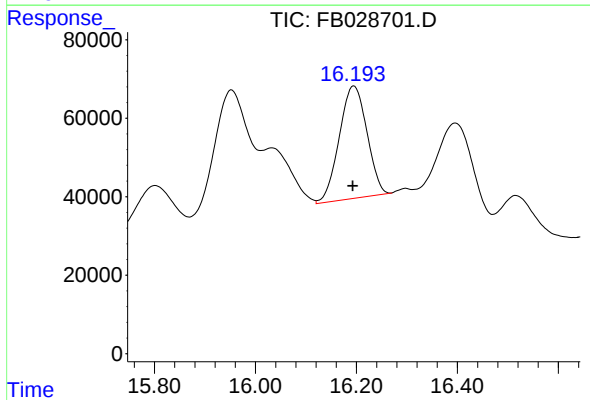

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 1089747
Conc: 56.29 ng/ml