

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102422\  
Data File : FB028702.D  
Signal(s) : FID2B.CH  
Acq On : 24 Oct 2022 17:08  
Operator : AJ/MA  
Sample : N5217-02  
Misc : 5.03G/5.00 ML DI WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 25 08:32:50 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 8) t m-Xylene               | 13.229 | 2500     | 0.127 ng/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102422\  
Data File : FB028702.D  
Signal(s) : FID2B.CH  
Acq On : 24 Oct 2022 17:08  
Operator : AJ/MA  
Sample : N5217-02  
Misc : 5.03G/5.00 ML DI WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 25 08:32:50 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

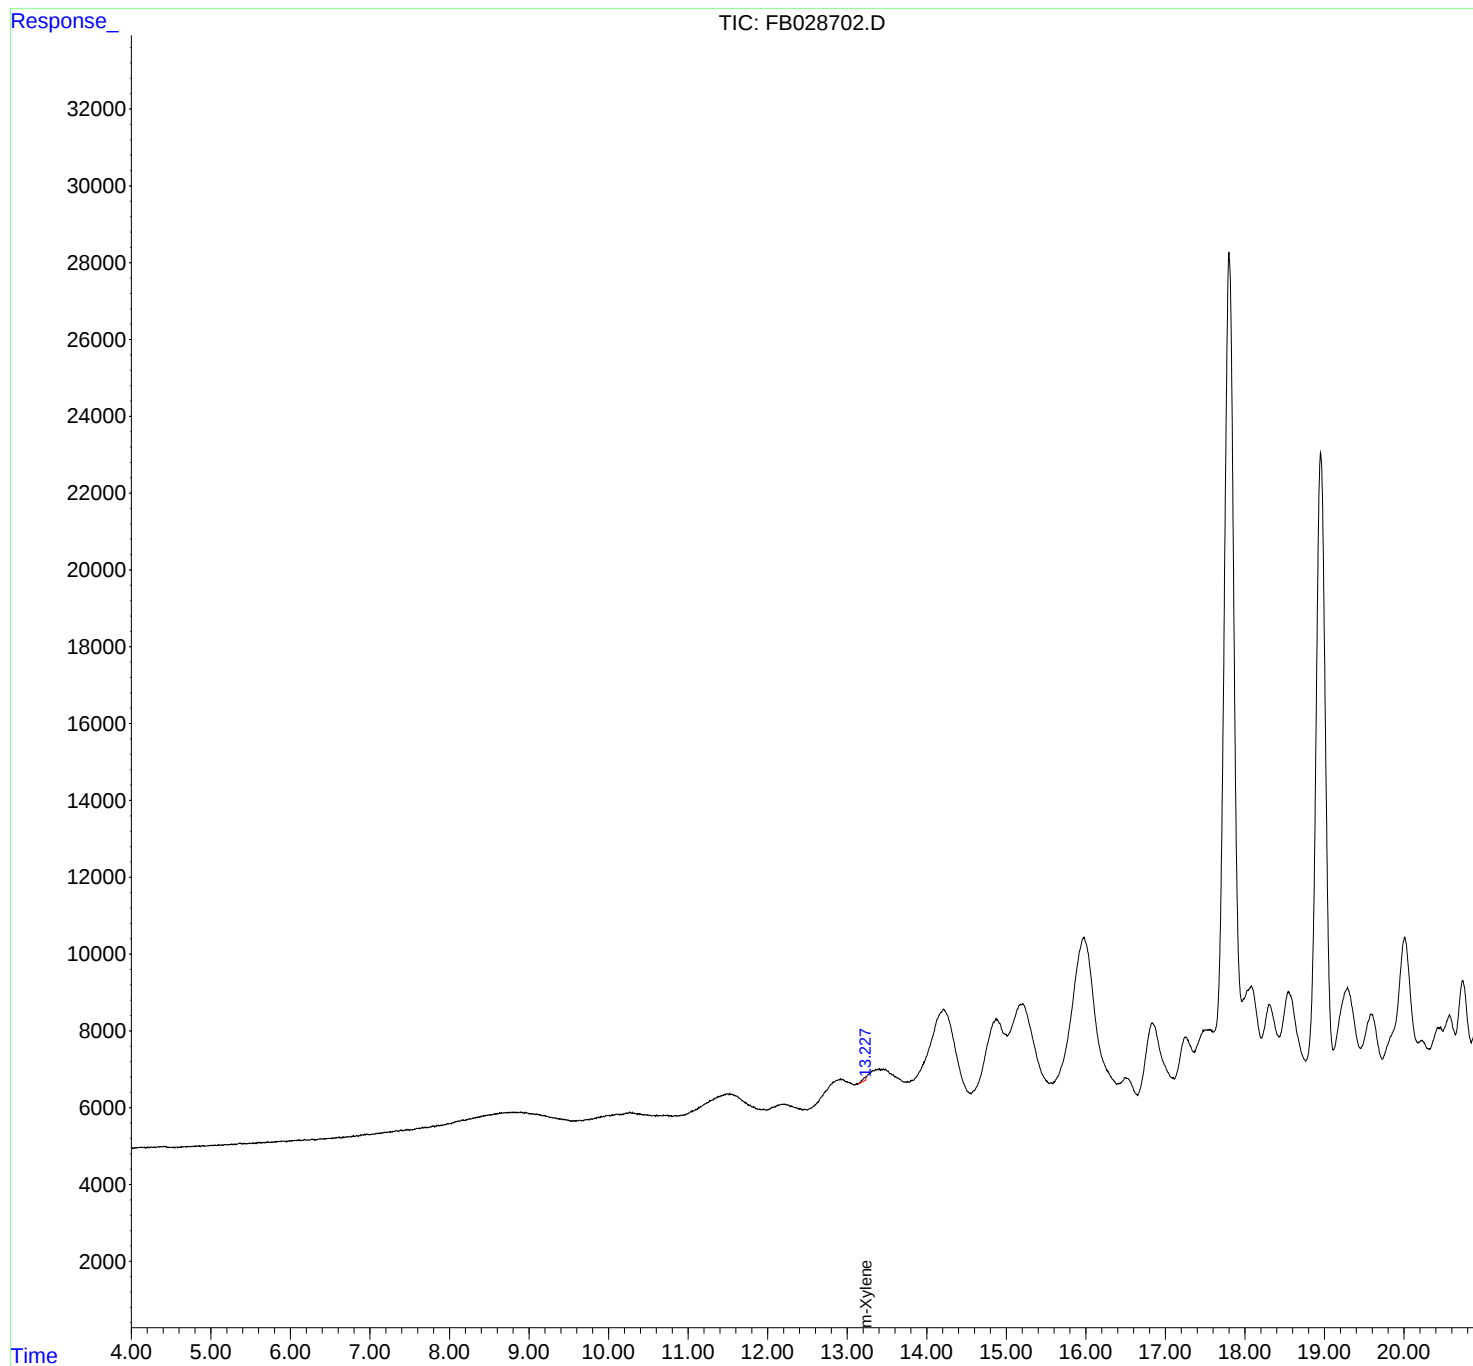


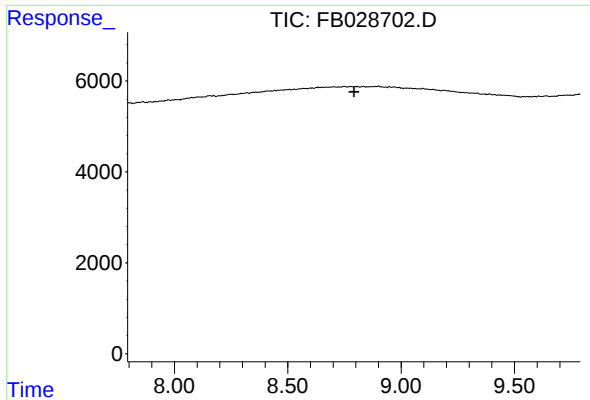

#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T.: 8.793 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_B  
ClientSampleId :

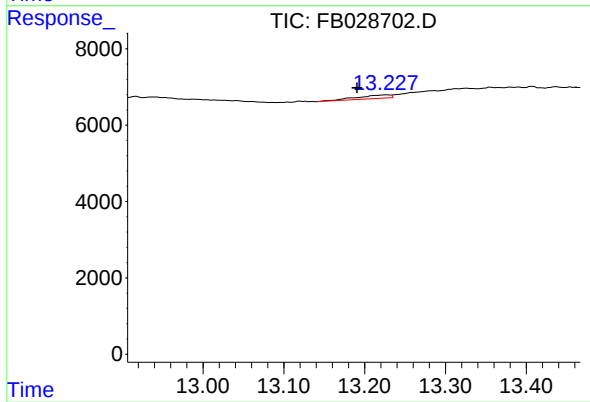

#8 m-Xylene

R.T.: 13.229 min  
Delta R.T.: 0.038 min  
Response: 2500  
Conc: 0.13 ng/ml