

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
Data File : FB028702.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2022 17:08
Operator : AJ/MA
Sample : N5217-02
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-A1-COMP

Integration File: Calibration.e
Quant Time: Oct 25 08:32:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
8) t m-Xylene	13.229	2500	0.127 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
Data File : FB028702.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2022 17:08
Operator : AJ/MA
Sample : N5217-02
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-A1-COMP

Integration File: Calibration.e
Quant Time: Oct 25 08:32:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

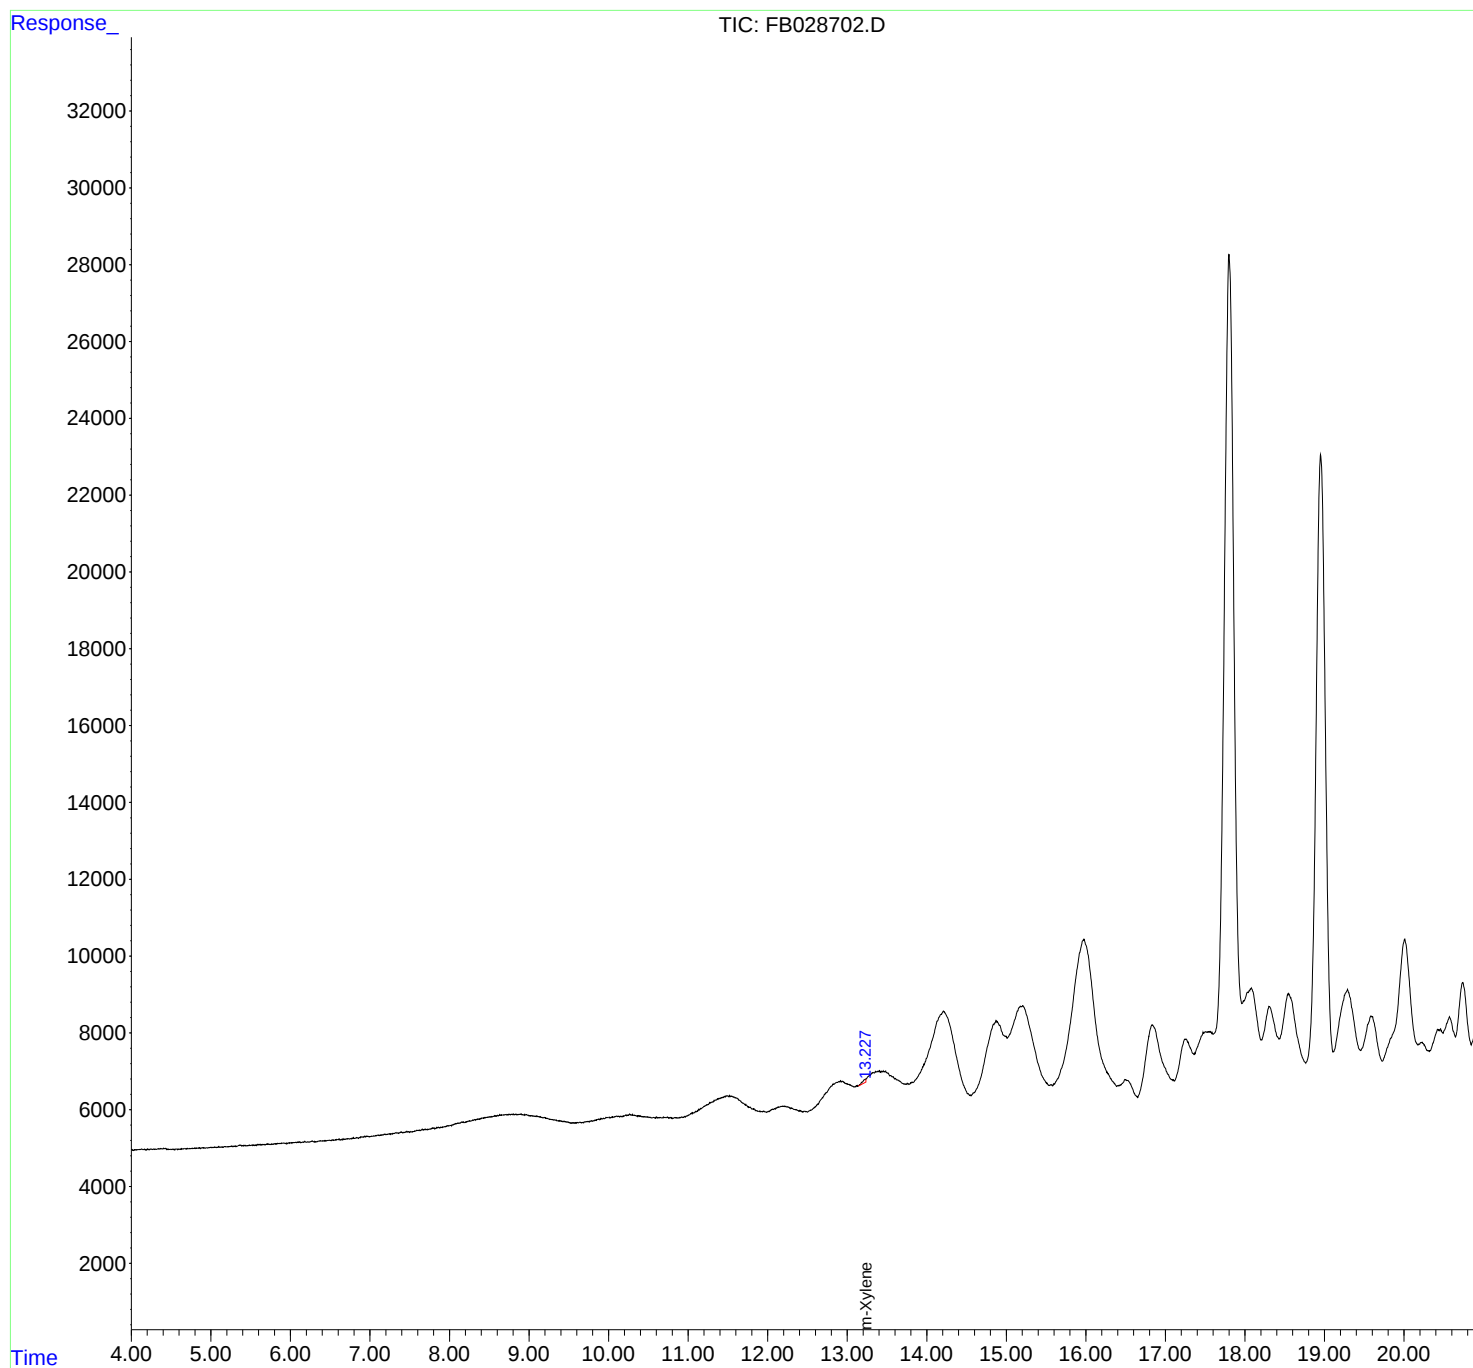


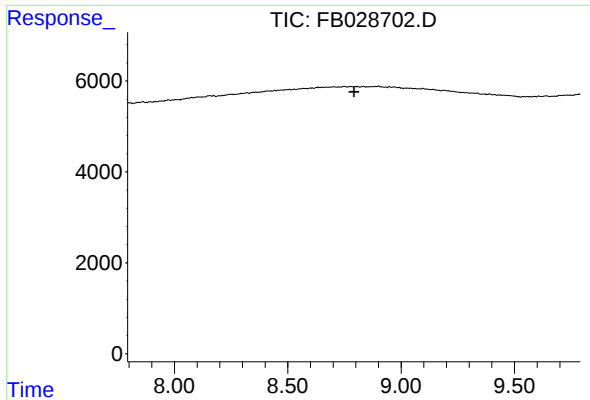

#5 AAA-TFT

R.T.: 0.000 min
Exp R.T.: 8.793 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :
SB-A1-COMP

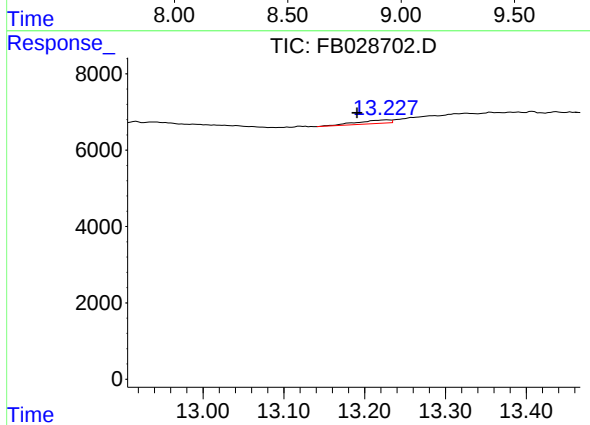

#8 m-Xylene

R.T.: 13.229 min
Delta R.T.: 0.038 min
Response: 2500
Conc: 0.13 ng/ml