

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
 Data File : FB028704.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2022 18:26
 Operator : AJ/MA
 Sample : BSF1024S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1024S2

Integration File: Calibration.e
 Quant Time: Oct 25 08:32:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	249579	19.292 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	441259	26.973 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	486592	26.925 ng/ml
3) t n-Heptane	7.753	153944	9.089 ng/ml
4) t Benzene	7.888	194652	8.862 ng/ml
6) t Toluene	10.622	555800	26.517 ng/ml
7) t Ethylbenzene	13.059	174063	8.771 ng/ml
8) t m-Xylene	13.191	344802	17.502 ng/ml
9) t O-Xylene	13.918	342153	17.587 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	333616	17.233 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102422\
Data File : FB028704.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2022 18:26
Operator : AJ/MA
Sample : BSF1024S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1024S2

Integration File: Calibration.e
Quant Time: Oct 25 08:32:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

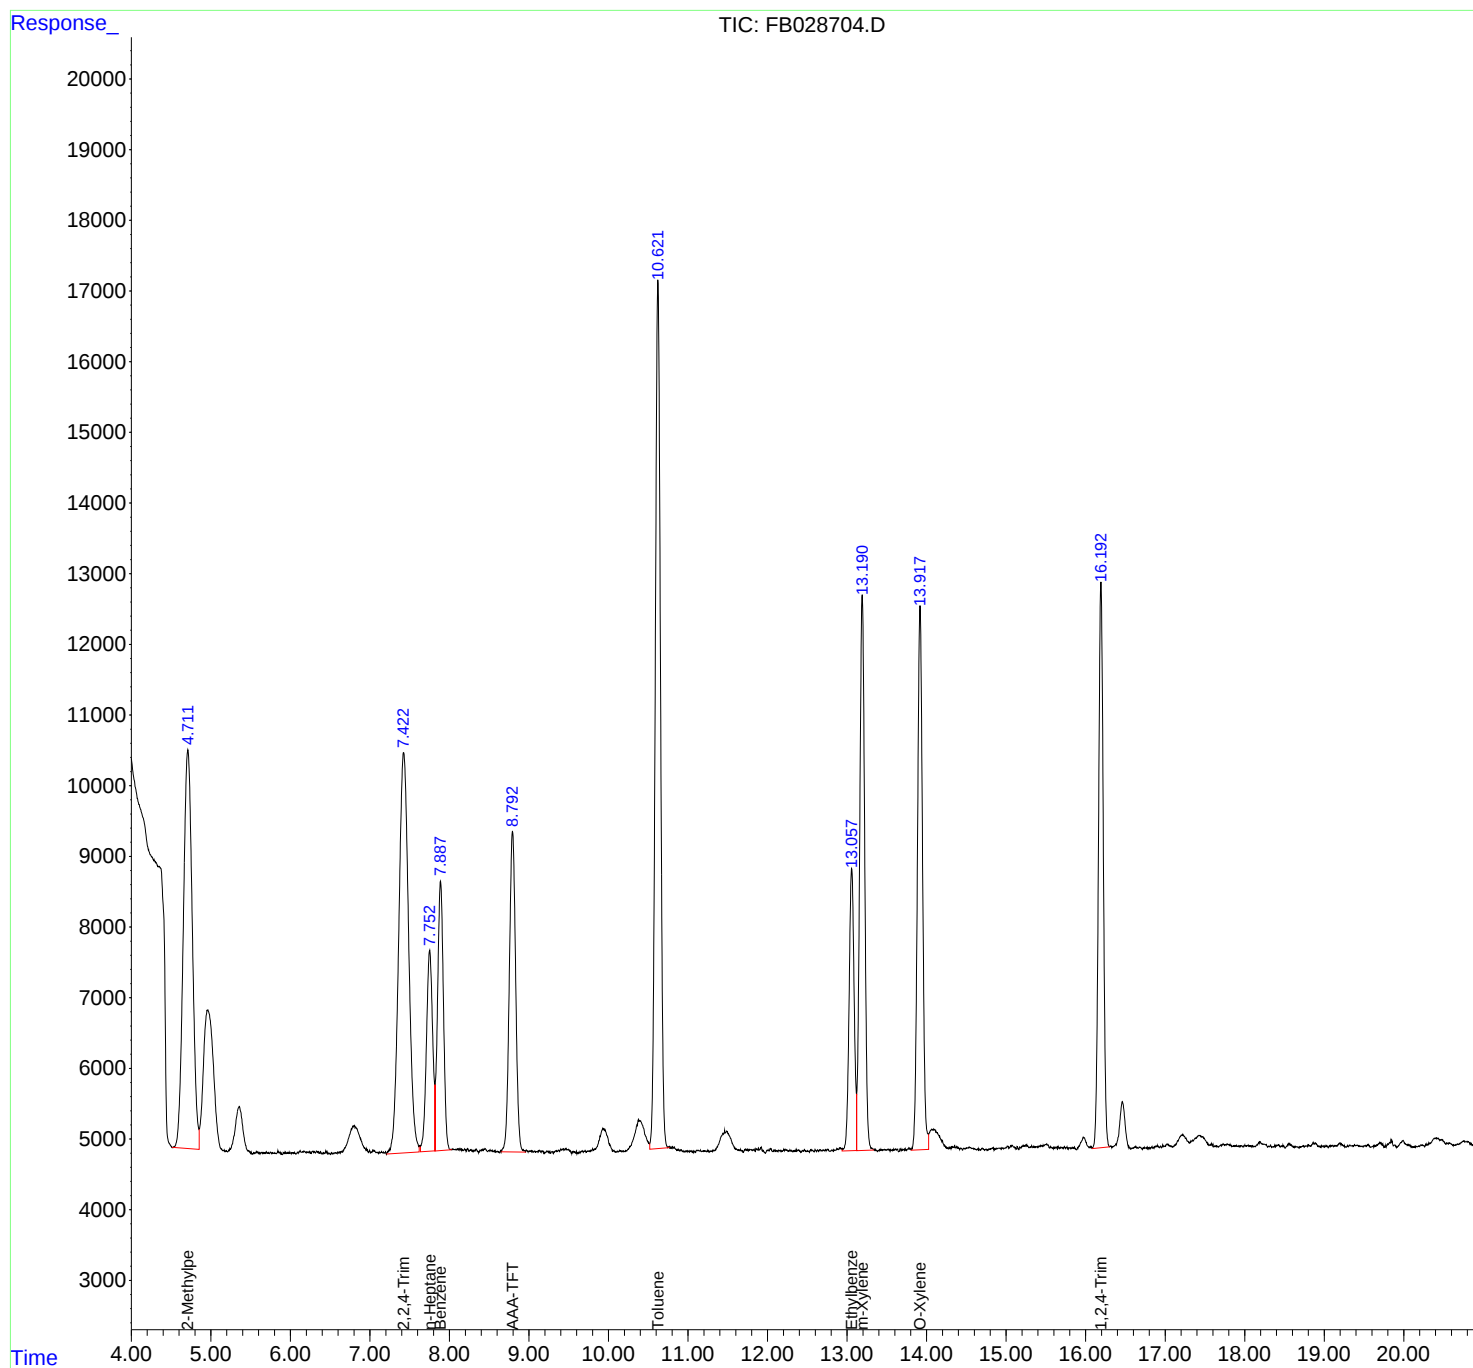


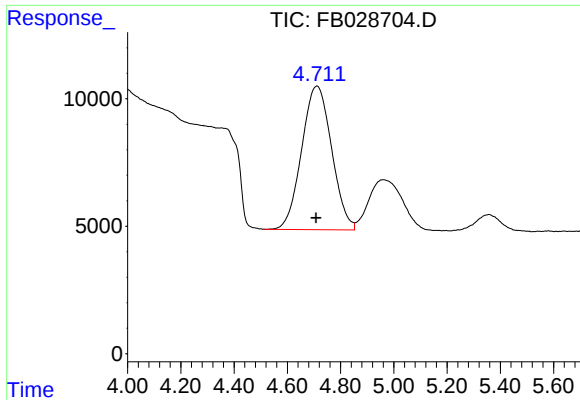

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.004 min
Response: 441259
Conc: 26.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S2

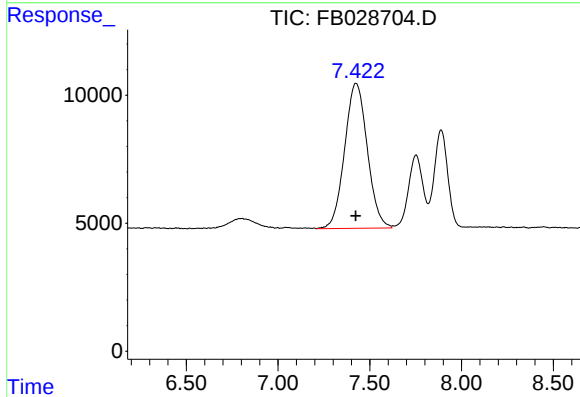


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 486592
Conc: 26.93 ng/ml

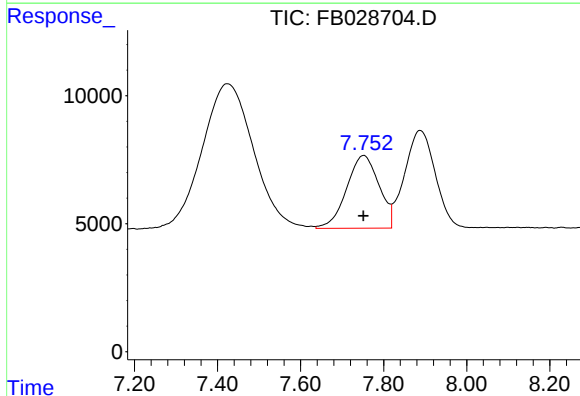


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 153944
Conc: 9.09 ng/ml

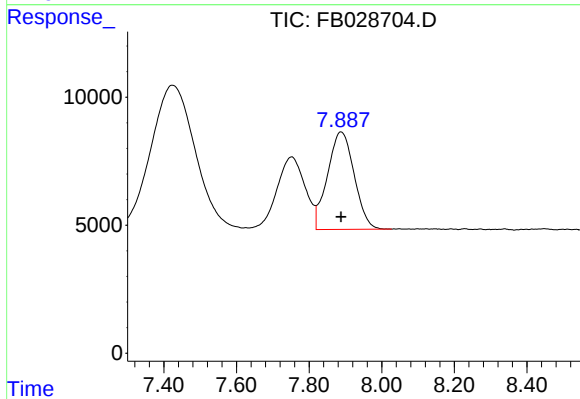

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 194652
Conc: 8.86 ng/ml

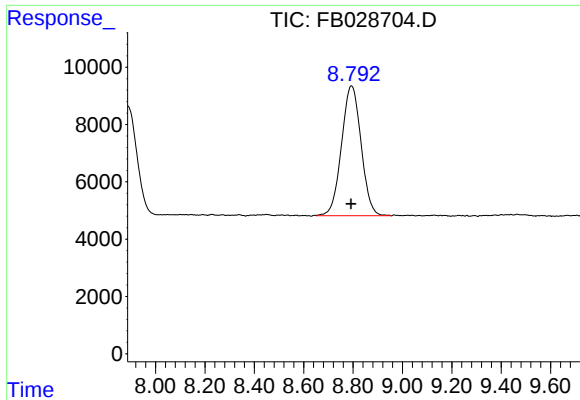

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.001 min
Response: 249579
Conc: 19.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S2

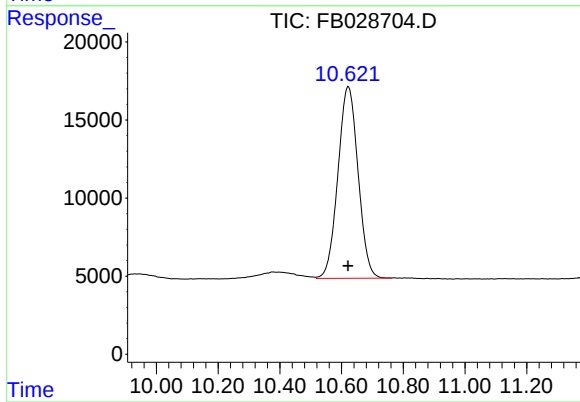


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 555800
Conc: 26.52 ng/ml

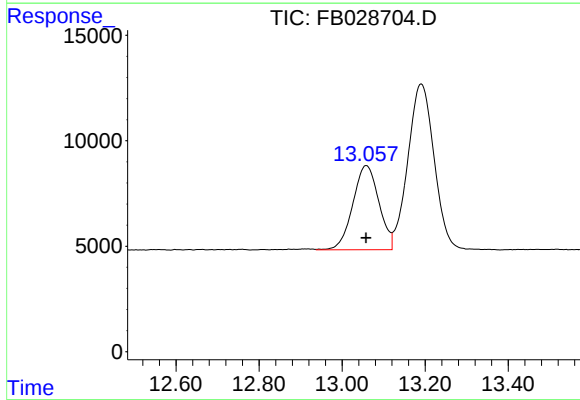


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.000 min
Response: 174063
Conc: 8.77 ng/ml

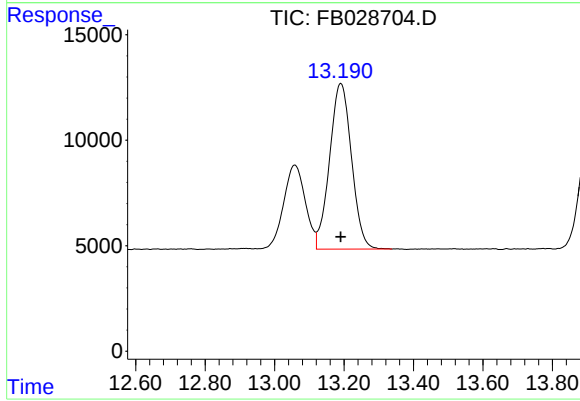

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 344802
Conc: 17.50 ng/ml

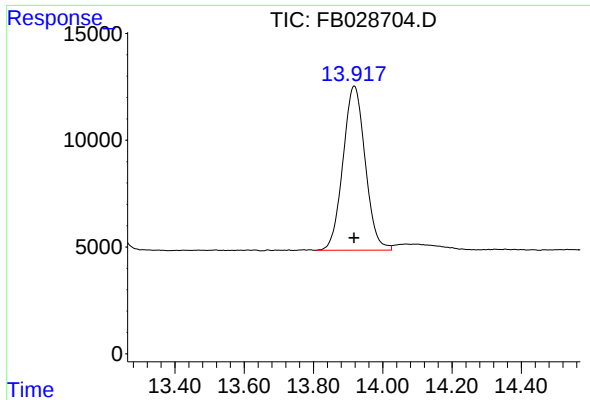

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 342153
Conc: 17.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S2

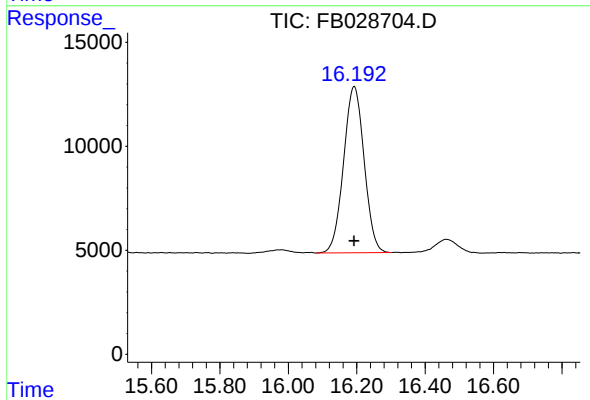

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 333616
Conc: 17.23 ng/ml