

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102422\  
Data File : FB028720.D  
Signal(s) : FID2B.CH  
Acq On : 25 Oct 2022 5:43  
Operator : AJ/MA  
Sample : N5217-08  
Misc : 5.08G/5.00 ML DI WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-D1-COMP

Integration File: Calibration.e  
Quant Time: Oct 25 08:34:07 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T. | Response | Conc Units |
|-----------------------------|------|----------|------------|
| -----                       |      |          |            |
| System Monitoring Compounds |      |          |            |
| Target Compounds            |      |          |            |
| -----                       |      |          |            |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102422\  
Data File : FB028720.D  
Signal(s) : FID2B.CH  
Acq On : 25 Oct 2022 5:43  
Operator : AJ/MA  
Sample : N5217-08  
Misc : 5.08G/5.00 ML DI WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-D1-COMP

Integration File: Calibration.e  
Quant Time: Oct 25 08:34:07 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100522.M  
Quant Title :  
QLast Update : Wed Oct 05 12:47:25 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

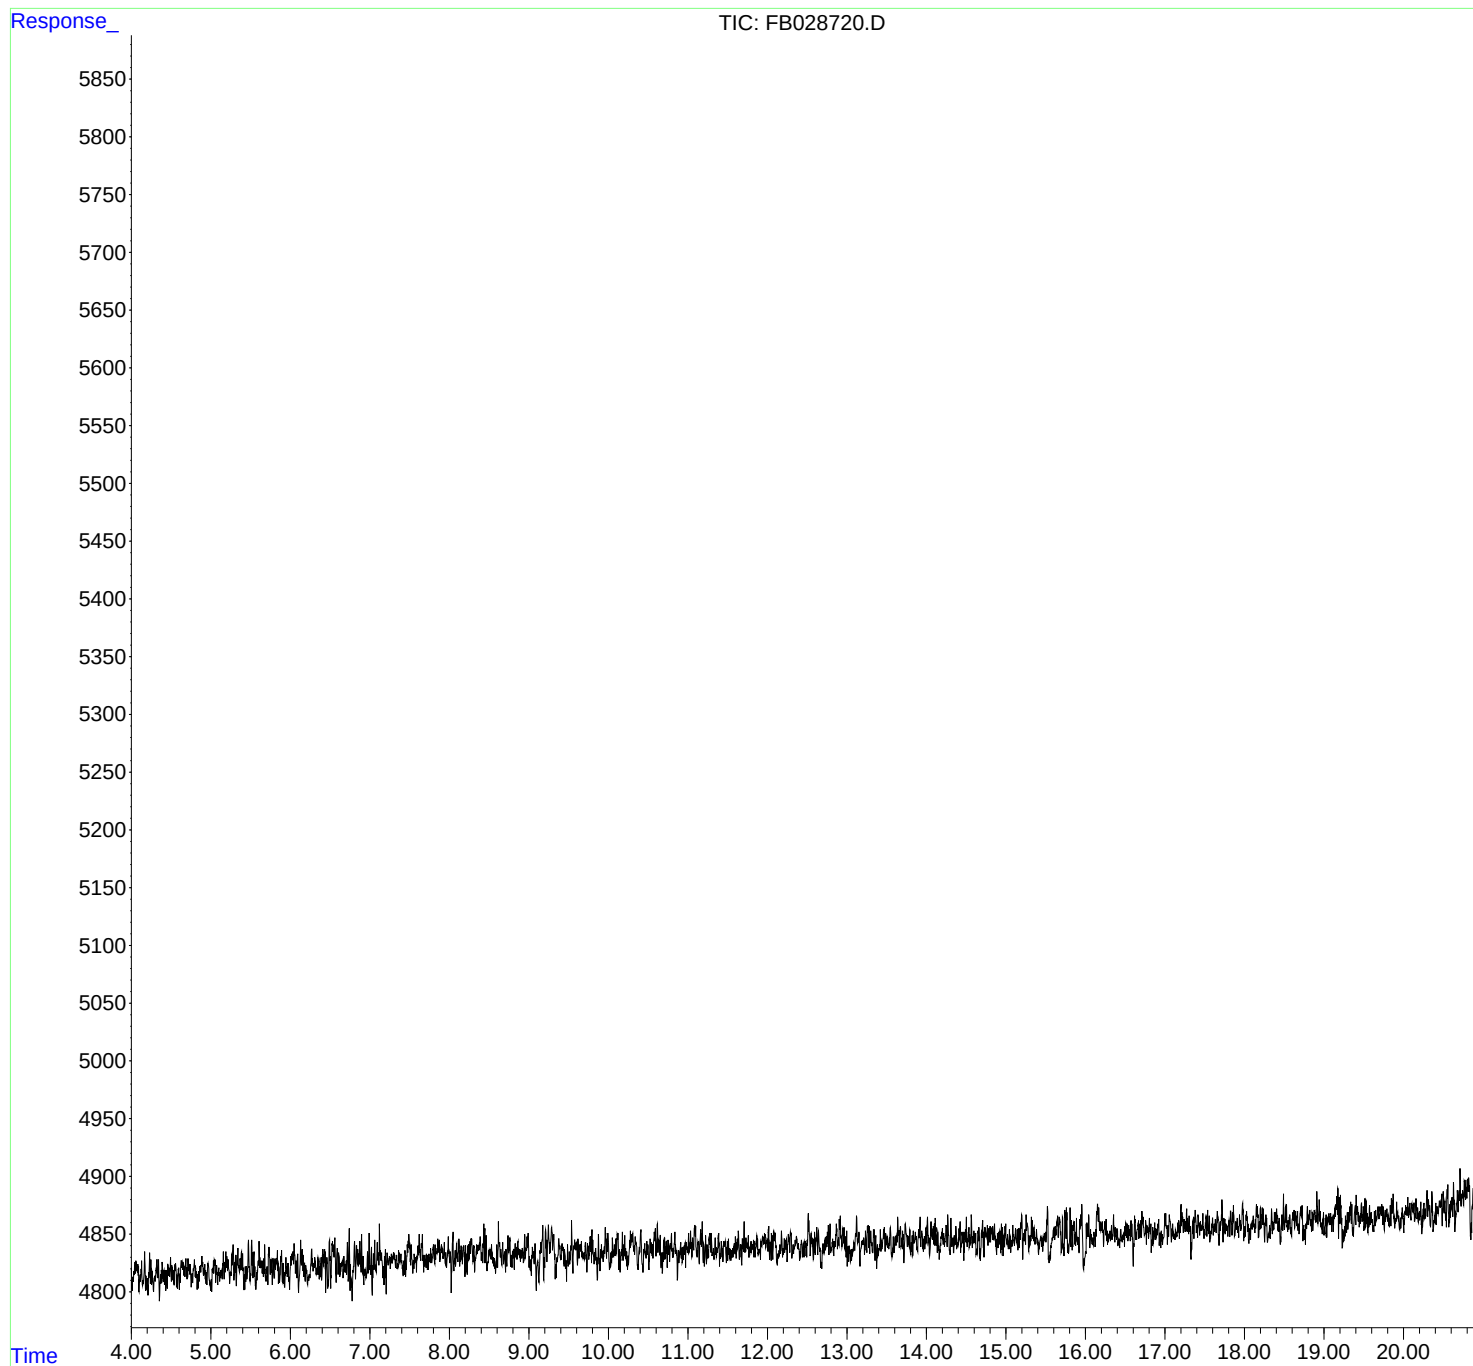

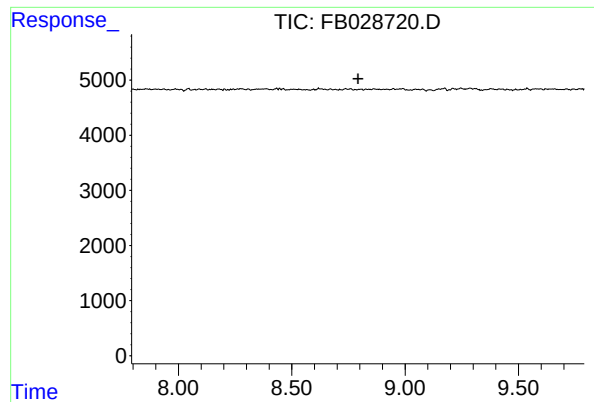

#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T.: 8.793 min  
Response: 0  
Conc: N.D.

Instrument :

FID\_B

ClientSampleId :

SB-D1-COMP