

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102423\
 Data File : FB030409.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2023 12:01
 Operator : YP/AJ
 Sample : BSF1024S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 25 01:07:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.782	184731	16.179 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	422258	30.180 ng/ml
2) t 2,2,4-Trimethylpentane	7.406	464327	28.123 ng/ml
3) t n-Heptane	7.742	154511	10.308 ng/ml
4) t Benzene	7.877	201981	9.845 ng/ml
6) t Toluene	10.609	604556	29.944 ng/ml
7) t Ethylbenzene	13.046	193565	9.697 ng/ml
8) t m-Xylene	13.178	380566	19.309 ng/ml
9) t O-Xylene	13.905	369372	18.767 ng/ml
10) t 1,2,4-Trimethylbenzene	16.180	364283	17.634 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102423\
Data File : FB030409.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2023 12:01
Operator : YP/AJ
Sample : BSF1024S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 01:07:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

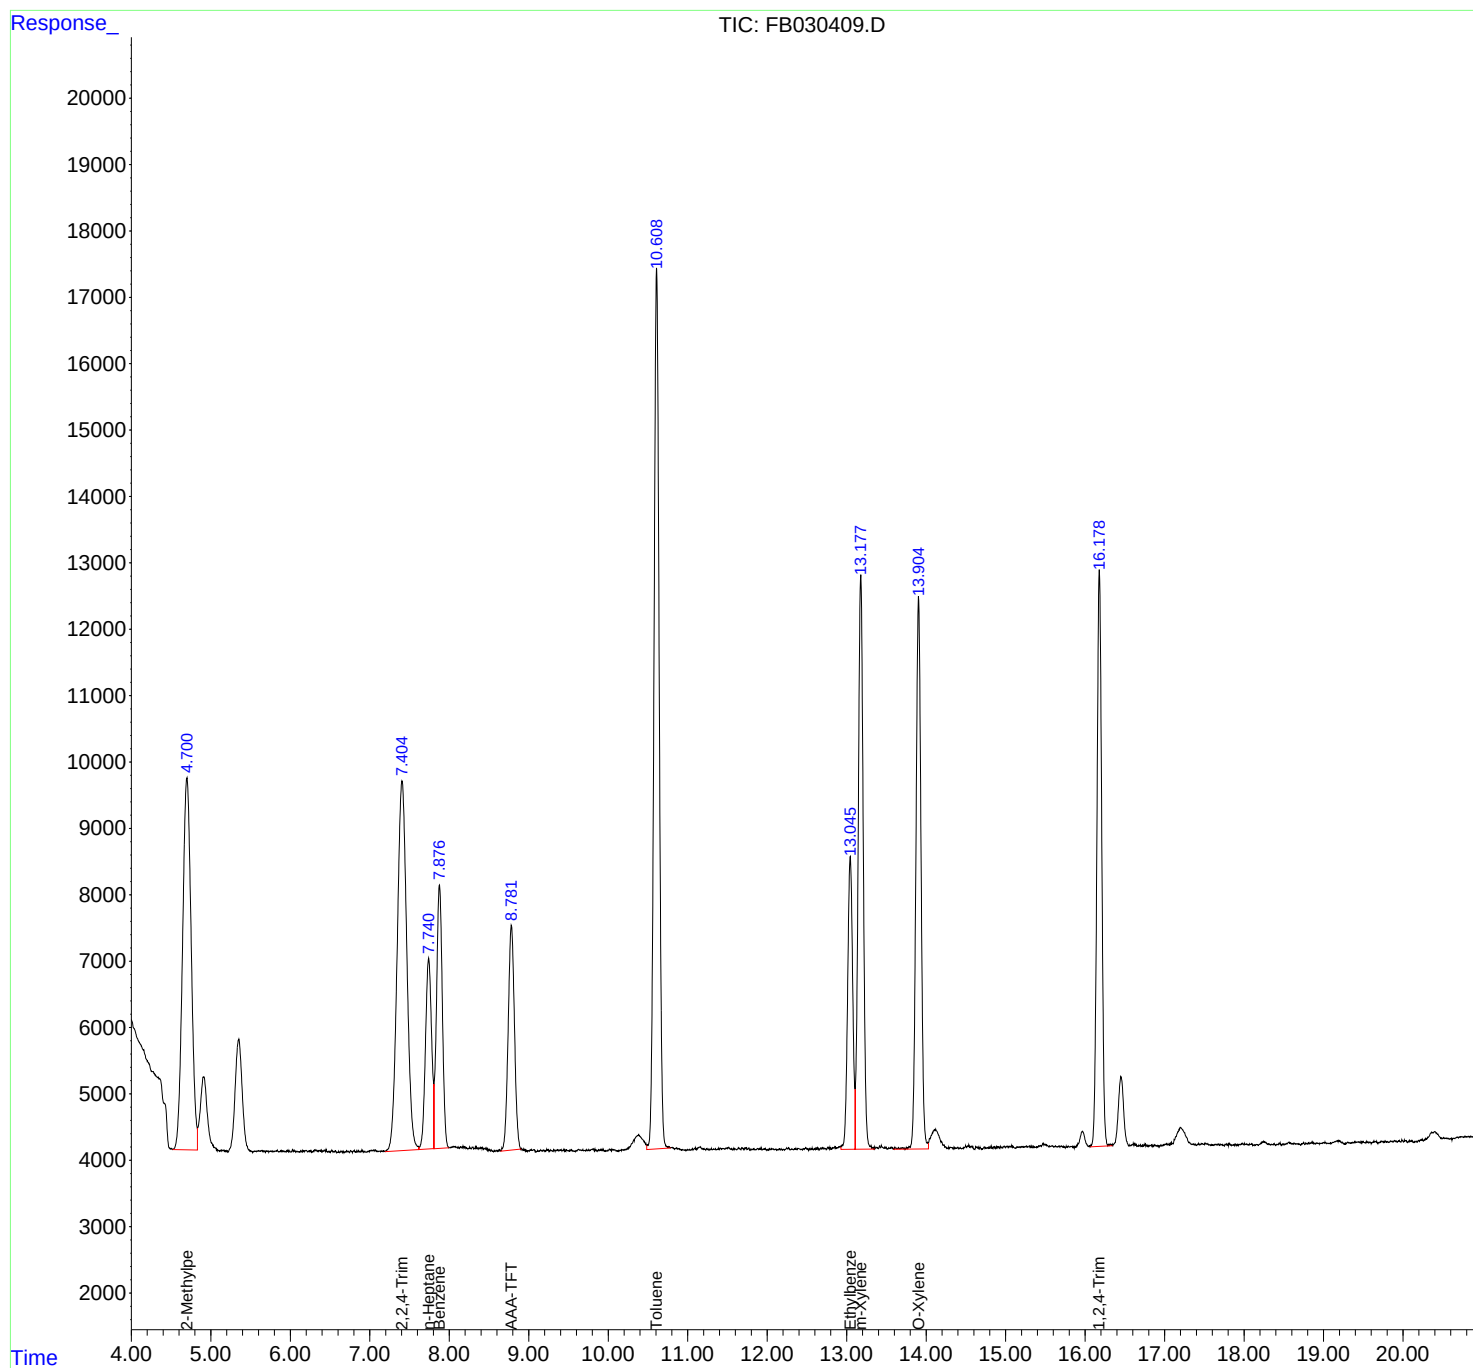

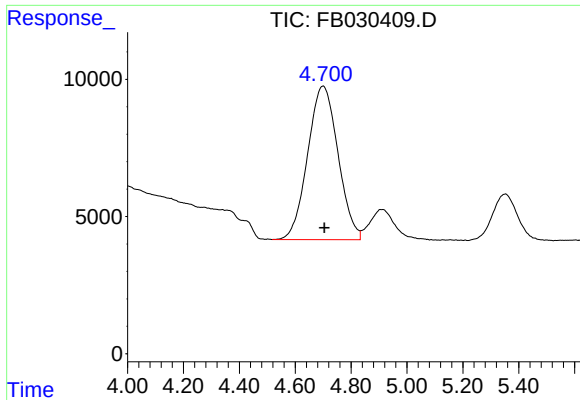


#1 2-Methylpentane

R.T.: 4.701 min
Delta R.T.: -0.003 min
Response: 422258
Conc: 30.18 ng/ml

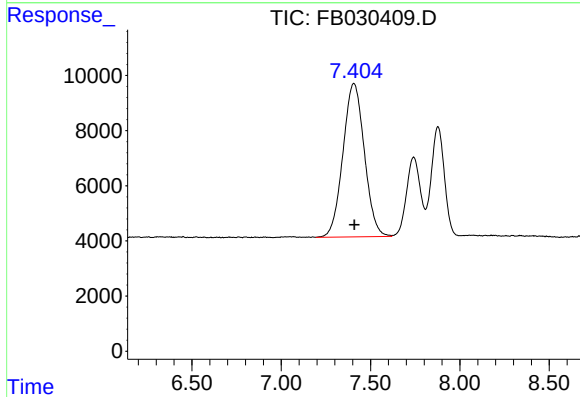


#2 2,2,4-Trimethylpentane

R.T.: 7.406 min
Delta R.T.: -0.003 min
Response: 464327
Conc: 28.12 ng/ml

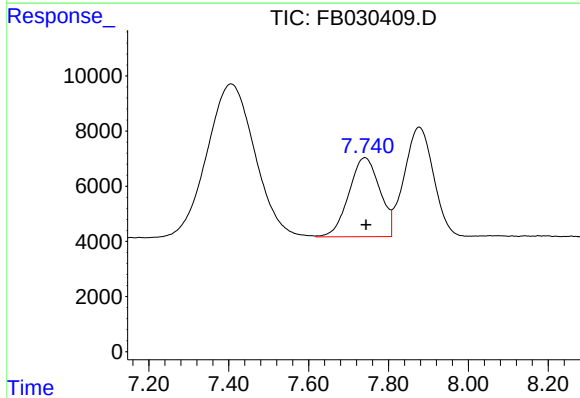


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: -0.002 min
Response: 154511
Conc: 10.31 ng/ml

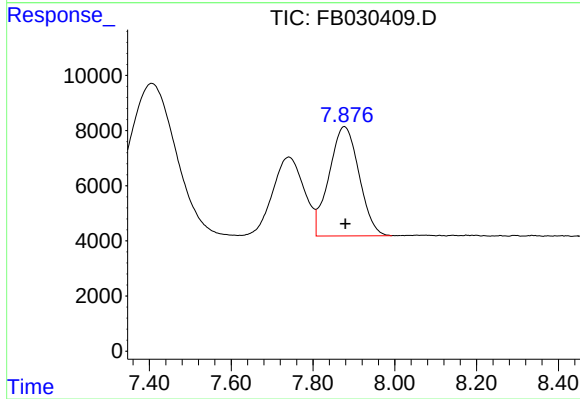


#4 Benzene

R.T.: 7.877 min
Delta R.T.: -0.002 min
Response: 201981
Conc: 9.84 ng/ml

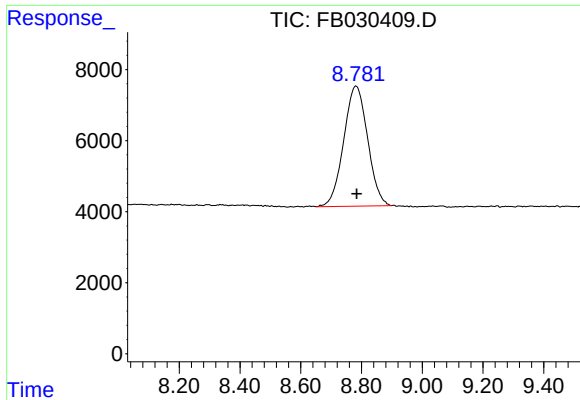


#5 AAA-TFT

R.T.: 8.782 min
 Delta R.T.: -0.002 min
 Response: 184731
 Conc: 16.18 ng/ml

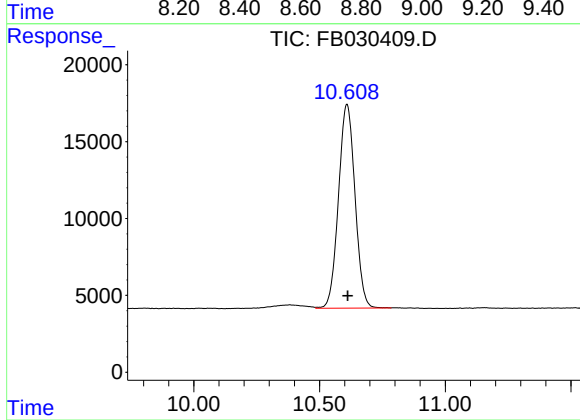


#6 Toluene

R.T.: 10.609 min
 Delta R.T.: -0.003 min
 Response: 604556
 Conc: 29.94 ng/ml

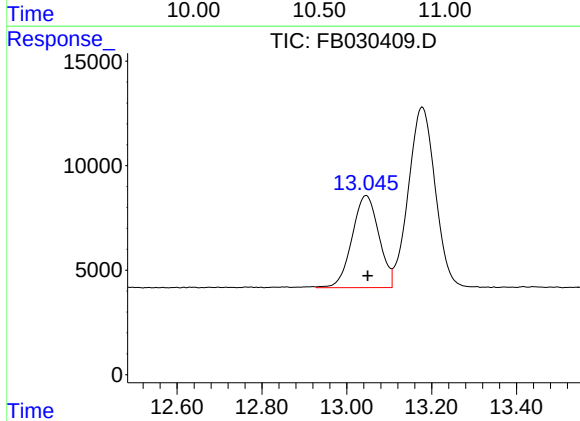


#7 Ethylbenzene

R.T.: 13.046 min
 Delta R.T.: -0.003 min
 Response: 193565
 Conc: 9.70 ng/ml

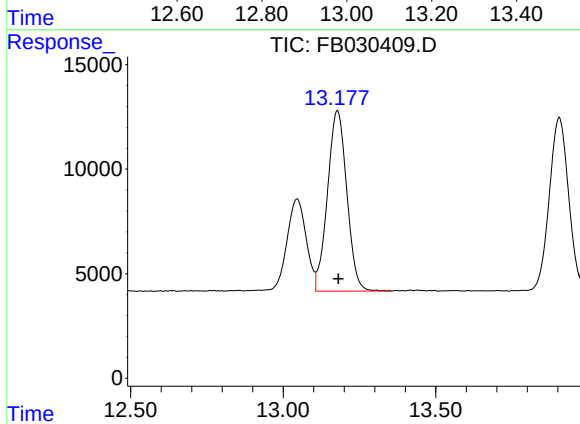


#8 m-Xylene

R.T.: 13.178 min
 Delta R.T.: -0.003 min
 Response: 380566
 Conc: 19.31 ng/ml

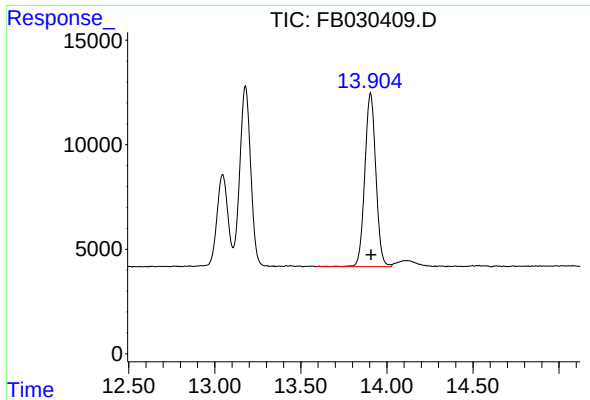

#9 O-Xylene

R.T.: 13.905 min
Delta R.T.: -0.003 min
Response: 369372
Conc: 18.77 ng/ml

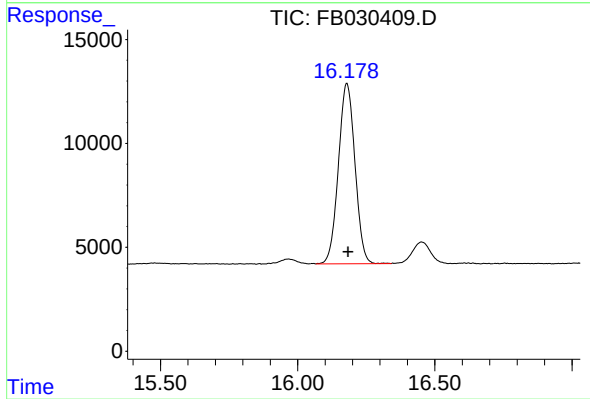

#10 1,2,4-Trimethylbenzene

R.T.: 16.180 min
Delta R.T.: -0.004 min
Response: 364283
Conc: 17.63 ng/ml