

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102423\
 Data File : FB030415.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2023 15:51
 Operator : YP/AJ
 Sample : BSF1024S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 25 01:09:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
 Quant Title :
 QLast Update : Tue Oct 10 11:38:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.787	177775	15.570 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.706	415070	29.666 ng/ml
2) t	2,2,4-Trimethylpentane	7.412	484144	29.323 ng/ml
3) t	n-Heptane	7.746	151818	10.129 ng/ml
4) t	Benzene	7.882	203495	9.918 ng/ml
6) t	Toluene	10.614	601364	29.786 ng/ml
7) t	Ethylbenzene	13.050	189904	9.514 ng/ml
8) t	m-Xylene	13.183	374388	18.995 ng/ml
9) t	O-Xylene	13.909	368197	18.708 ng/ml
10) t	1,2,4-Trimethylbenzene	16.184	367672	17.798 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102423\
Data File : FB030415.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2023 15:51
Operator : YP/AJ
Sample : BSF1024S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 01:09:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101023.M
Quant Title :
QLast Update : Tue Oct 10 11:38:40 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

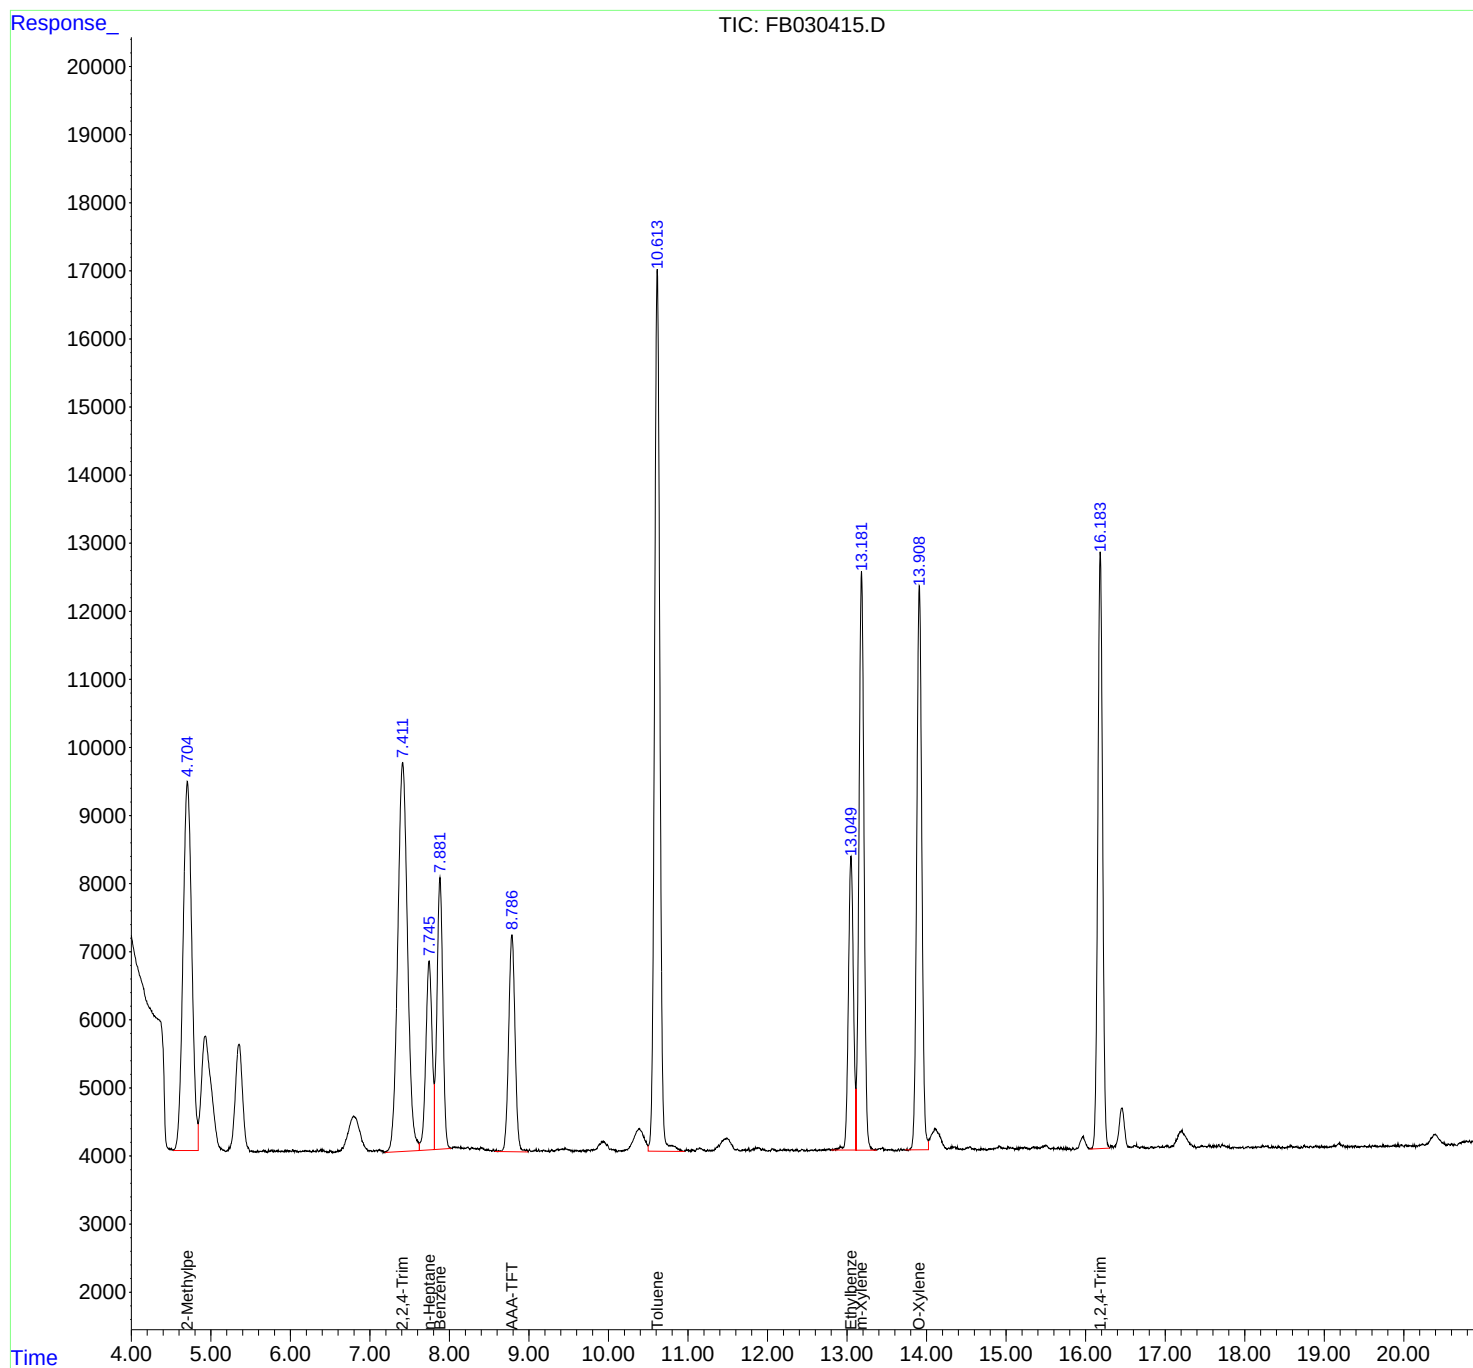

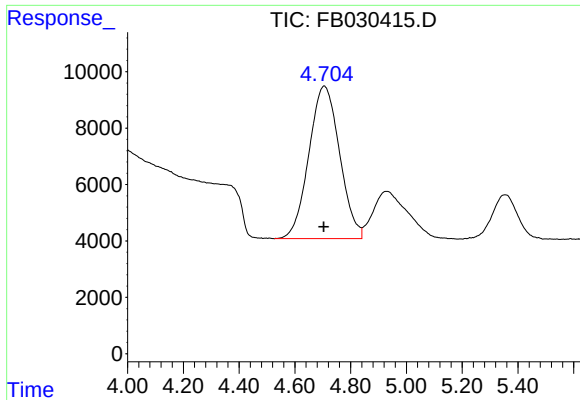


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: 0.002 min
Response: 415070
Conc: 29.67 ng/ml

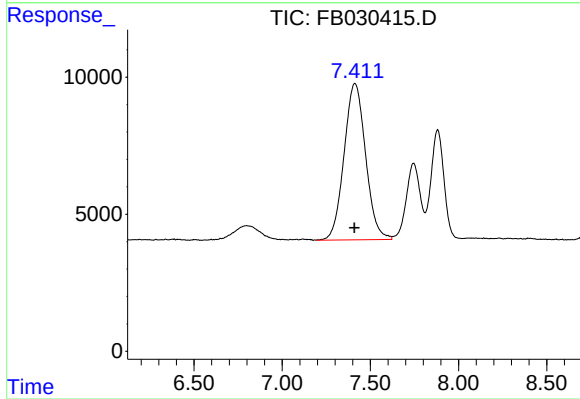


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.003 min
Response: 484144
Conc: 29.32 ng/ml

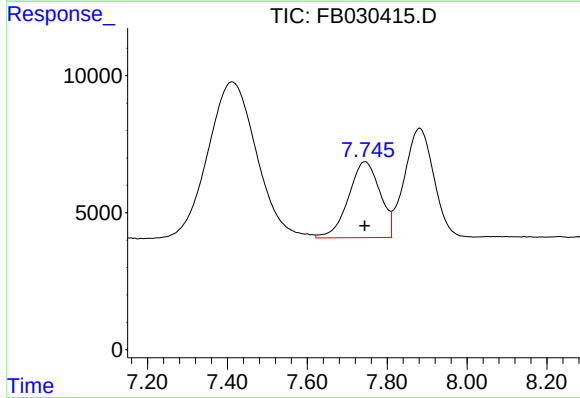


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: 0.002 min
Response: 151818
Conc: 10.13 ng/ml

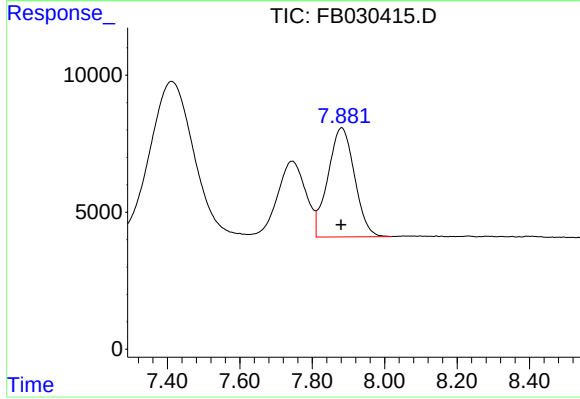


#4 Benzene

R.T.: 7.882 min
Delta R.T.: 0.002 min
Response: 203495
Conc: 9.92 ng/ml

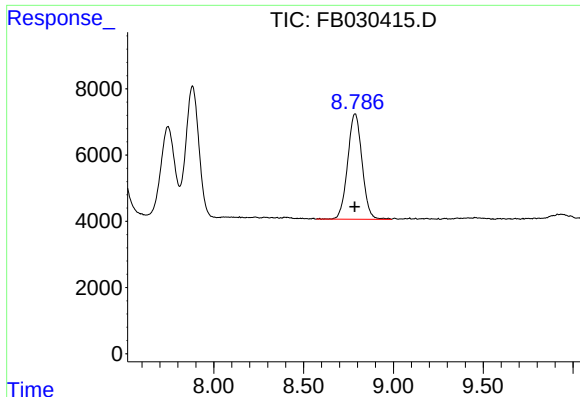


#5 AAA-TFT

R.T.: 8.787 min
Delta R.T.: 0.002 min
Response: 177775
Conc: 15.57 ng/ml

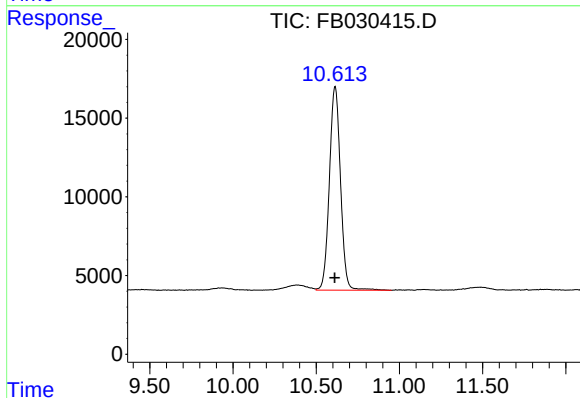


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.001 min
Response: 601364
Conc: 29.79 ng/ml

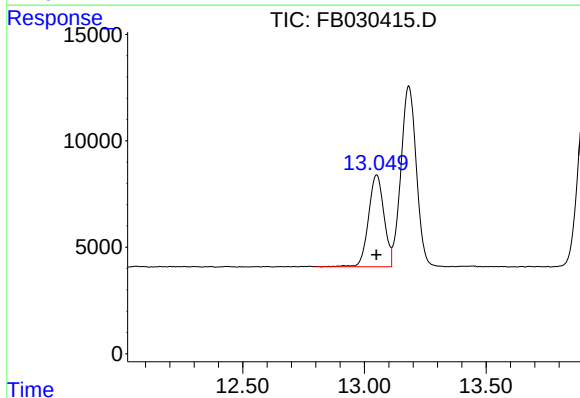


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: 0.000 min
Response: 189904
Conc: 9.51 ng/ml

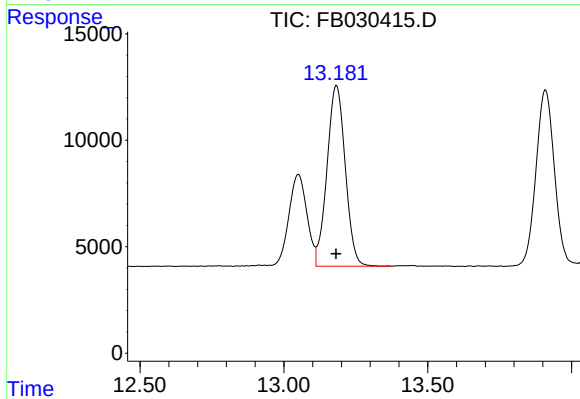


#8 m-Xylene

R.T.: 13.183 min
Delta R.T.: 0.000 min
Response: 374388
Conc: 19.00 ng/ml

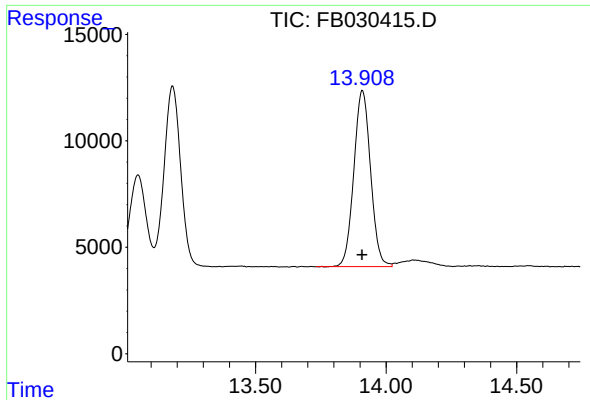

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: 0.001 min
Response: 368197
Conc: 18.71 ng/ml

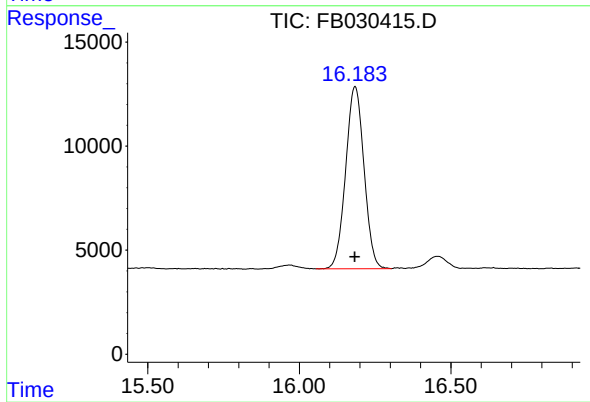

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: 0.001 min
Response: 367672
Conc: 17.80 ng/ml