

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102424\  
 Data File : FB031012.D  
 Signal(s) : FID2B.CH  
 Acq On : 24 Oct 2024 9:33  
 Operator : YP/AJ  
 Sample : VBF1024S1  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Oct 25 04:01:32 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100424.M  
 Quant Title :  
 QLast Update : Fri Oct 04 11:53:51 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.793  | 557254   | 18.589 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.612 | 340      | 0.006 ng/ml  |
| 8) t m-Xylene                | 13.185 | 948      | 0.018 ng/ml  |
| 9) t O-Xylene                | 13.911 | 3839     | 0.079 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.196 | 10791    | 0.329 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102424\  
Data File : FB031012.D  
Signal(s) : FID2B.CH  
Acq On : 24 Oct 2024 9:33  
Operator : YP/AJ  
Sample : VBF1024S1  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 25 04:01:32 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB100424.M  
Quant Title :  
QLast Update : Fri Oct 04 11:53:51 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

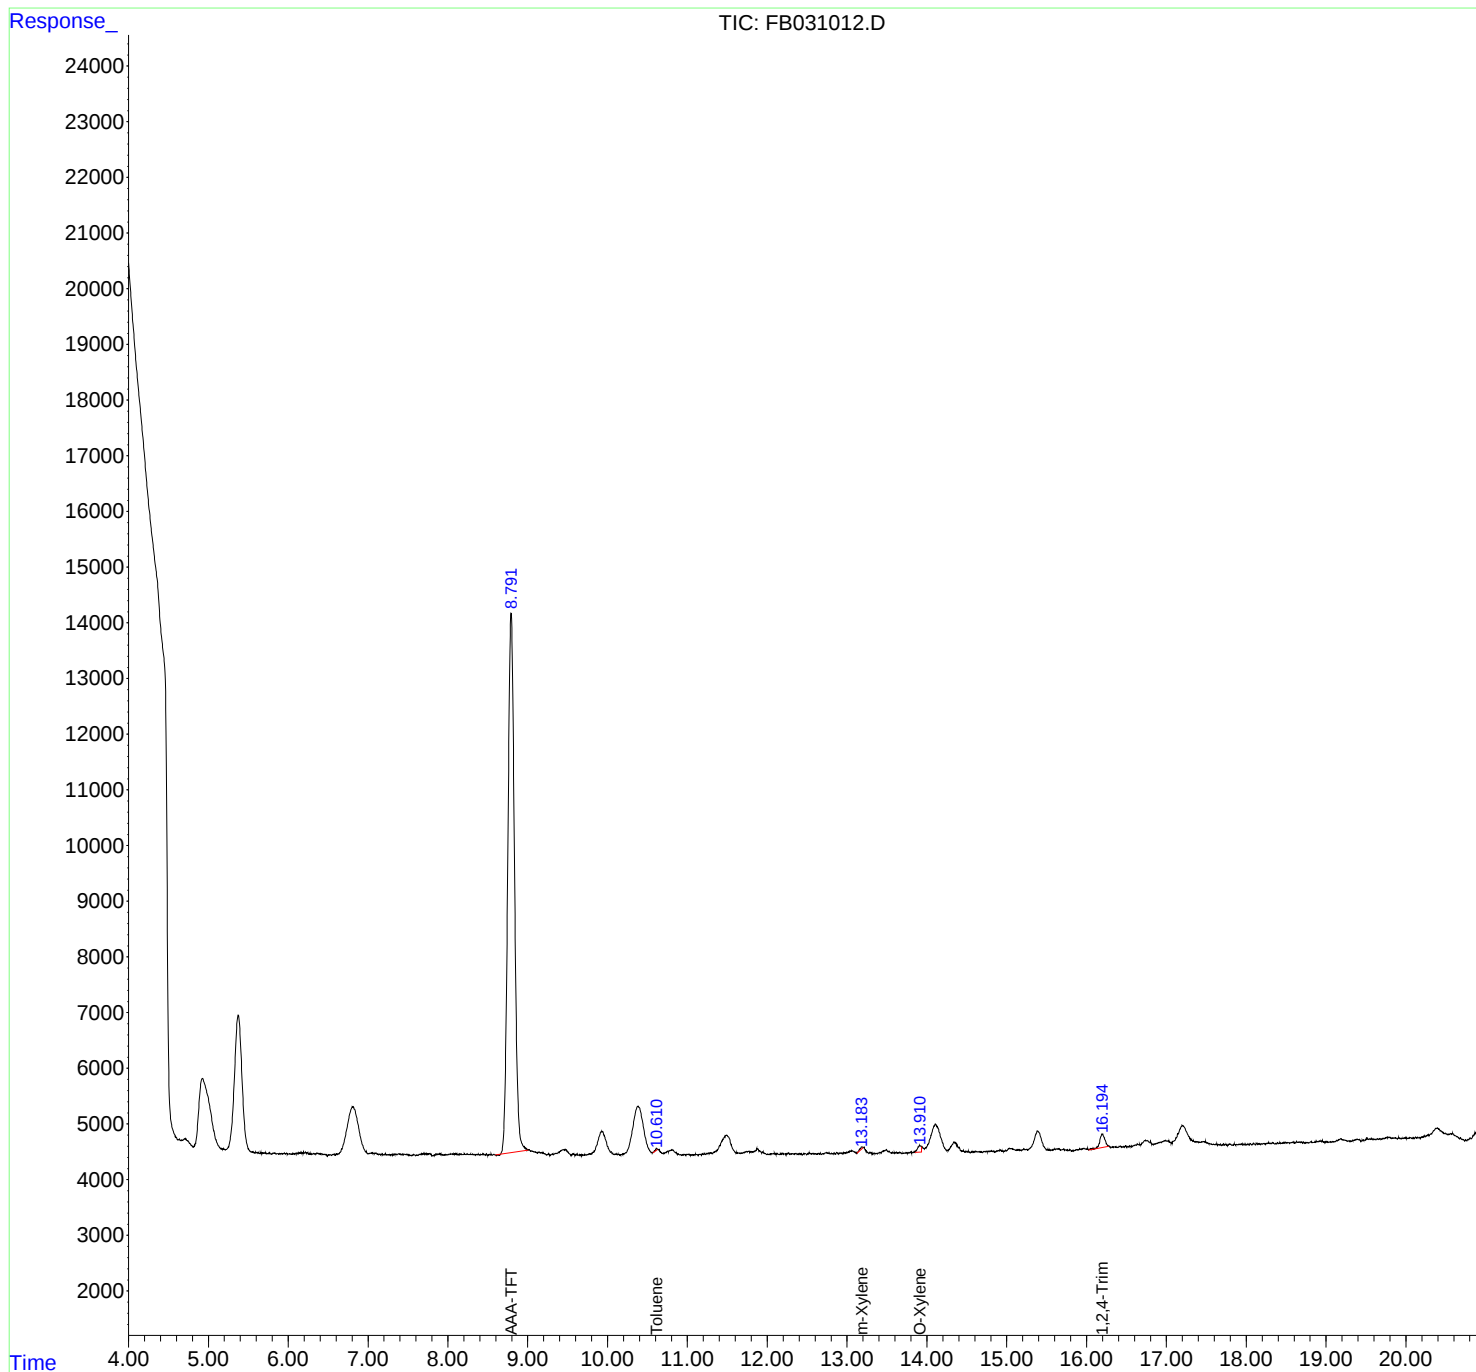


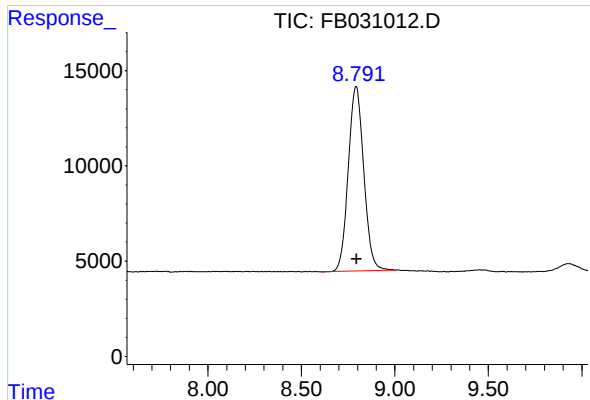

#5 AAA-TFT


R.T.: 8.793 min  
Delta R.T.: -0.003 min  
Response: 557254  
Conc: 18.59 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

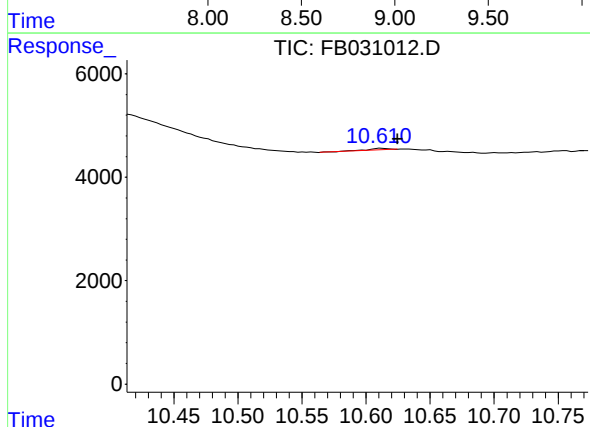


#6 Toluene

R.T.: 10.612 min  
Delta R.T.: -0.012 min  
Response: 340  
Conc: 0.01 ng/ml

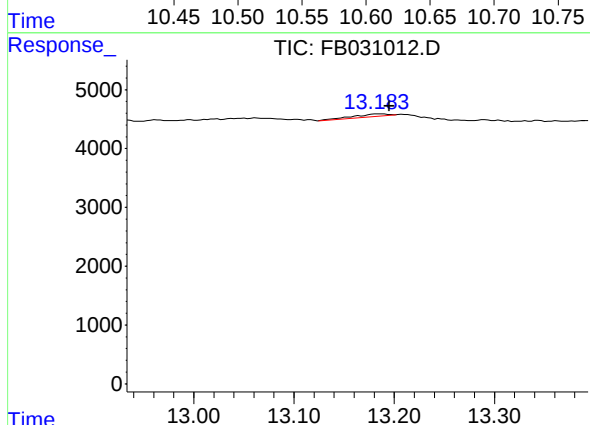


#8 m-Xylene

R.T.: 13.185 min  
Delta R.T.: -0.010 min  
Response: 948  
Conc: 0.02 ng/ml

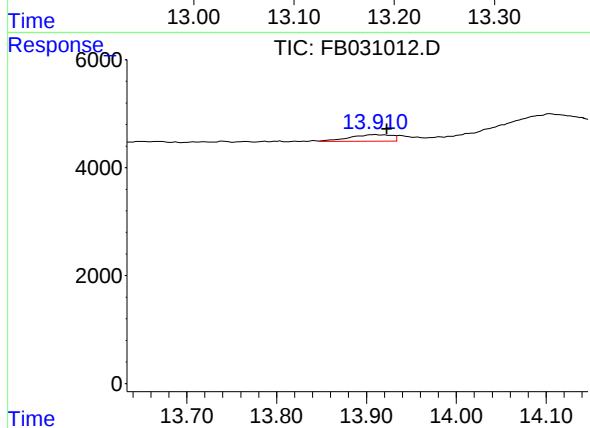

#9 O-Xylene

R.T.: 13.911 min  
Delta R.T.: -0.012 min  
Response: 3839  
Conc: 0.08 ng/ml

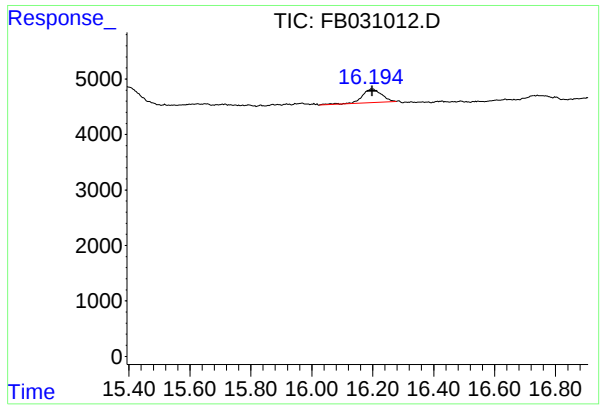

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min

Delta R.T.: -0.003 min

Response: 10791

Conc: 0.33 ng/ml

Instrument :

FID\_B

ClientSampleId :