

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031016.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 11:20
 Operator : YP/AJ
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 25 04:01:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	923248	30.798 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.726	24985	0.692 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	383104	8.039 ng/ml
3) t n-Heptane	7.760	296611	6.576 ng/ml
4) t Benzene	7.898	203111	3.695 ng/ml
6) t Toluene	10.627	7566341	140.066 ng/ml
7) t Ethylbenzene	13.063	2924384	61.696 ng/ml
8) t m-Xylene	13.196	11677330	223.839 ng/ml
9) t O-Xylene	13.926	5376730	110.530 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	19780862	603.662 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031016.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 11:20
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:01:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

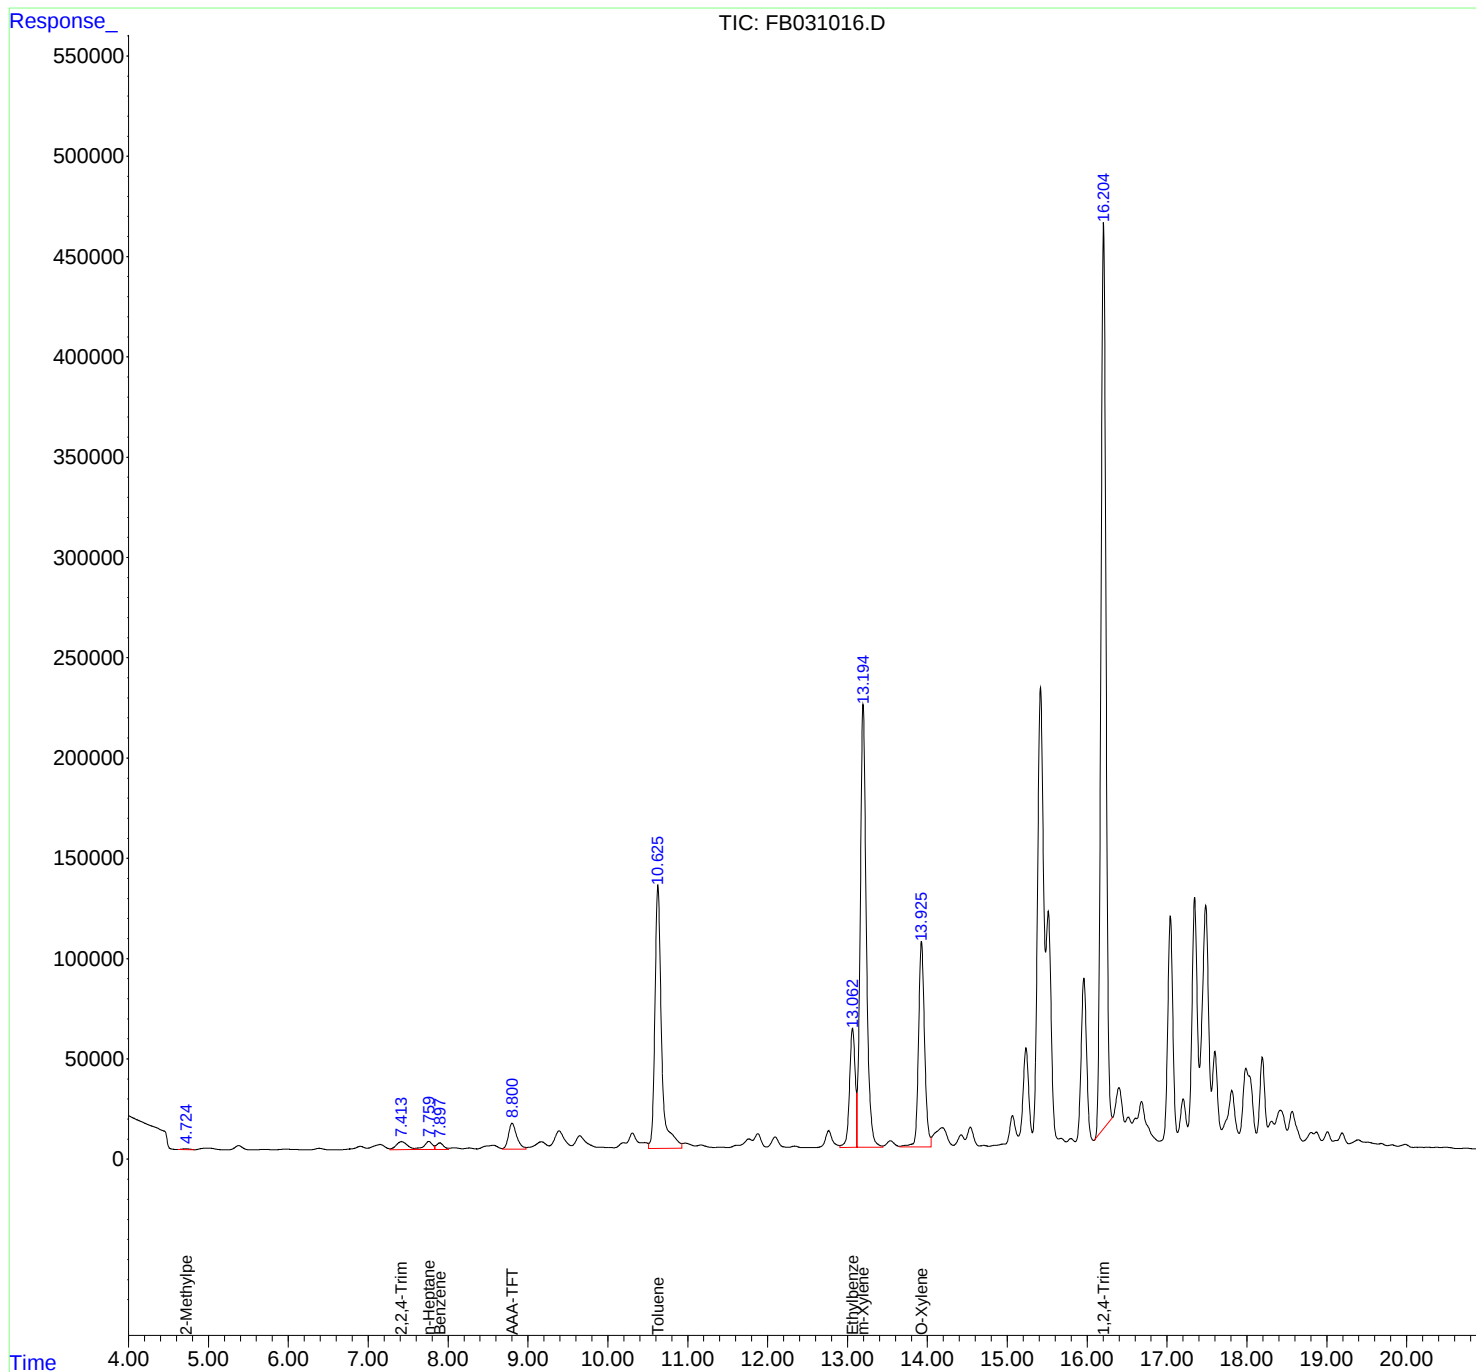

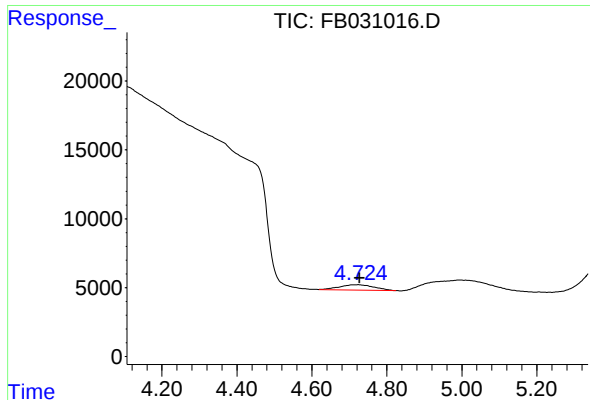


#1 2-Methylpentane

R.T.: 4.726 min
Delta R.T.: -0.002 min
Response: 24985
Conc: 0.69 ng/ml


Instrument : FID_B

ClientSampleId :

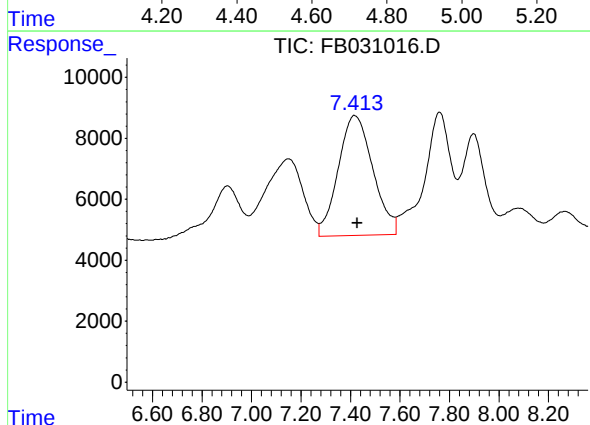


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.013 min
Response: 383104
Conc: 8.04 ng/ml

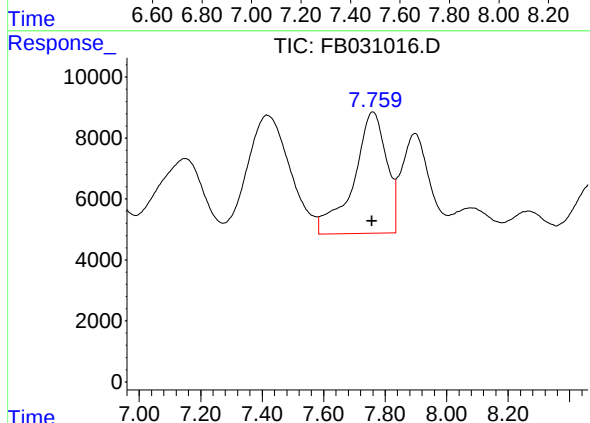


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.003 min
Response: 296611
Conc: 6.58 ng/ml

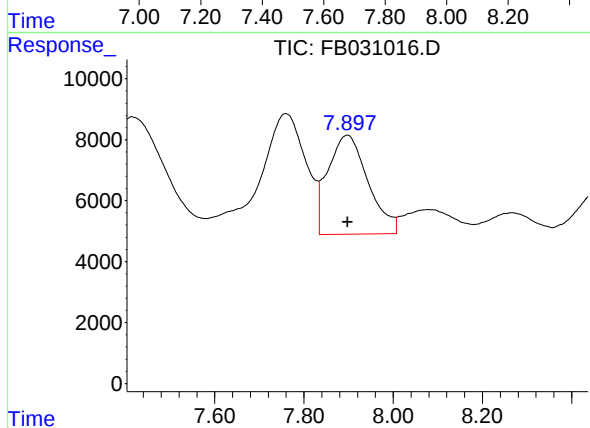

#4 Benzene


R.T.: 7.898 min
Delta R.T.: 0.000 min
Response: 203111
Conc: 3.70 ng/ml

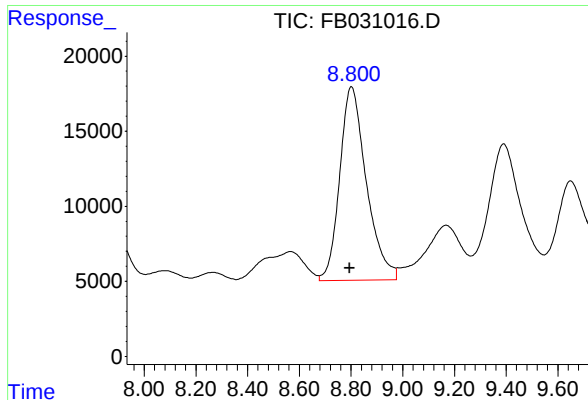

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.006 min
Response: 923248
Conc: 30.80 ng/ml

Instrument :
FID_B
ClientSampleId :

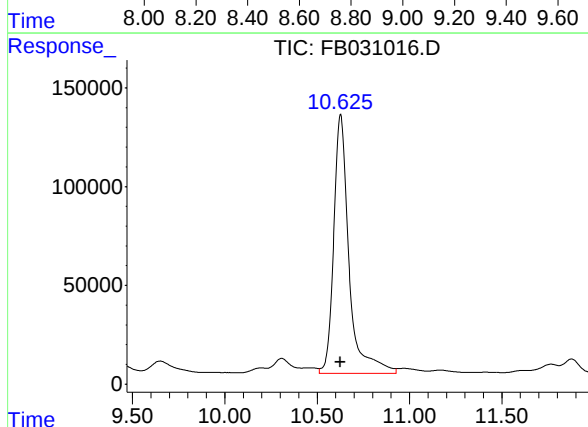


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.002 min
Response: 7566341
Conc: 140.07 ng/ml

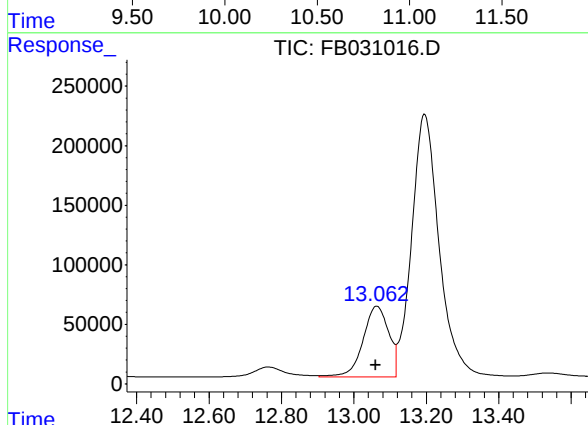


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.003 min
Response: 2924384
Conc: 61.70 ng/ml

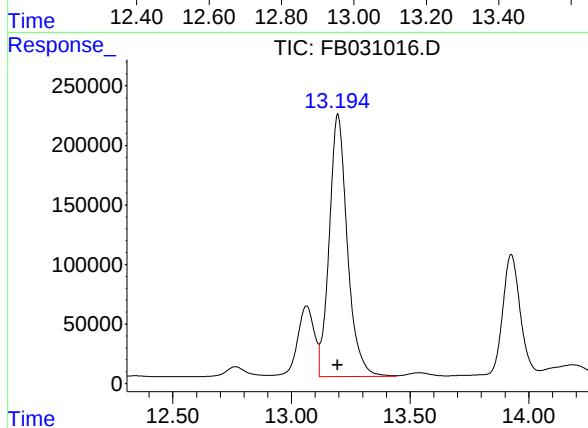

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.000 min
Response: 11677330
Conc: 223.84 ng/ml

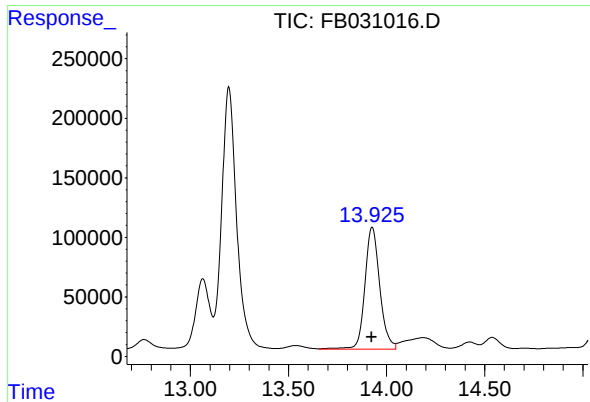

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.004 min
Response: 5376730
Conc: 110.53 ng/ml

Instrument :
FID_B
ClientSampleId :

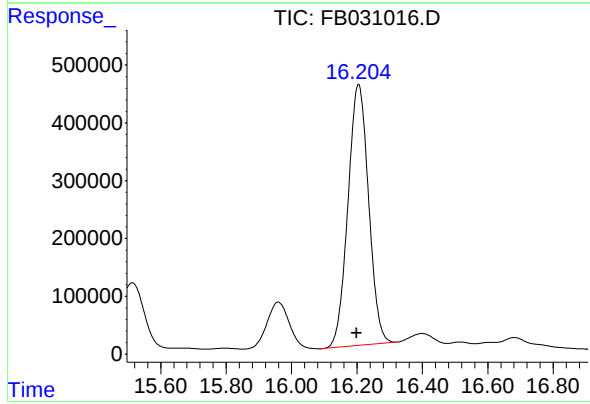

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.007 min
Response: 19780862
Conc: 603.66 ng/ml