

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031018.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 12:26
 Operator : YP/AJ
 Sample : I.BLK
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 25 04:02:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	647499	21.599 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.416	66218	1.390 ng/ml
3) t n-Heptane	7.754	37253	0.826 ng/ml
4) t Benzene	7.891	25781	0.469 ng/ml
6) t Toluene	10.624	1173676	21.727 ng/ml
7) t Ethylbenzene	13.060	464275	9.795 ng/ml
8) t m-Xylene	13.192	1849582	35.454 ng/ml
9) t O-Xylene	13.922	896996	18.440 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	3093317	94.400 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031018.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 12:26
Operator : YP/AJ
Sample : I.BLK
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:02:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

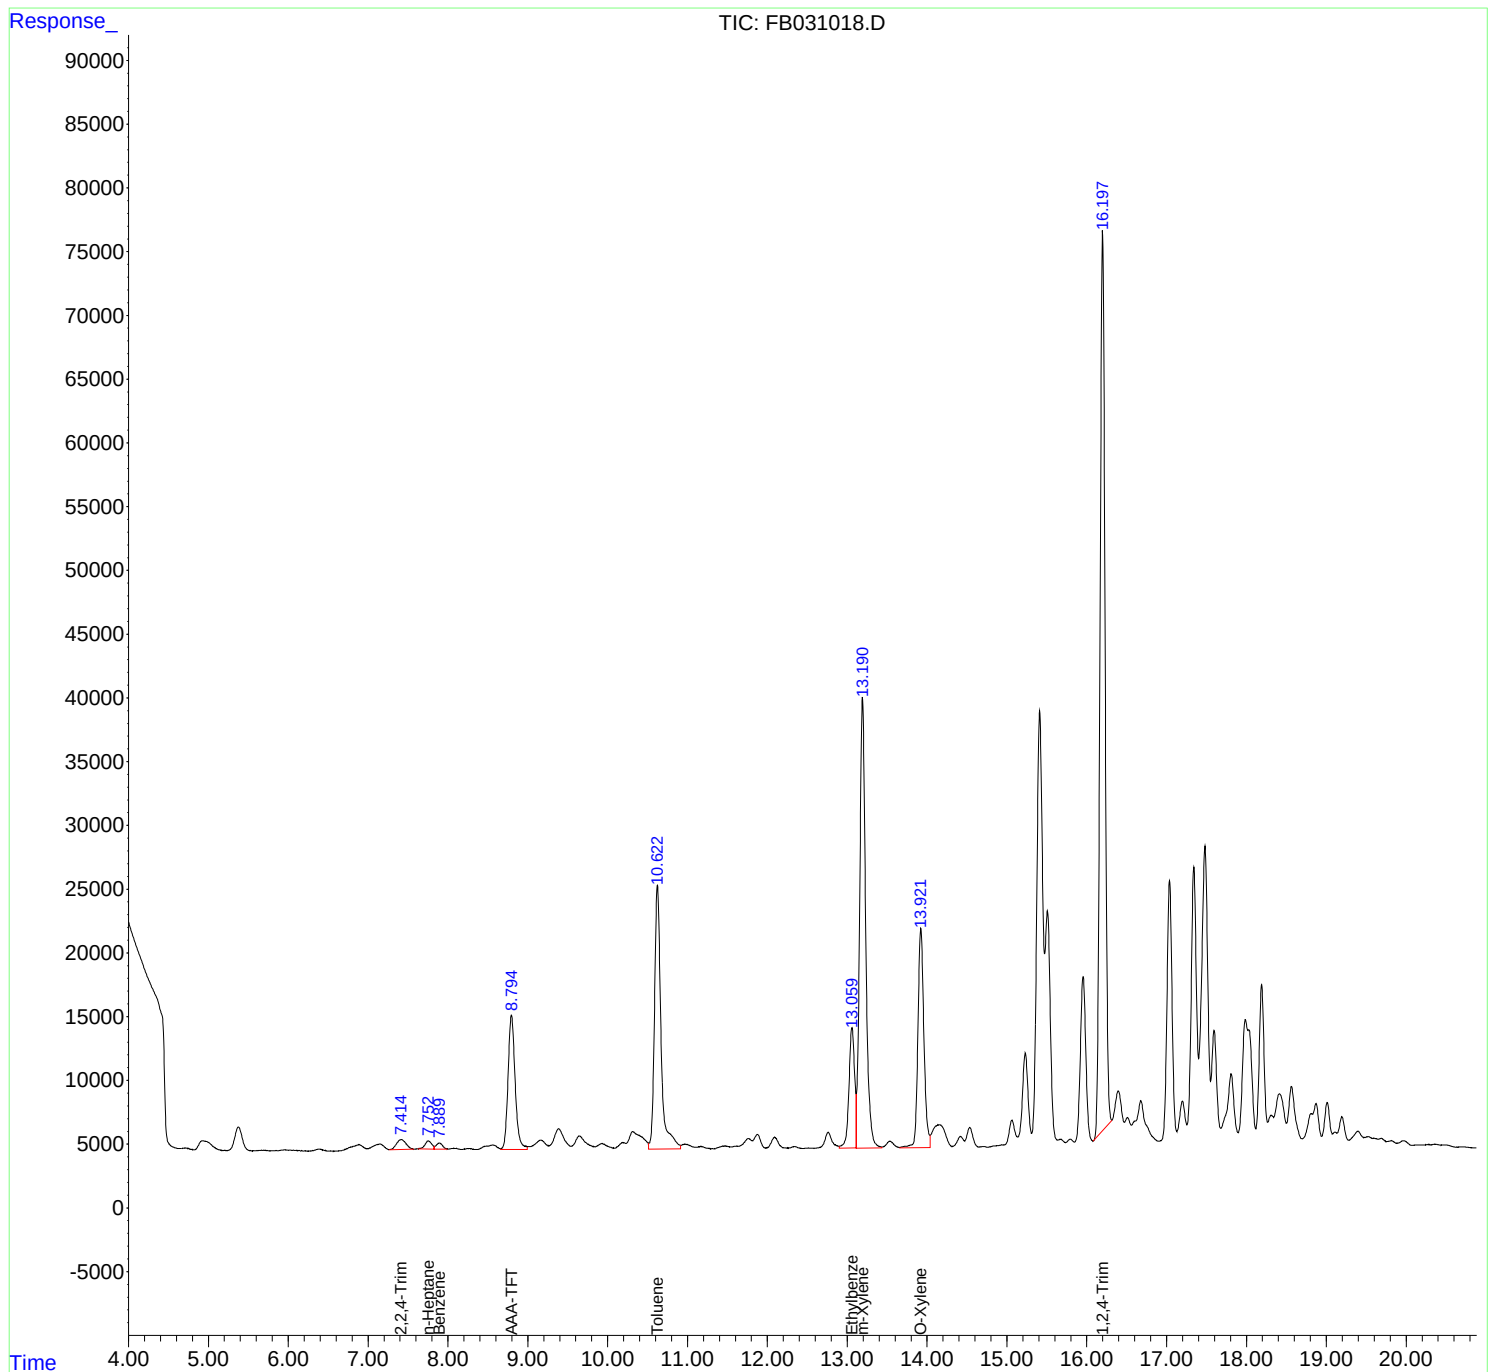

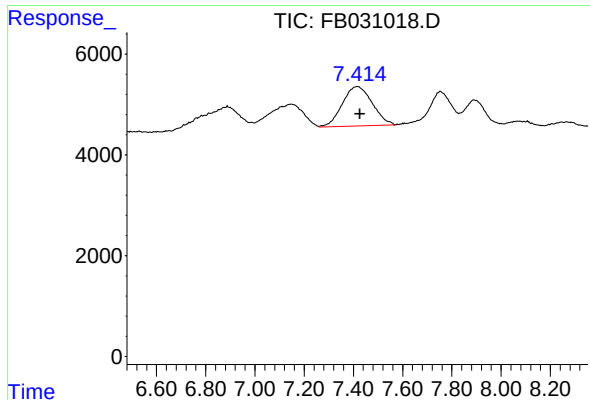


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.012 min
Response: 66218
Conc: 1.39 ng/ml

Instrument :


FID_B

ClientSampleId :

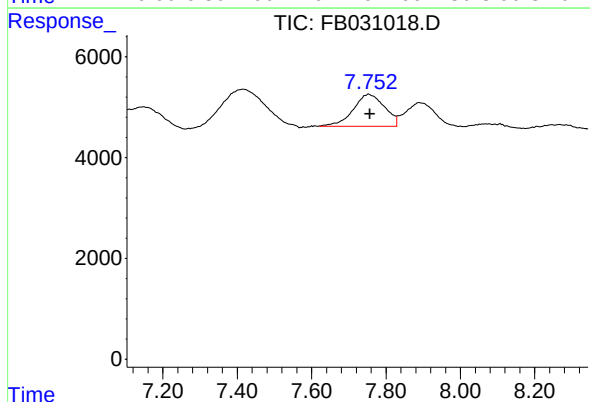


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.003 min
Response: 37253
Conc: 0.83 ng/ml

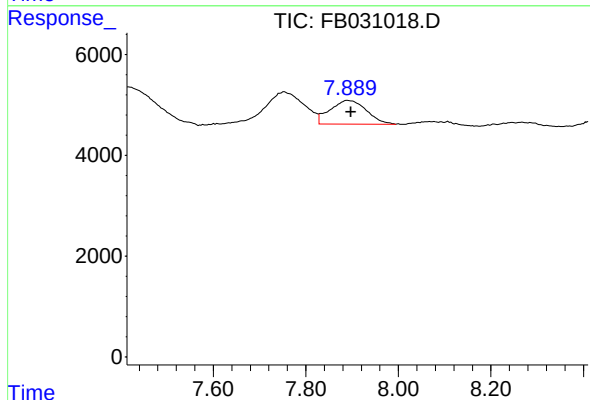


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.007 min
Response: 25781
Conc: 0.47 ng/ml

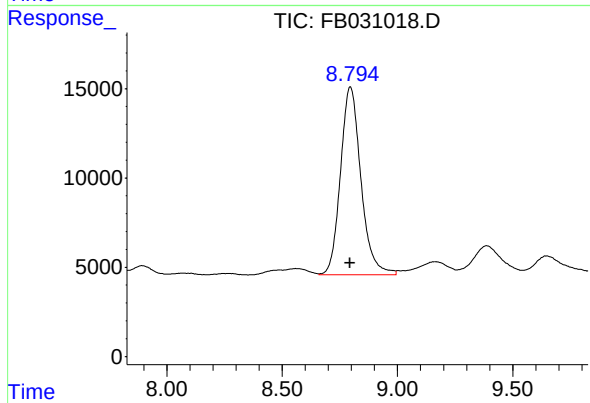

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 647499
Conc: 21.60 ng/ml

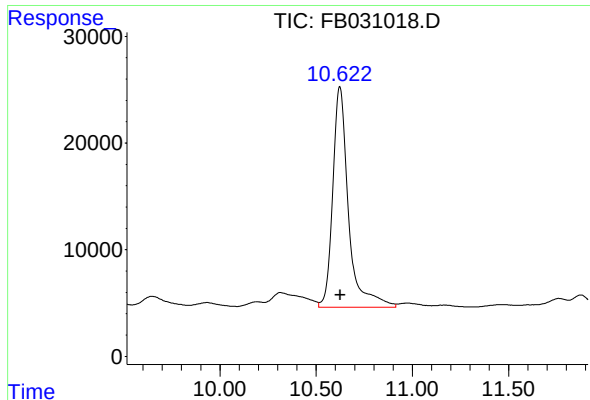

#6 Toluene


R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 1173676
Conc: 21.73 ng/ml

Instrument : FID_B
ClientSampleId :

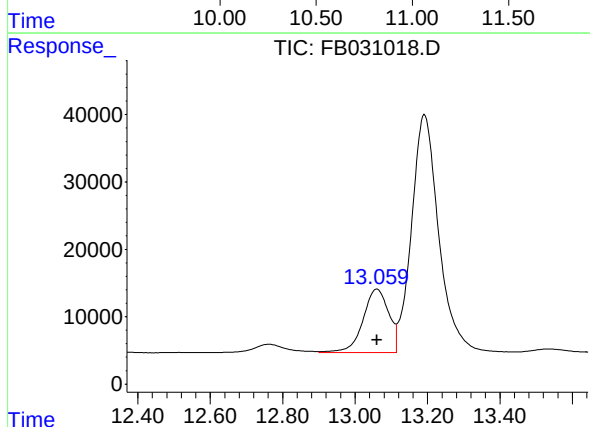


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.000 min
Response: 464275
Conc: 9.79 ng/ml

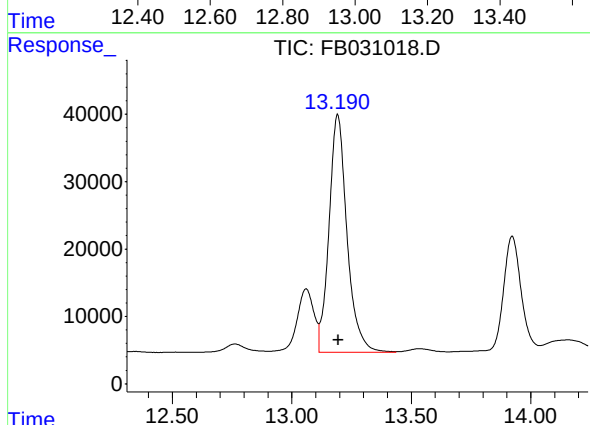


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.003 min
Response: 1849582
Conc: 35.45 ng/ml

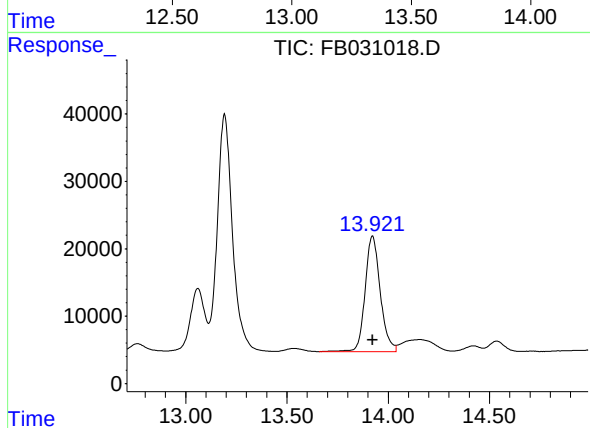

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.000 min
Response: 896996
Conc: 18.44 ng/ml

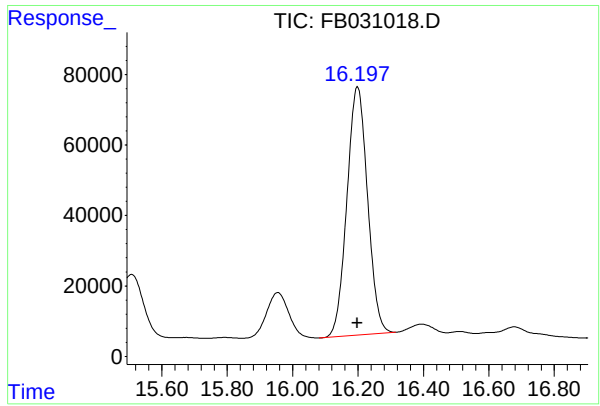

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min

Delta R.T.: 0.000 min

Response: 3093317

Conc: 94.40 ng/ml

Instrument :

FID_B

ClientSampleId :