

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031025.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 16:00
 Operator : YP/AJ
 Sample : P4518-03
 Misc : 8.38G/5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 25 04:02:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.862	8778867	292.849 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.729	5595860	155.075 ng/ml
2) t 2,2,4-Trimethylpentane	7.442	11100232	232.937 ng/ml
3) t n-Heptane	7.758	6906446	153.120 ng/ml
4) t Benzene	7.884	2316253	42.141 ng/ml
6) t Toluene	10.634	2852135	52.798 ng/ml
7) t Ethylbenzene	13.055	7844858	165.503 ng/ml
8) t m-Xylene	13.194	12010305	230.222 ng/ml
9) t O-Xylene	13.929	6486016	133.333 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	3210893	97.988 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031025.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 16:00
Operator : YP/AJ
Sample : P4518-03
Misc : 8.38G/5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:02:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

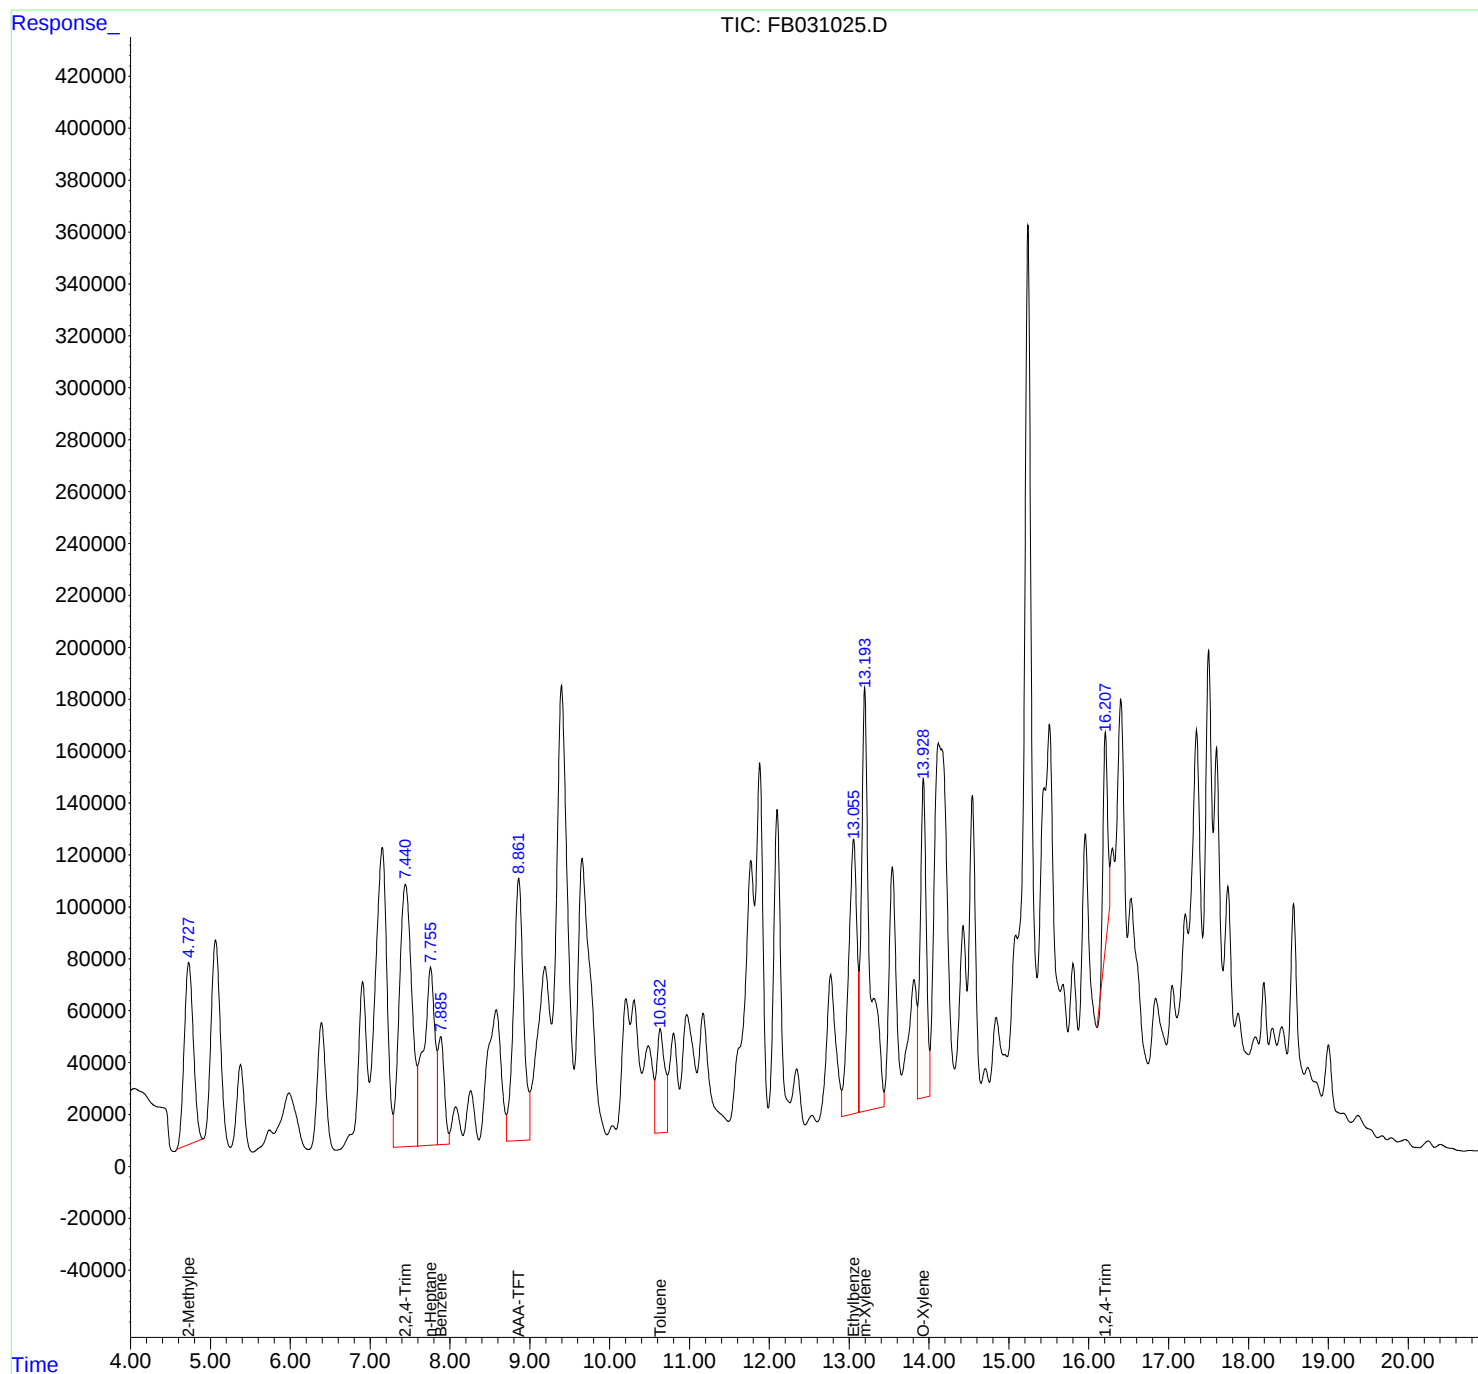


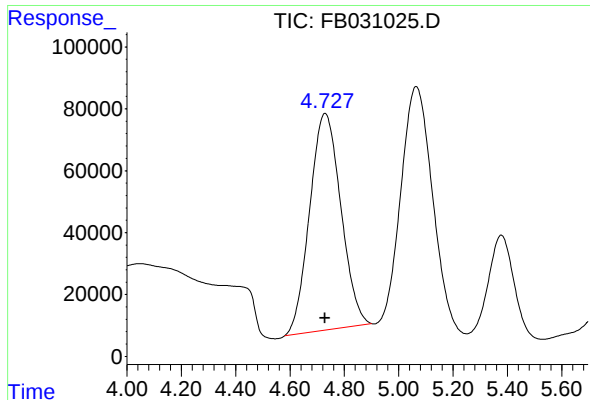

#1 2-Methylpentane


R.T.: 4.729 min
Delta R.T.: 0.001 min
Response: 5595860
Conc: 155.08 ng/ml

Instrument :
FID_B
ClientSampleId :

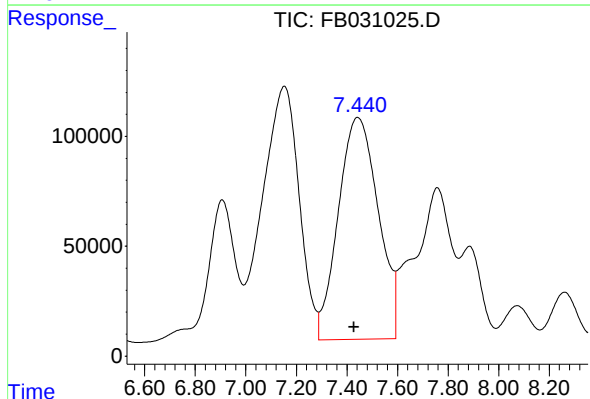


#2 2,2,4-Trimethylpentane

R.T.: 7.442 min
Delta R.T.: 0.015 min
Response: 11100232
Conc: 232.94 ng/ml

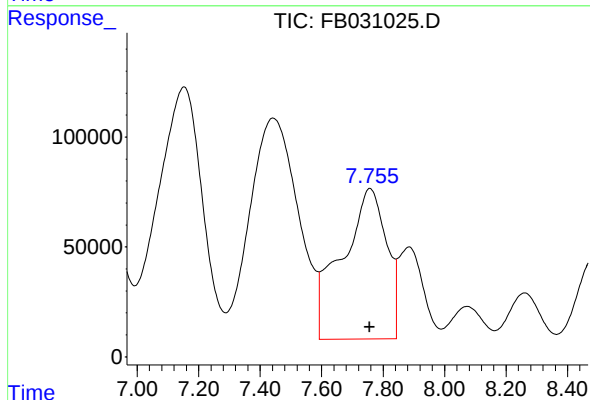


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.001 min
Response: 6906446
Conc: 153.12 ng/ml

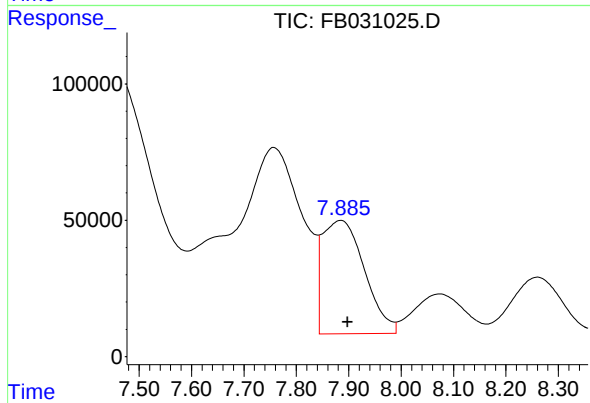

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.014 min
Response: 2316253
Conc: 42.14 ng/ml

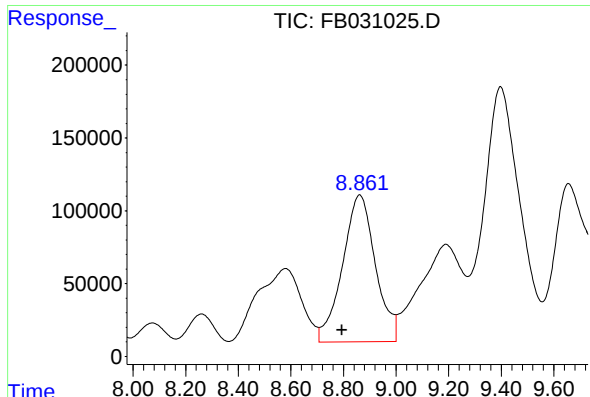

#5 AAA-TFT


R.T.: 8.862 min
Delta R.T.: 0.067 min
Response: 8778867
Conc: 292.85 ng/ml

Instrument :
FID_B
ClientSampleId :

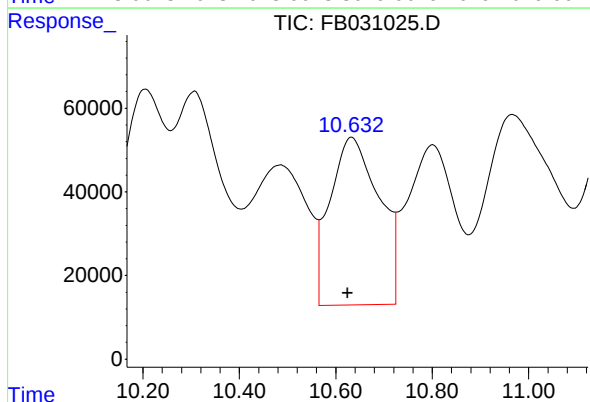


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.009 min
Response: 2852135
Conc: 52.80 ng/ml

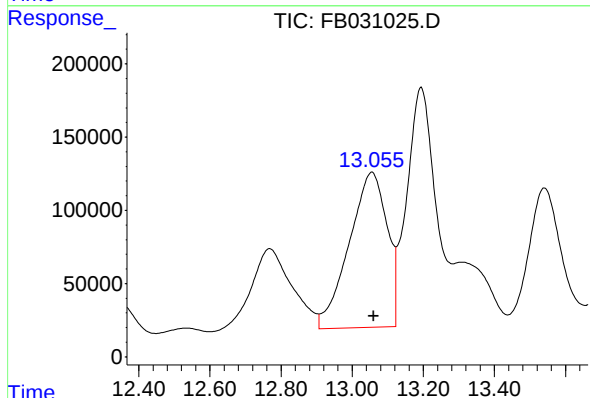


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.005 min
Response: 7844858
Conc: 165.50 ng/ml

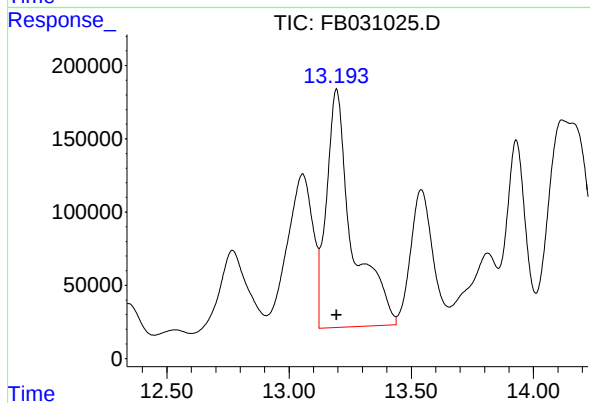

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: 0.000 min
Response: 12010305
Conc: 230.22 ng/ml

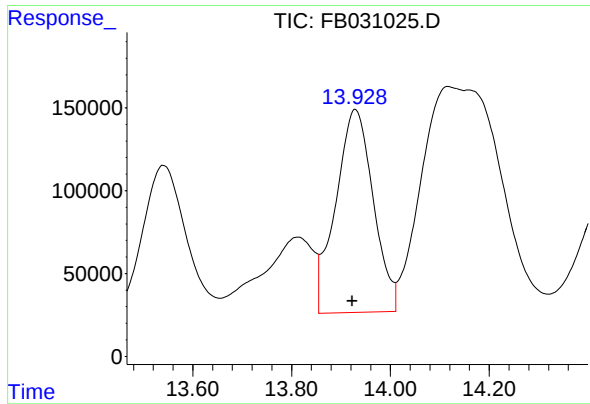

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.007 min
Response: 6486016
Conc: 133.33 ng/ml

Instrument :
FID_B
ClientSampleId :

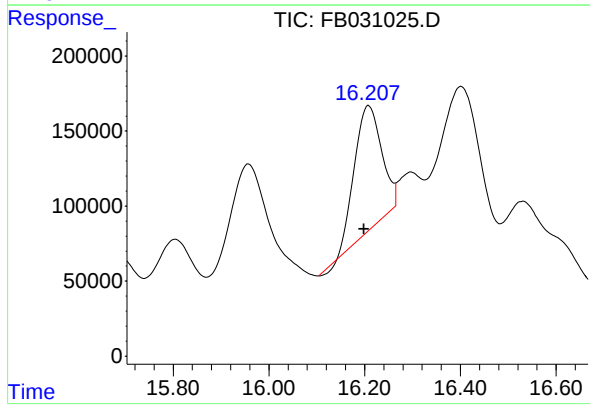

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.011 min
Response: 3210893
Conc: 97.99 ng/ml