

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031027.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 16:54
 Operator : YP/AJ
 Sample : P4518-05
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 25 04:03:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.862	7815474	260.711 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.730	4464019	123.709 ng/ml
2) t 2,2,4-Trimethylpentane	7.446	10683302	224.188 ng/ml
3) t n-Heptane	7.759	6221796	137.941 ng/ml
4) t Benzene	7.891	3320474	60.411 ng/ml
6) t Toluene	10.632	4368849	80.875 ng/ml
7) t Ethylbenzene	13.062	9761944	205.947 ng/ml
8) t m-Xylene	13.195	13315338	255.238 ng/ml
9) t O-Xylene	13.930	7606994	156.377 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	3005808	91.730 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031027.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 16:54
Operator : YP/AJ
Sample : P4518-05
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:03:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

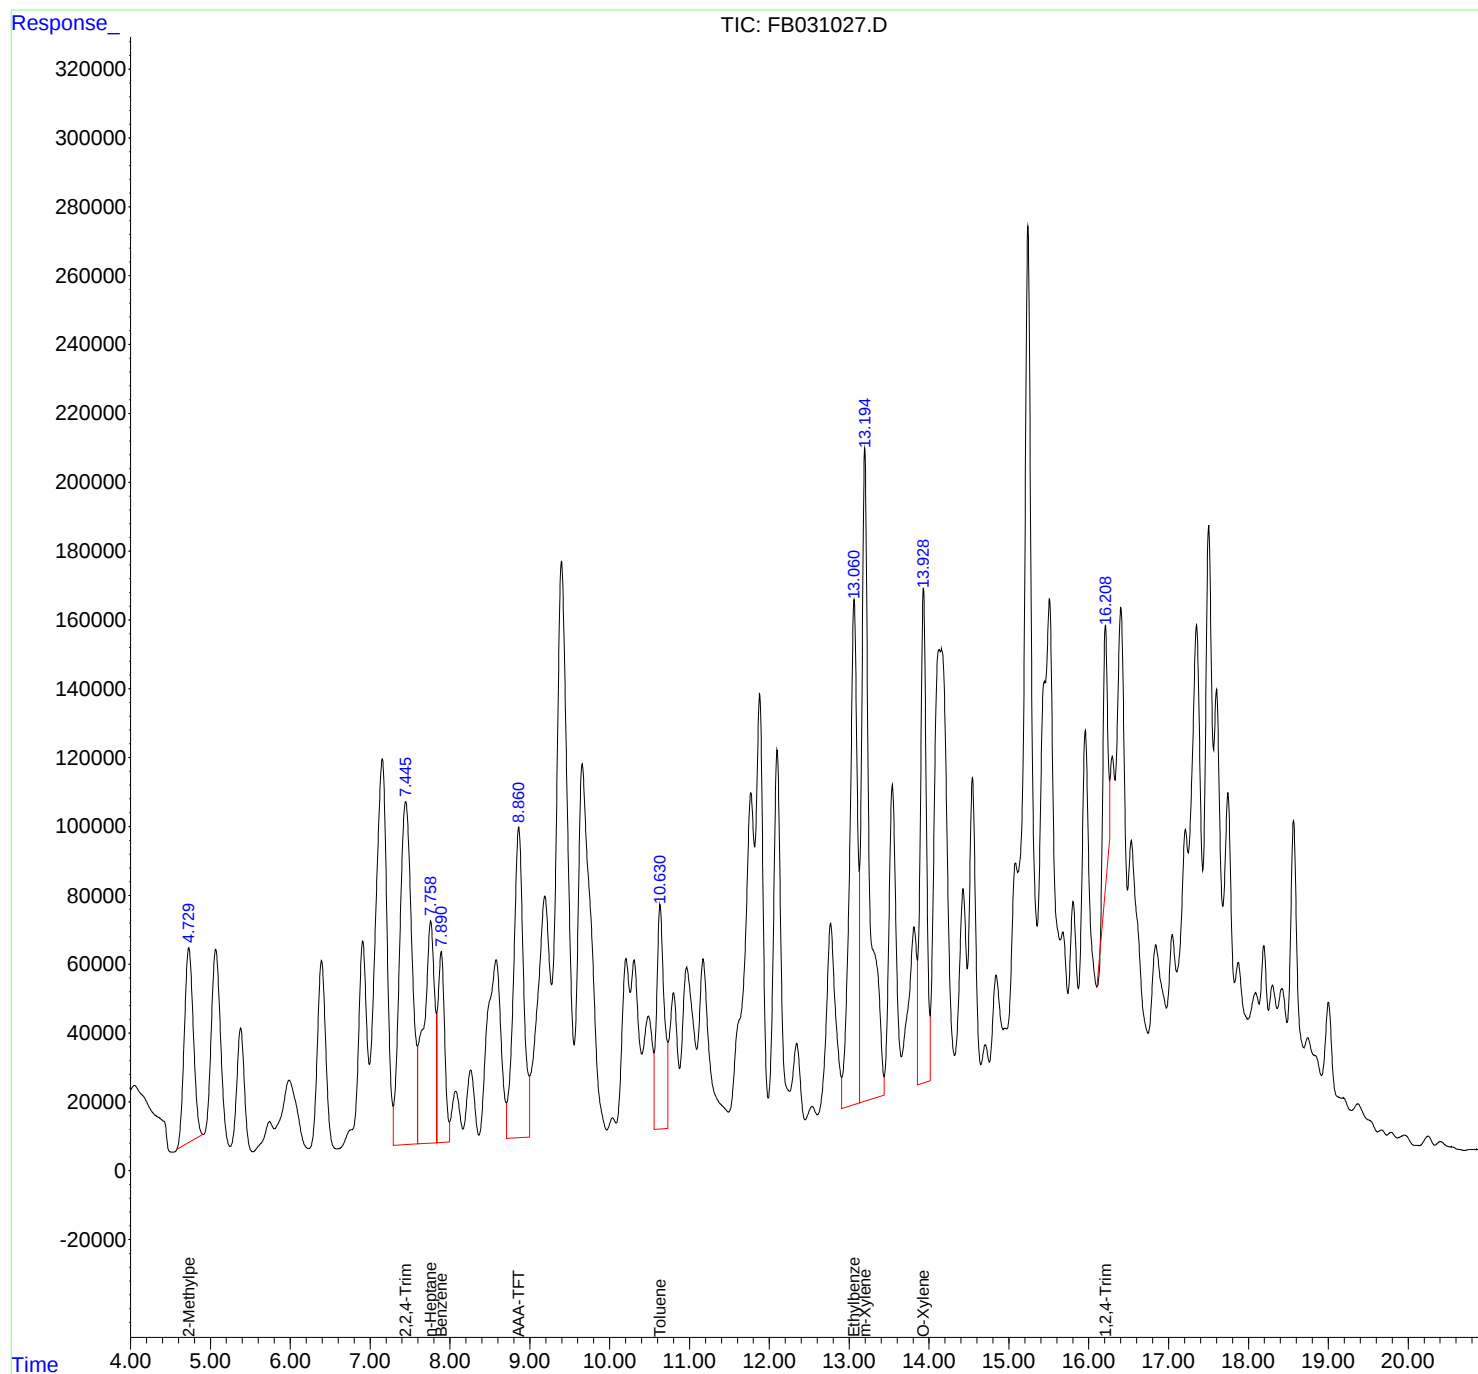


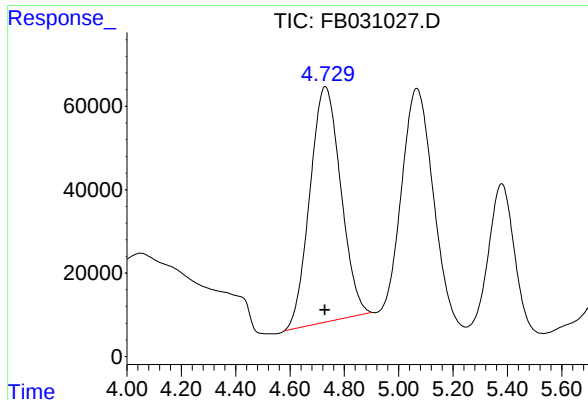

#1 2-Methylpentane


R.T.: 4.730 min
Delta R.T.: 0.002 min
Response: 4464019
Conc: 123.71 ng/ml

Instrument :
FID_B
ClientSampleId :

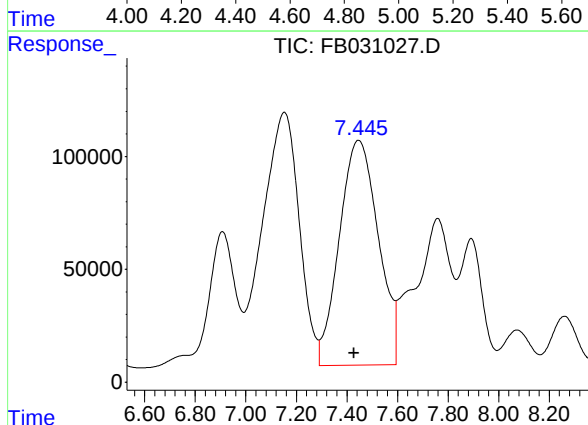


#2 2,2,4-Trimethylpentane

R.T.: 7.446 min
Delta R.T.: 0.018 min
Response: 10683302
Conc: 224.19 ng/ml

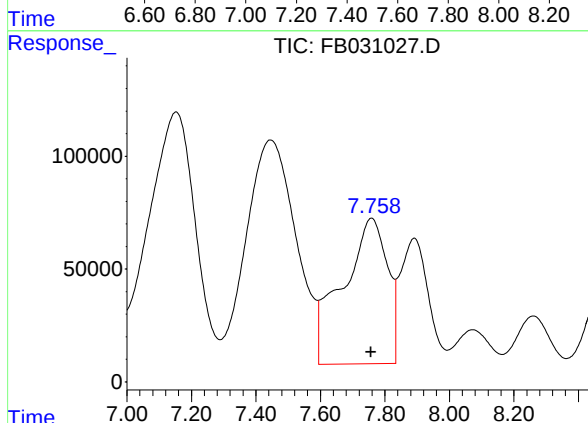


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.002 min
Response: 6221796
Conc: 137.94 ng/ml

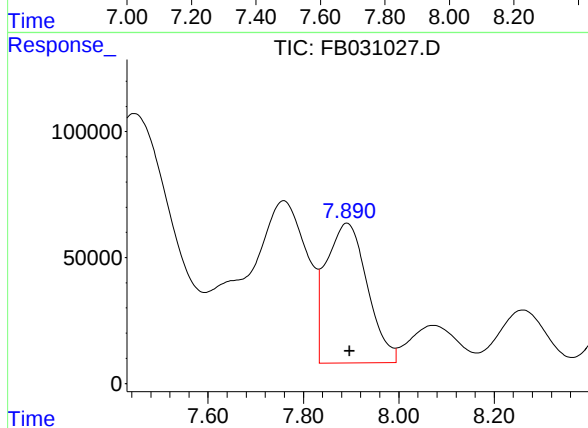

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.006 min
Response: 3320474
Conc: 60.41 ng/ml

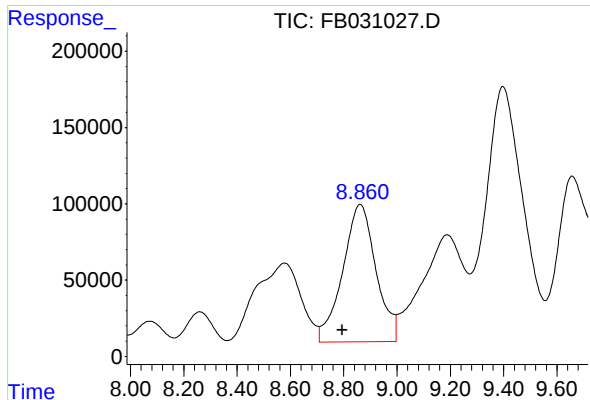

#5 AAA-TFT


R.T.: 8.862 min
Delta R.T.: 0.066 min
Response: 7815474
Conc: 260.71 ng/ml

Instrument :
FID_B
ClientSampleId :

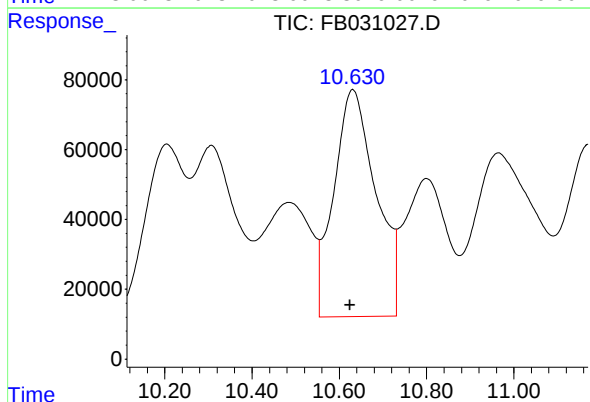


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.007 min
Response: 4368849
Conc: 80.88 ng/ml

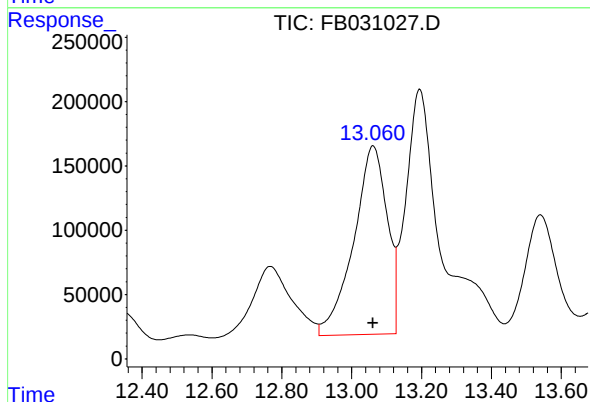


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.001 min
Response: 9761944
Conc: 205.95 ng/ml

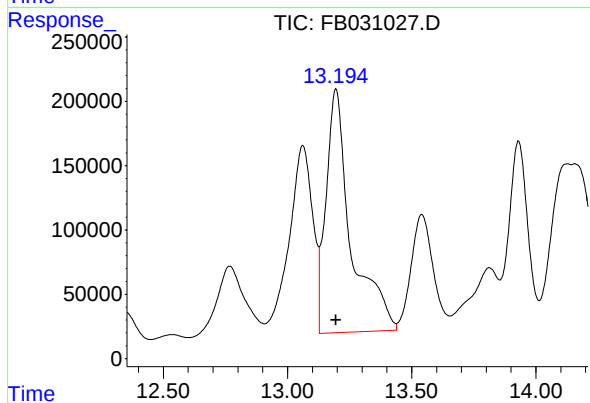

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.000 min
Response: 13315338
Conc: 255.24 ng/ml

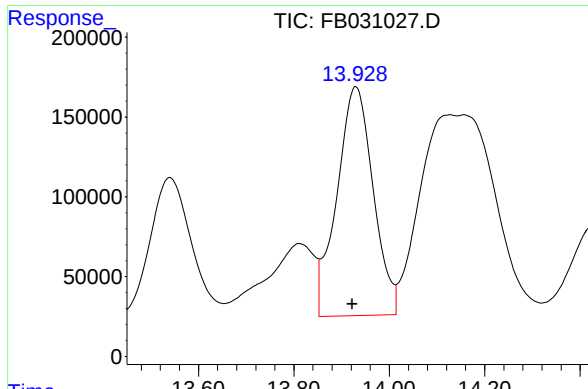

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.007 min
Response: 7606994
Conc: 156.38 ng/ml

Instrument :
FID_B
ClientSampleId :

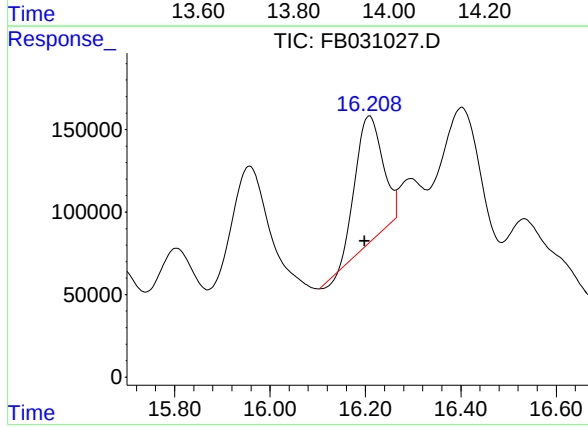

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.011 min
Response: 3005808
Conc: 91.73 ng/ml