

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031028.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 17:20
 Operator : YP/AJ
 Sample : P4509-01
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 25 04:03:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.860	21953	0.732 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.418	21726	0.456 ng/ml
6) t Toluene	10.630	17630	0.326 ng/ml
7) t Ethylbenzene	13.046	105260	2.221 ng/ml
8) t m-Xylene	13.190	78656	1.508 ng/ml
9) t O-Xylene	13.924	65358	1.344 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	120822	3.687 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031028.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 17:20
Operator : YP/AJ
Sample : P4509-01
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:03:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

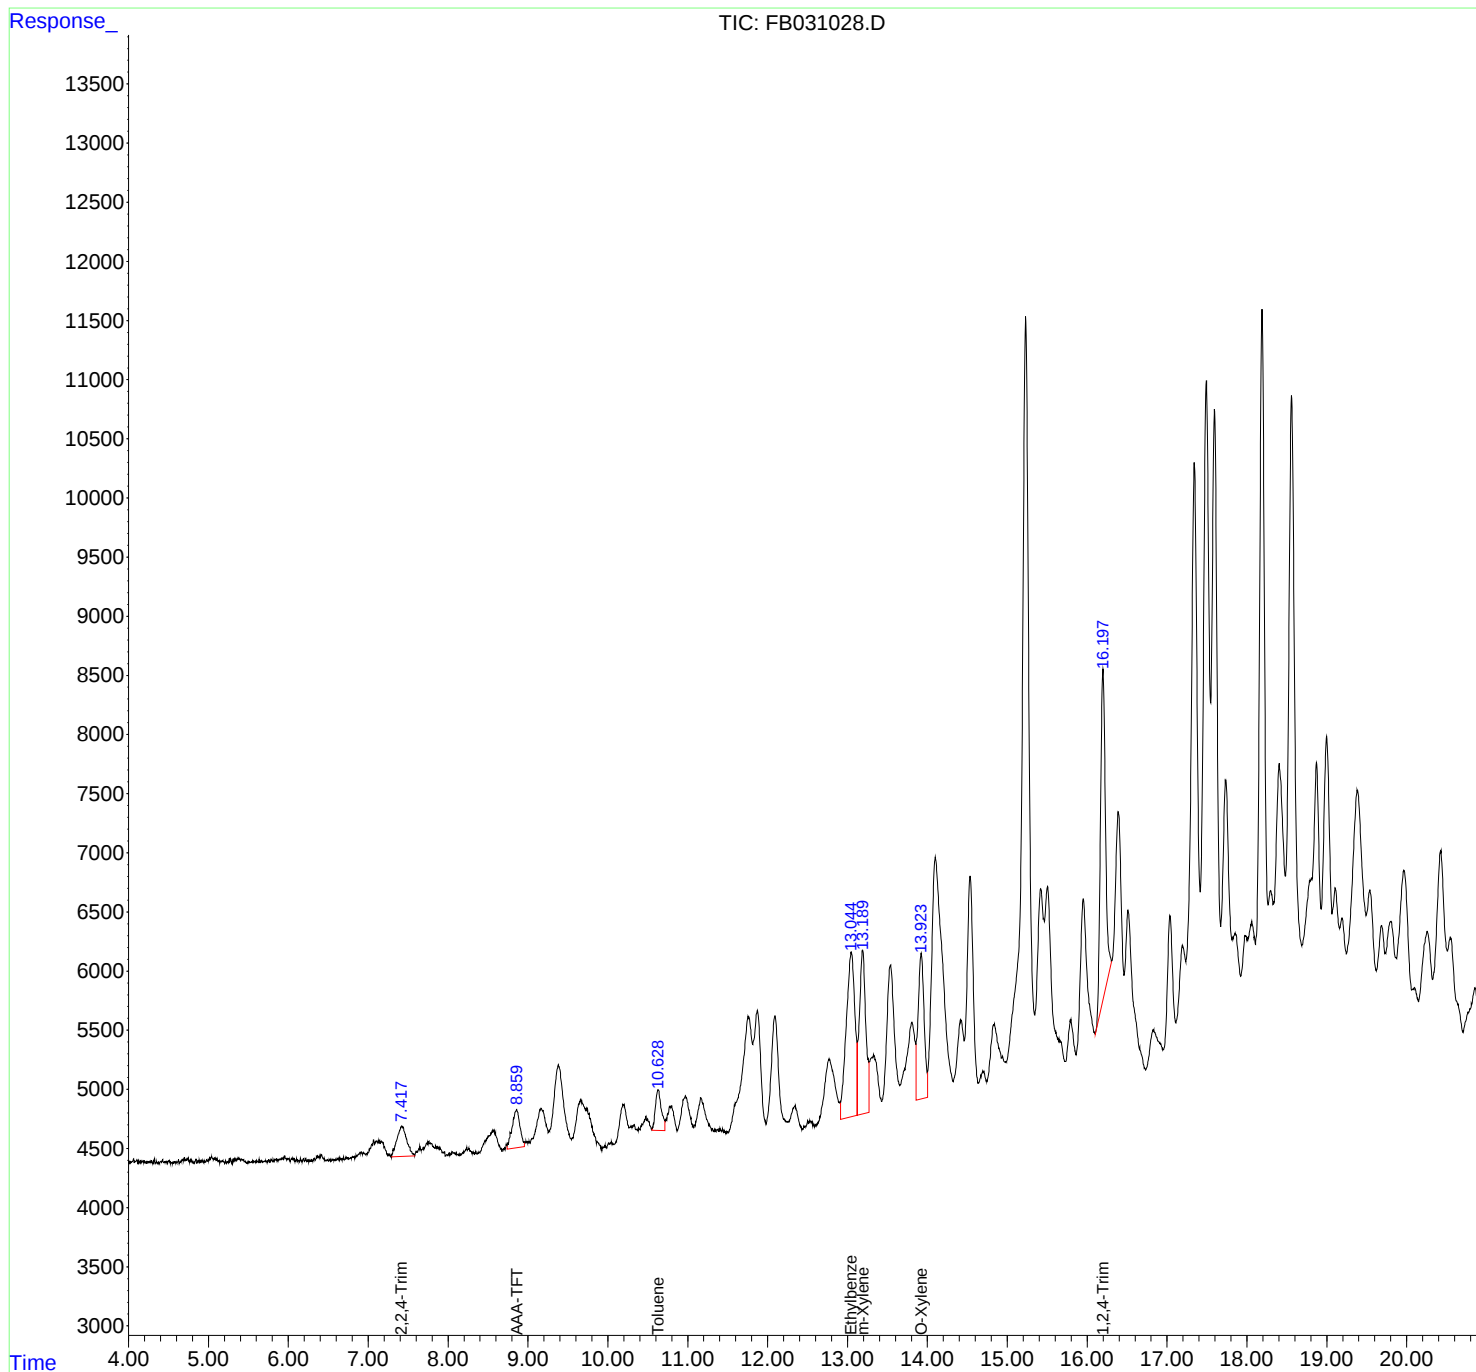

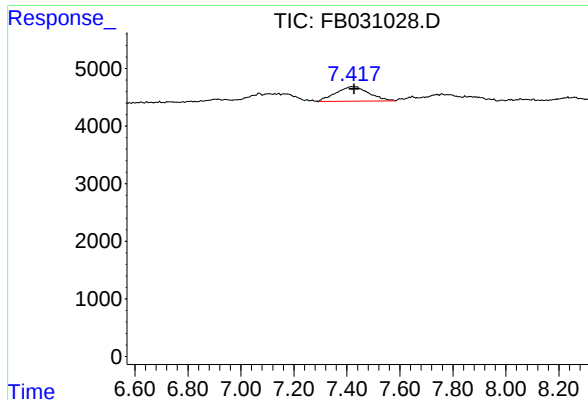


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.009 min
Response: 21726
Conc: 0.46 ng/ml

Instrument :


FID_B

ClientSampleId :

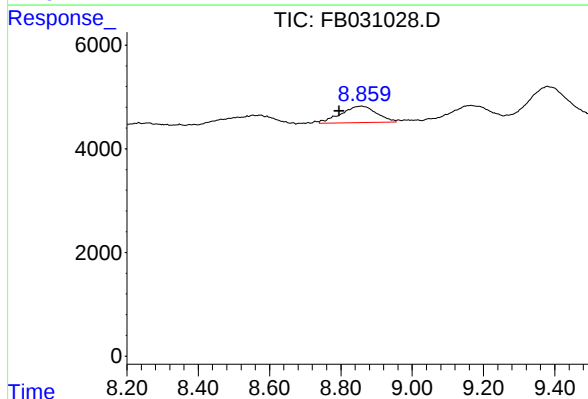


#5 AAA-TFT

R.T.: 8.860 min
Delta R.T.: 0.064 min
Response: 21953
Conc: 0.73 ng/ml

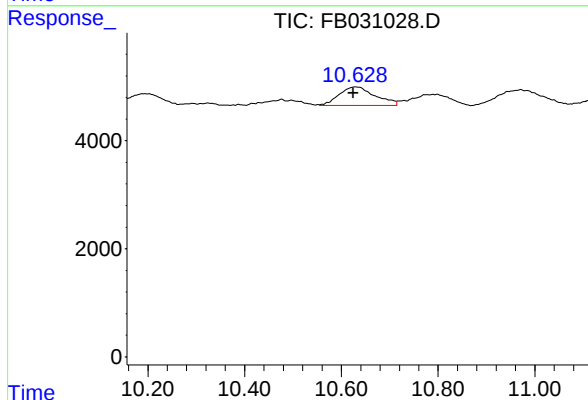


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.006 min
Response: 17630
Conc: 0.33 ng/ml

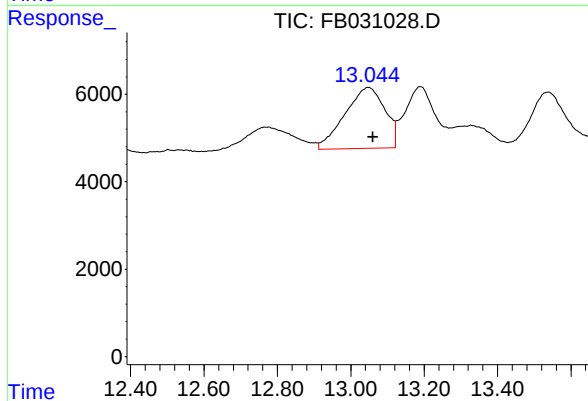

#7 Ethylbenzene


R.T.: 13.046 min
Delta R.T.: -0.014 min
Response: 105260
Conc: 2.22 ng/ml

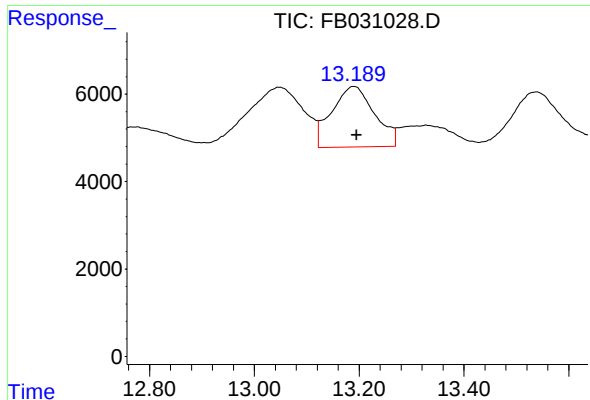

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.005 min
Response: 78656
Conc: 1.51 ng/ml

Instrument :
FID_B
ClientSampleId :

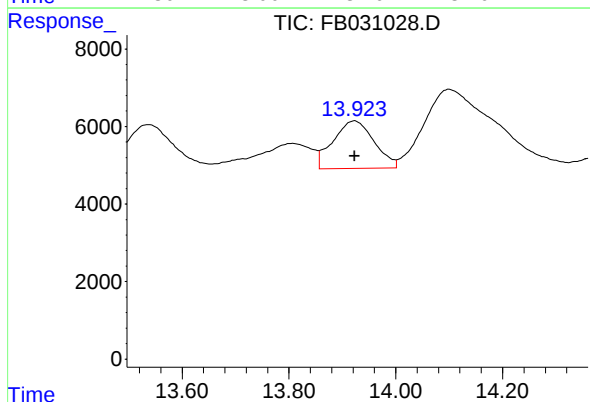

#9 o-Xylene

R.T.: 13.924 min
Delta R.T.: 0.001 min
Response: 65358
Conc: 1.34 ng/ml

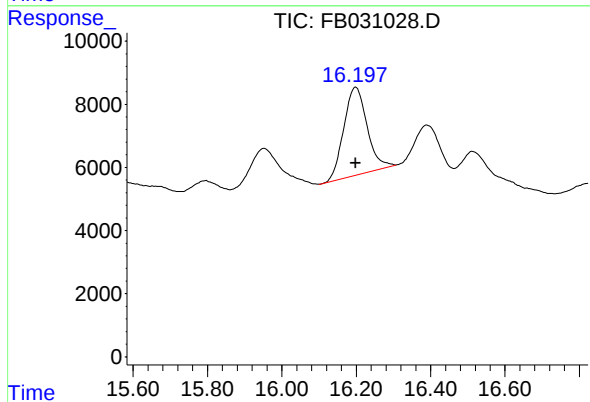

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.000 min
Response: 120822
Conc: 3.69 ng/ml