

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031029.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 17:47
Operator : YP/AJ
Sample : P4509-01
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:03:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.813	2038	0.068 ng/ml
Target Compounds			
6) t Toluene	10.626	9160	0.170 ng/ml
7) t Ethylbenzene	13.054	52137	1.100 ng/ml
8) t m-Xylene	13.188	37813	0.725 ng/ml
9) t O-Xylene	13.927	26991	0.555 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	65583	2.001 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031029.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 17:47
Operator : YP/AJ
Sample : P4509-01
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:03:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

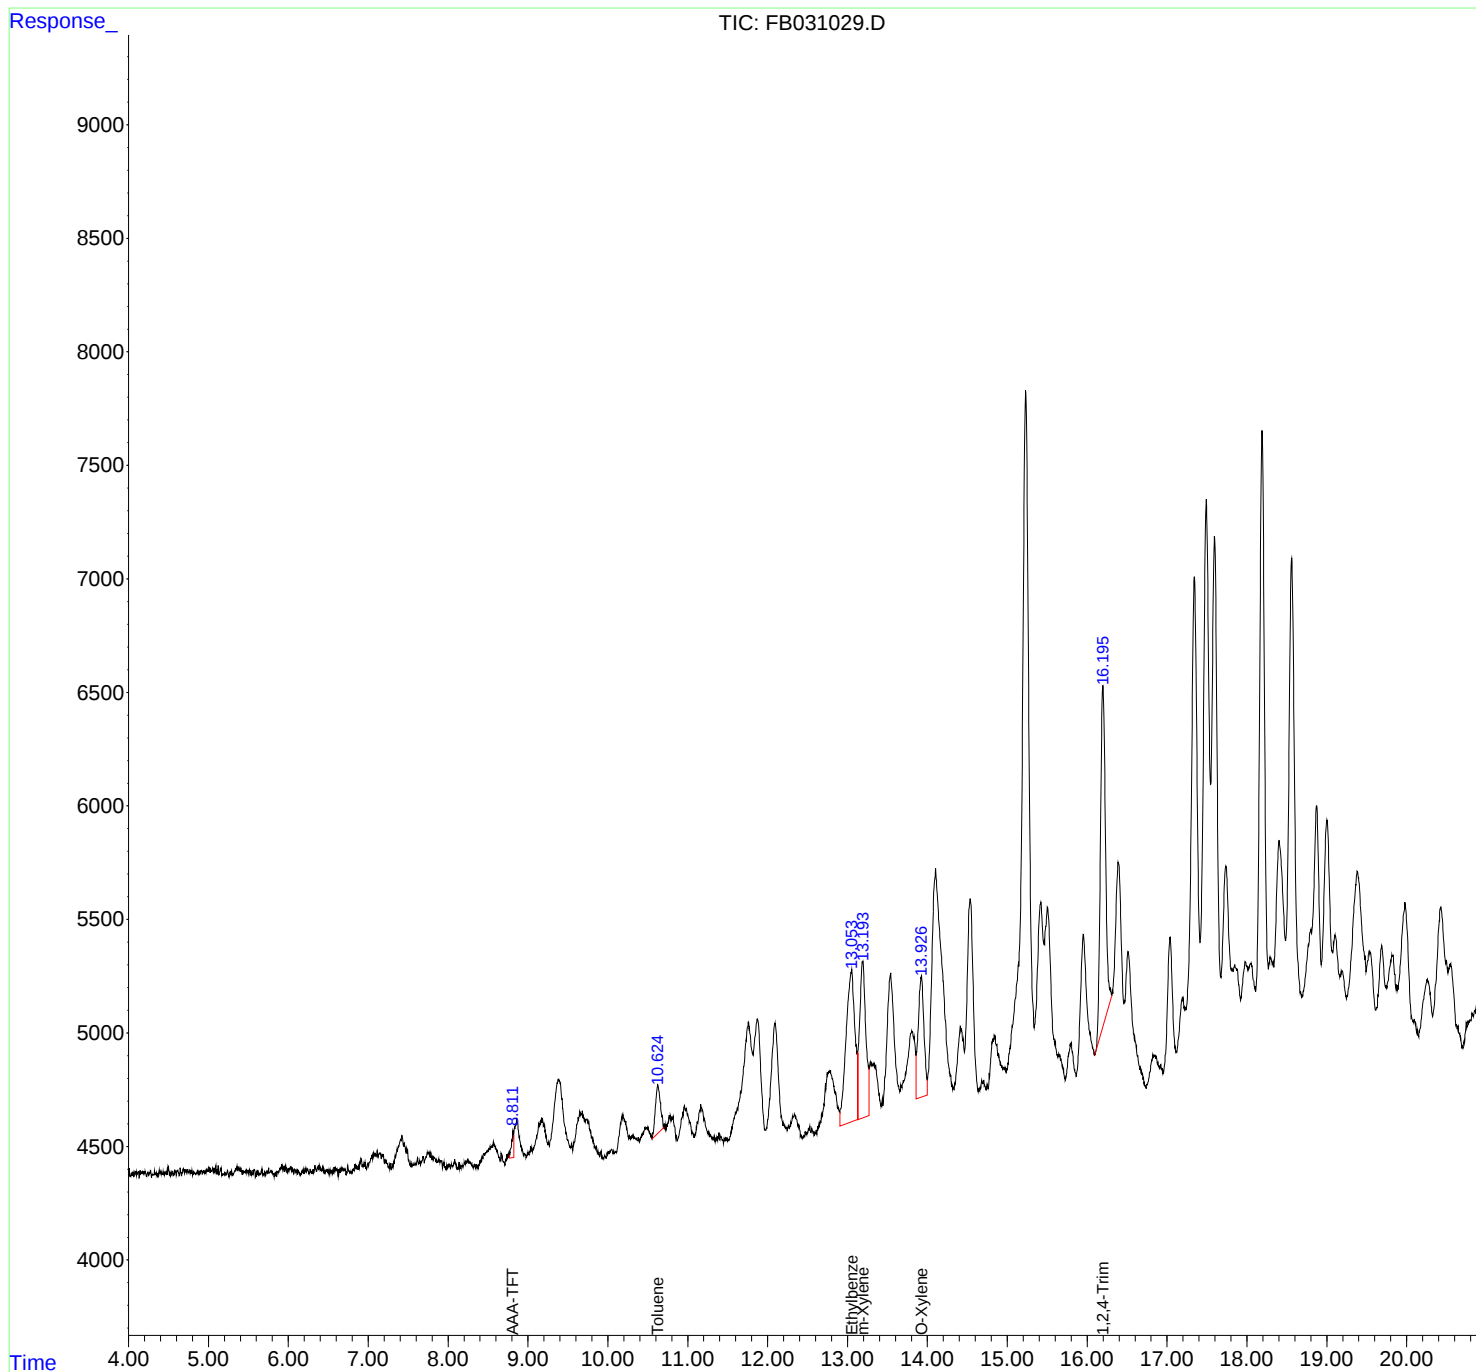


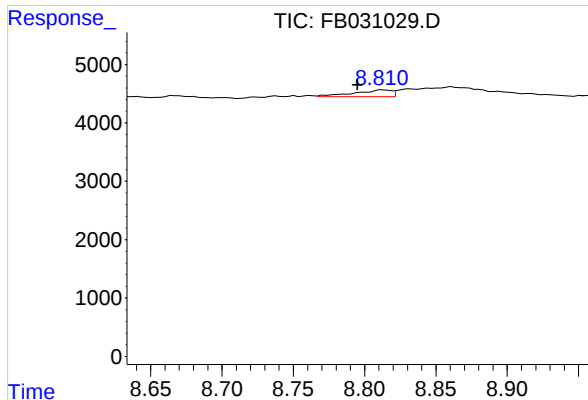

#5 AAA-TFT


R.T.: 8.813 min
Delta R.T.: 0.018 min
Response: 2038
Conc: 0.07 ng/ml

Instrument :
FID_B
ClientSampleId :

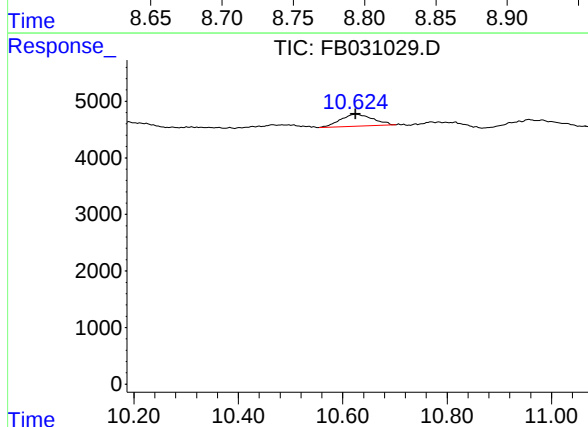


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.002 min
Response: 9160
Conc: 0.17 ng/ml

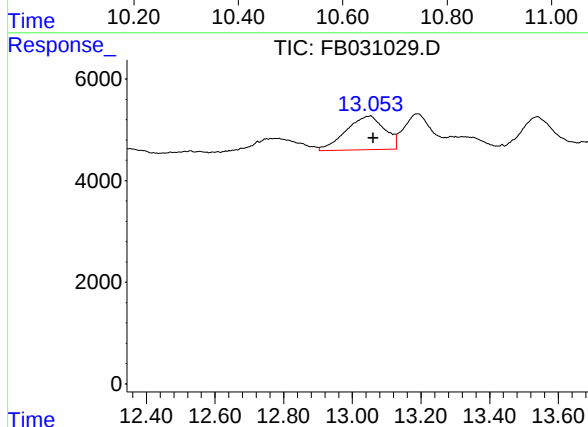


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.006 min
Response: 52137
Conc: 1.10 ng/ml

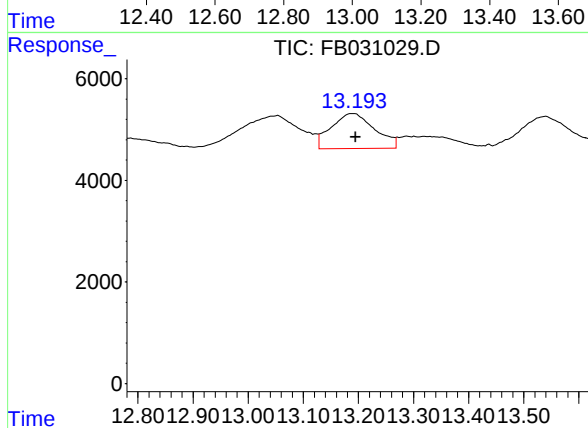

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.007 min
Response: 37813
Conc: 0.72 ng/ml

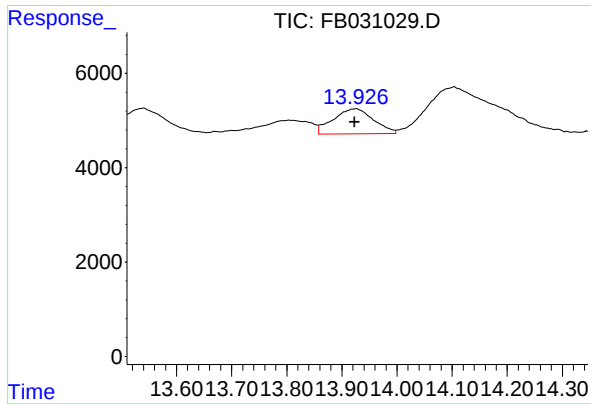

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.004 min
Response: 26991
Conc: 0.55 ng/ml

Instrument :
FID_B
ClientSampleId :

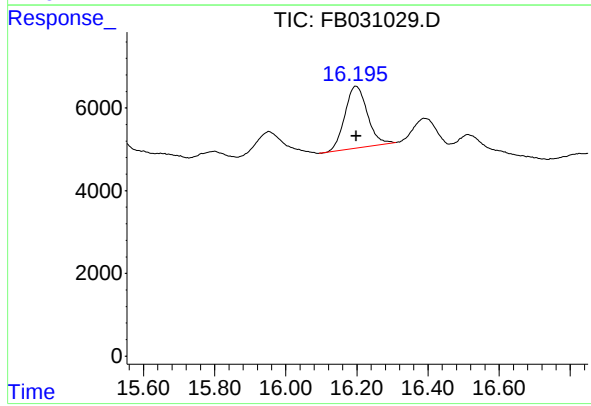

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.001 min
Response: 65583
Conc: 2.00 ng/ml