

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031030.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 18:14
 Operator : YP/AJ
 Sample : P4509-01 50X
 Misc : 4.99G/5.00 ML MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 25 04:03:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	524365	17.492 ng/ml
Target Compounds				
2) t	2,2,4-Trimethylpentane	7.445	10185	0.214 ng/ml
6) t	Toluene	10.623	29558	0.547 ng/ml
7) t	Ethylbenzene	13.051	47870	1.010 ng/ml
8) t	m-Xylene	13.195	48520	0.930 ng/ml
9) t	O-Xylene	13.925	26708	0.549 ng/ml
10) t	1,2,4-Trimethylbenzene	16.203	69638	2.125 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031030.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 18:14
Operator : YP/AJ
Sample : P4509-01 50X
Misc : 4.99G/5.00 ML MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:03:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

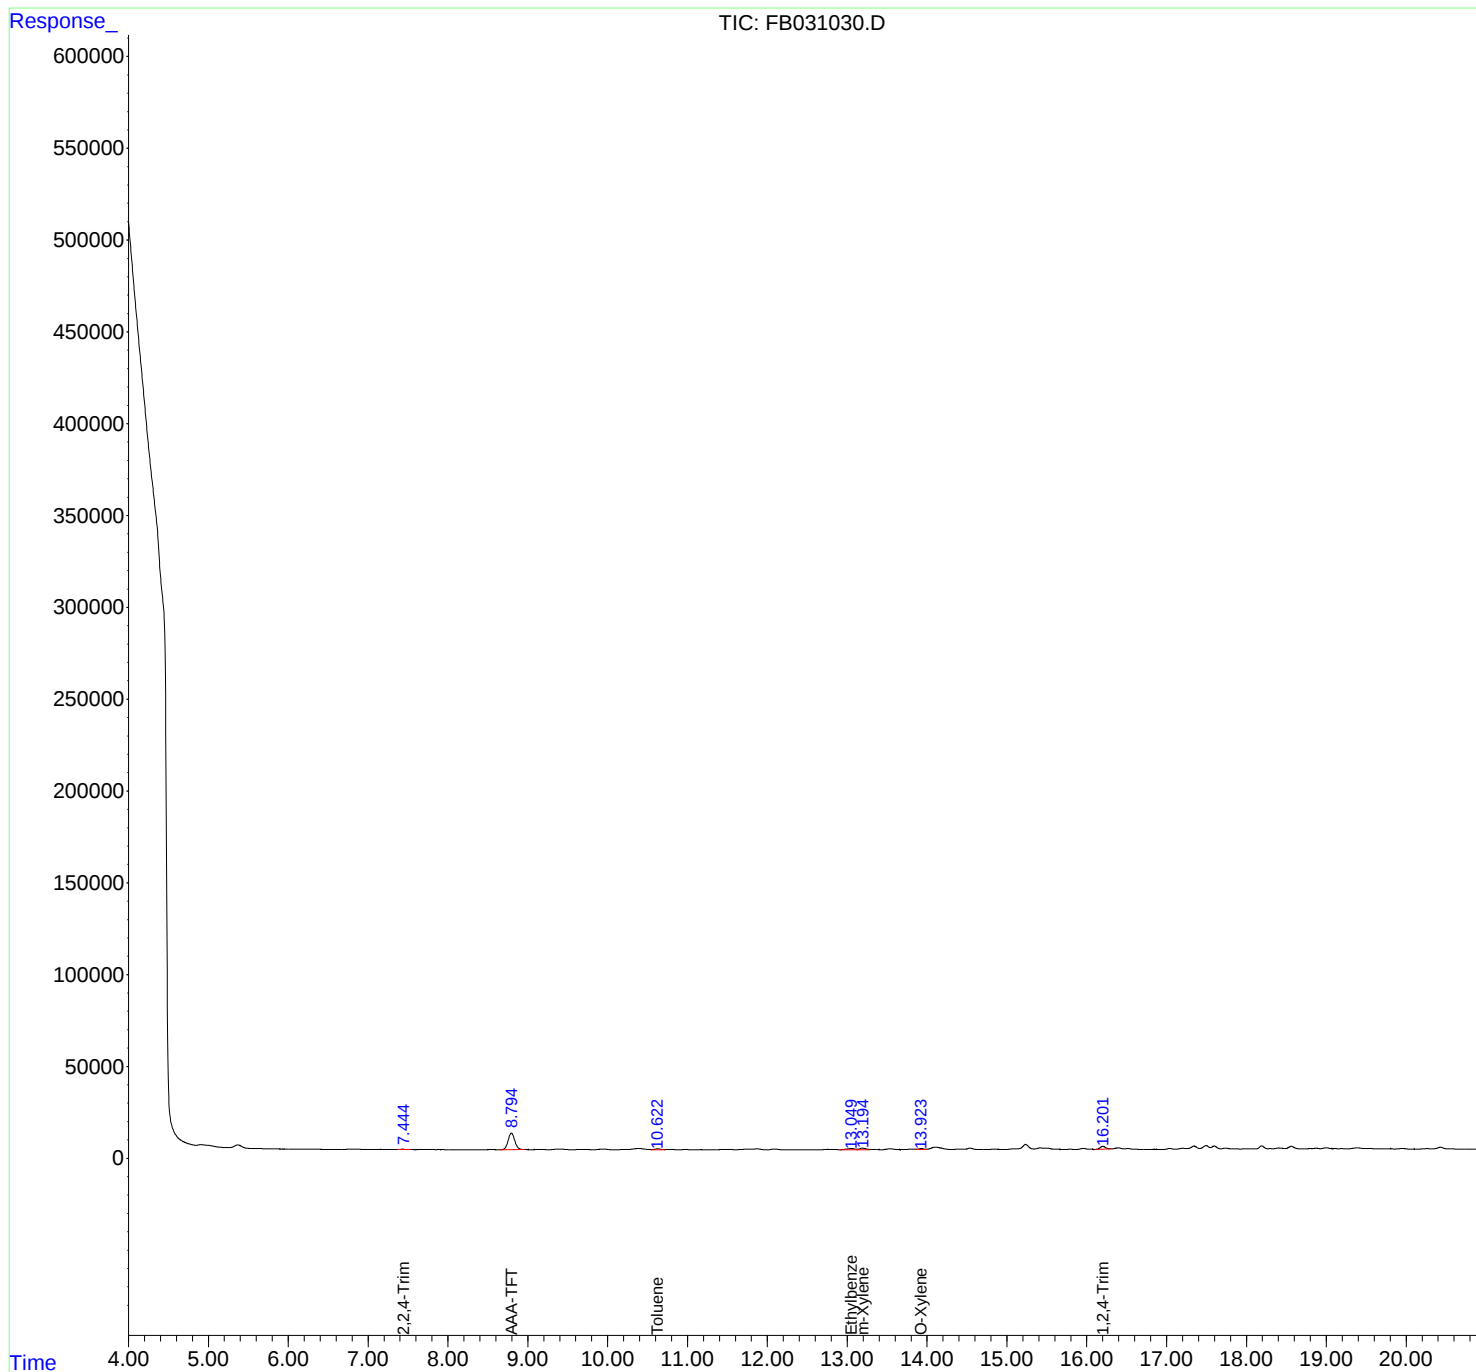


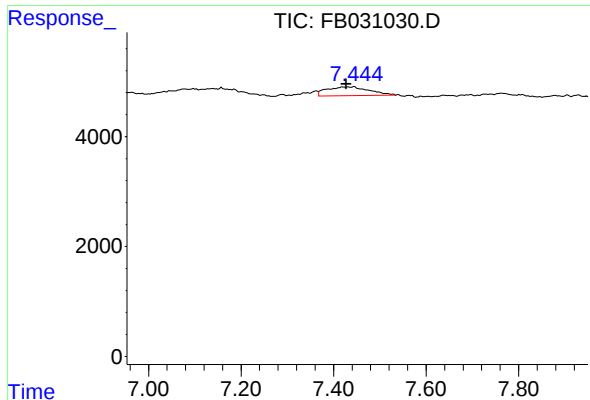

#2 2,2,4-Trimethylpentane


R.T.: 7.445 min
Delta R.T.: 0.017 min
Response: 10185
Conc: 0.21 ng/ml

Instrument :
FID_B
ClientSampleId :

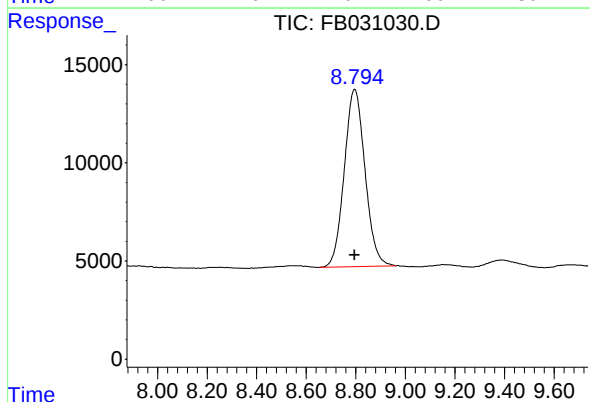


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 524365
Conc: 17.49 ng/ml

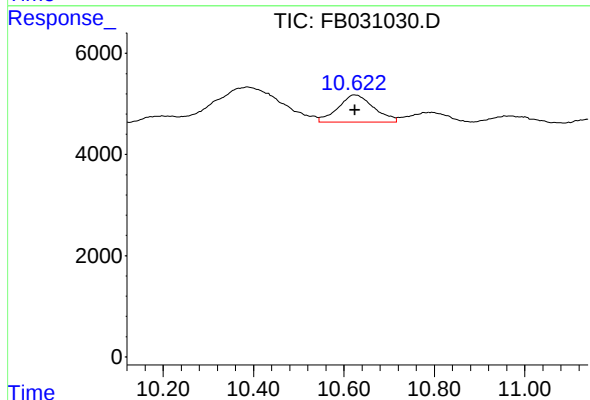


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.001 min
Response: 29558
Conc: 0.55 ng/ml

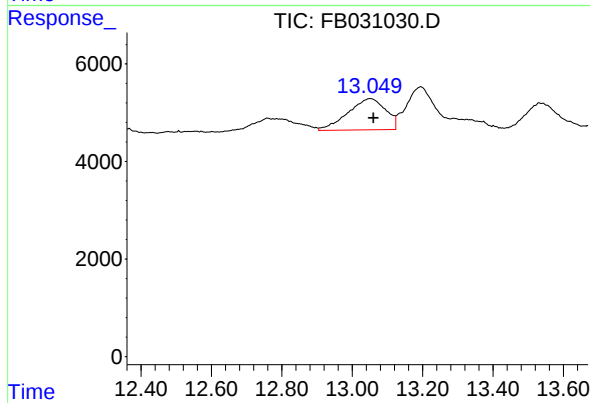

#7 Ethylbenzene


R.T.: 13.051 min
Delta R.T.: -0.010 min
Response: 47870
Conc: 1.01 ng/ml

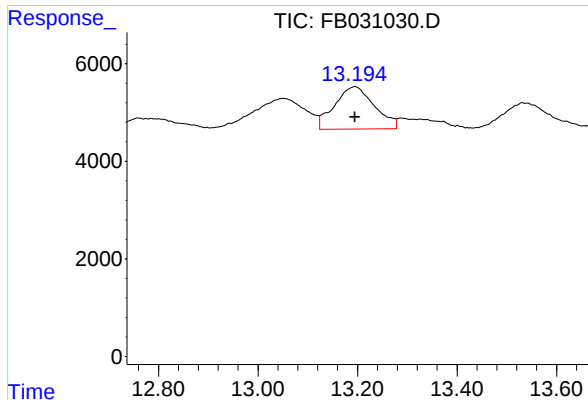

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.000 min
Response: 48520
Conc: 0.93 ng/ml

Instrument :
FID_B
ClientSampleId :

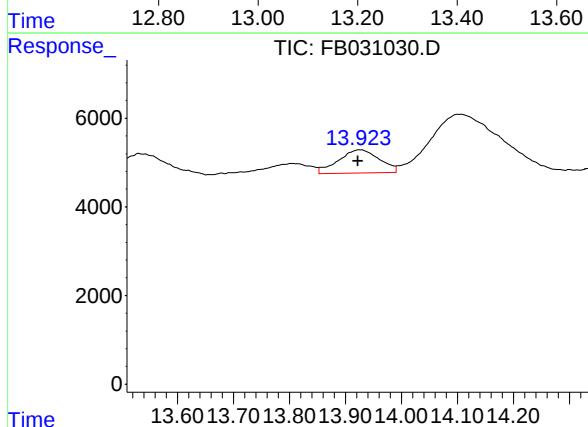

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.002 min
Response: 26708
Conc: 0.55 ng/ml

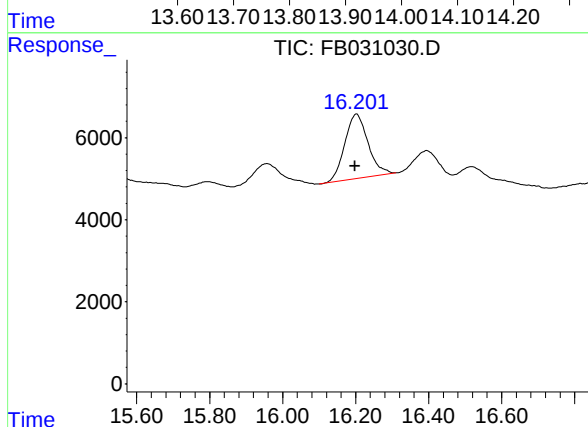

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: 0.004 min
Response: 69638
Conc: 2.13 ng/ml