

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031032.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 19:07
 Operator : YP/AJ
 Sample : P4509-01MSD 50X
 Misc : 5.02G/5.00 ML MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 25 04:03:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	377061	12.578 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	560345	15.529 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	868135	18.218 ng/ml
3) t n-Heptane	7.754	233599	5.179 ng/ml
4) t Benzene	7.895	311336	5.664 ng/ml
6) t Toluene	10.625	880590	16.301 ng/ml
7) t Ethylbenzene	13.063	278950	5.885 ng/ml
8) t m-Xylene	13.197	584751	11.209 ng/ml
9) t O-Xylene	13.926	523379	10.759 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	396462	12.099 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031032.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 19:07
Operator : YP/AJ
Sample : P4509-01MSD 50X
Misc : 5.02G/5.00 ML MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 25 04:03:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

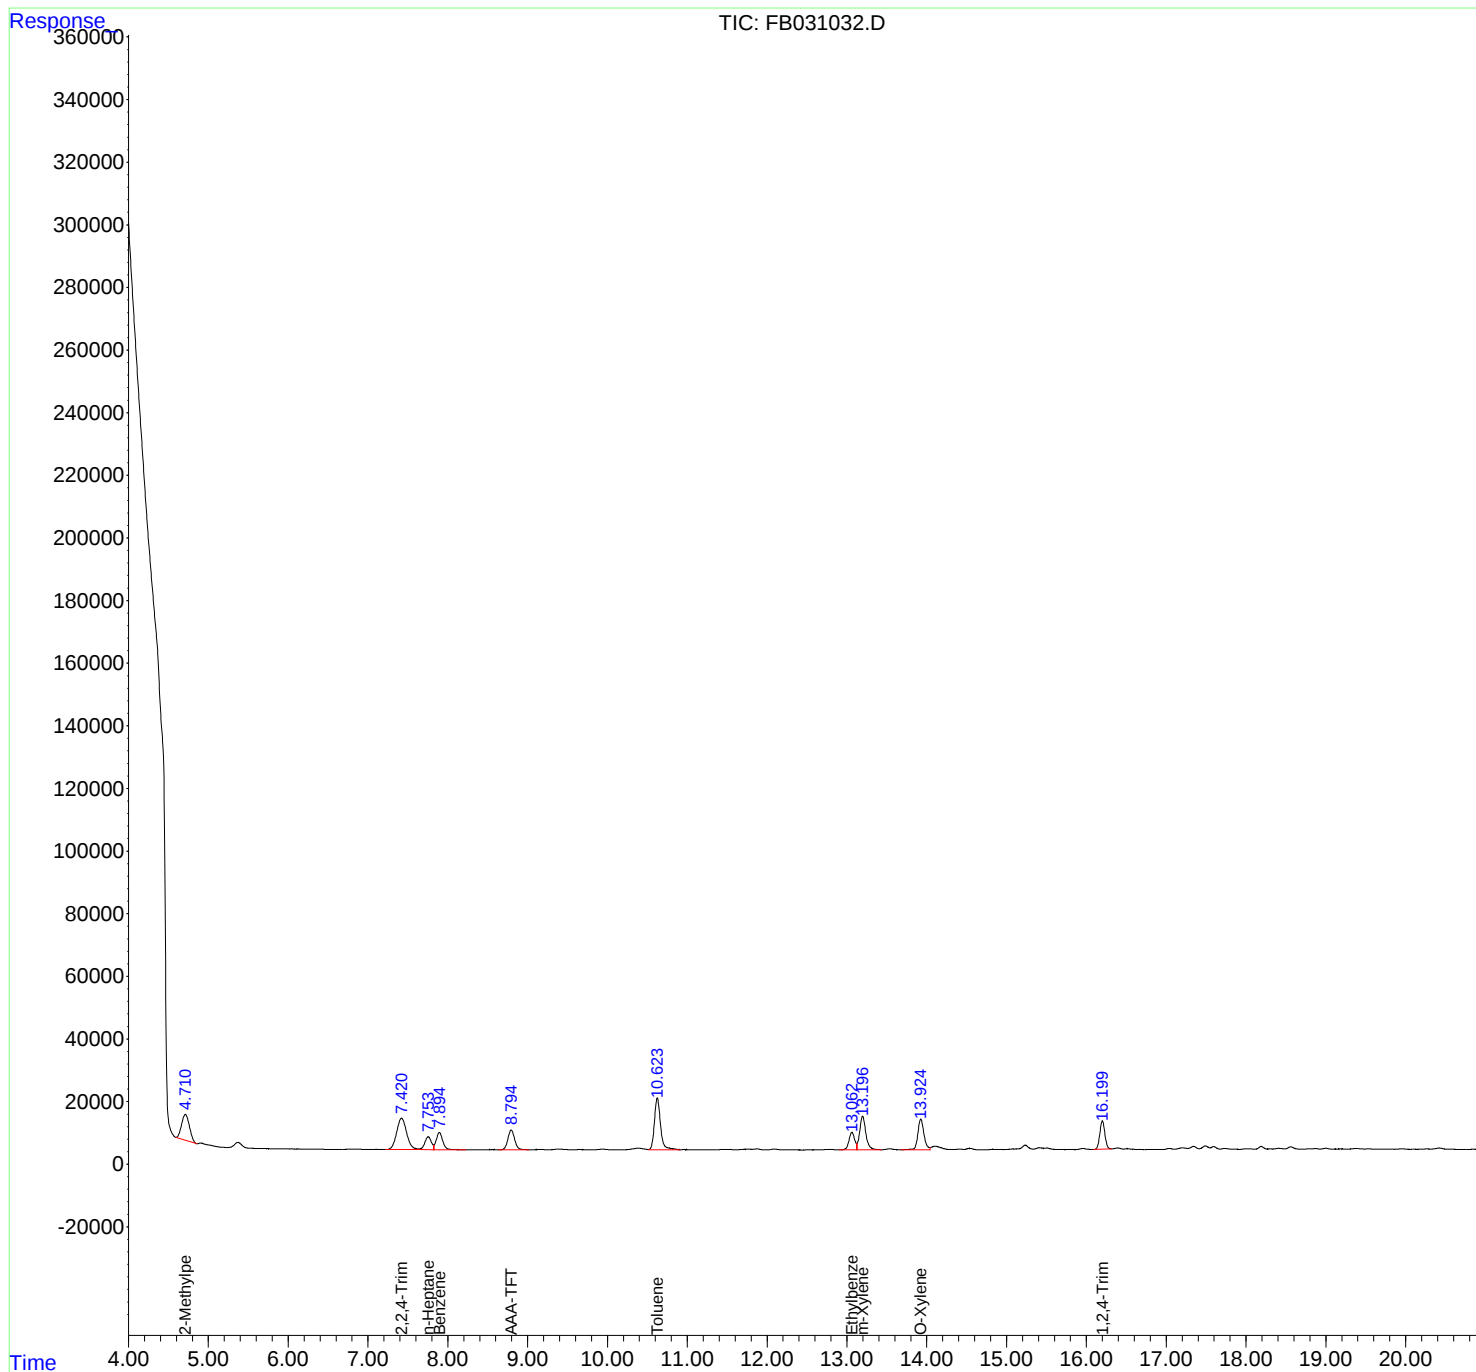

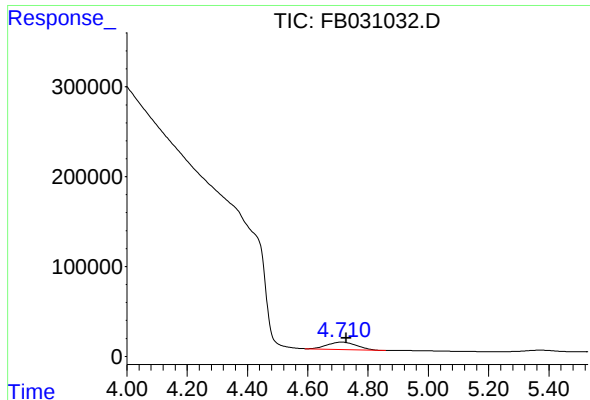


#1 2-Methylpentane

R.T.: 4.712 min
Delta R.T.: -0.016 min
Response: 560345
Conc: 15.53 ng/ml

Instrument :


FID_B

ClientSampleId :

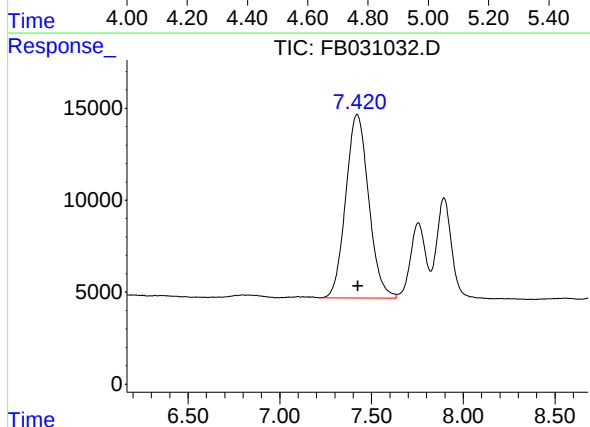


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.006 min
Response: 868135
Conc: 18.22 ng/ml

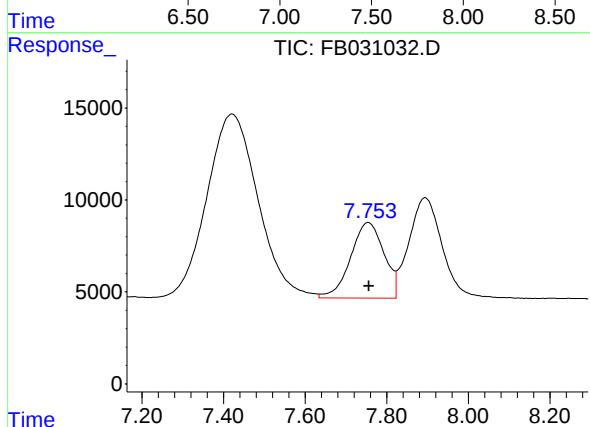


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.002 min
Response: 233599
Conc: 5.18 ng/ml

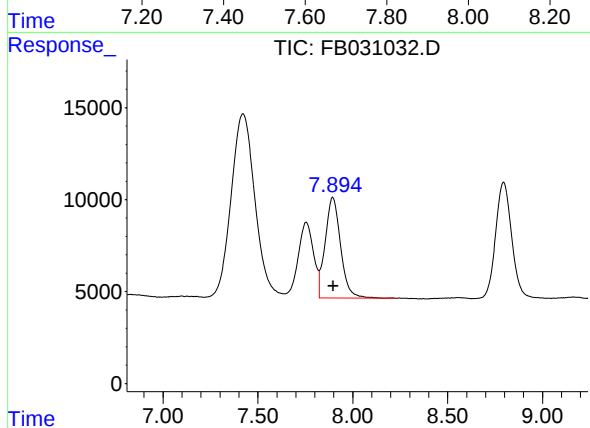

#4 Benzene


R.T.: 7.895 min
Delta R.T.: -0.003 min
Response: 311336
Conc: 5.66 ng/ml

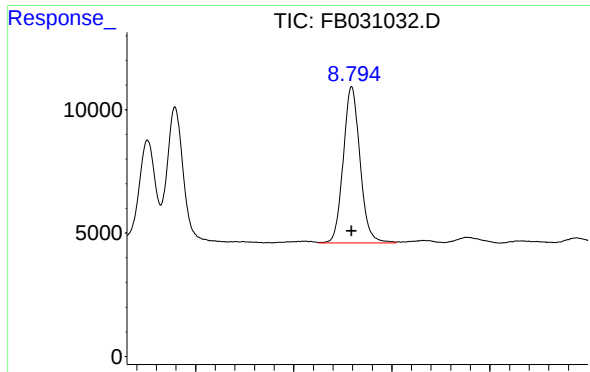

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 377061
Conc: 12.58 ng/ml

Instrument :
FID_B
ClientSampleId :

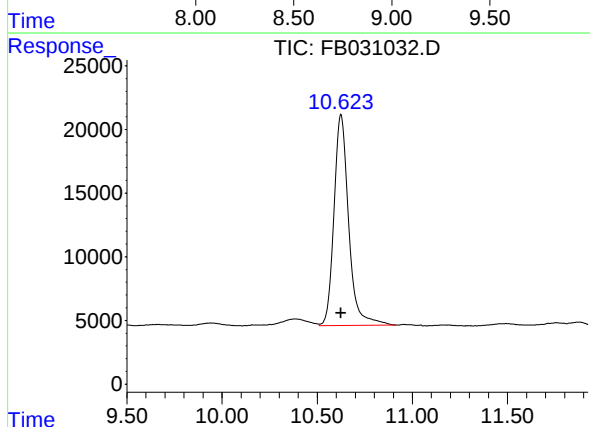


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.000 min
Response: 880590
Conc: 16.30 ng/ml

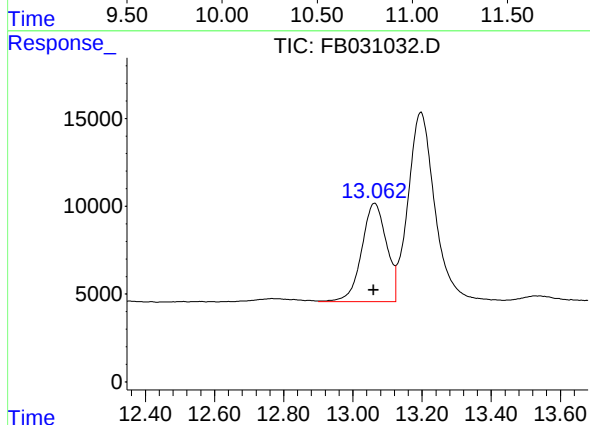


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.003 min
Response: 278950
Conc: 5.88 ng/ml

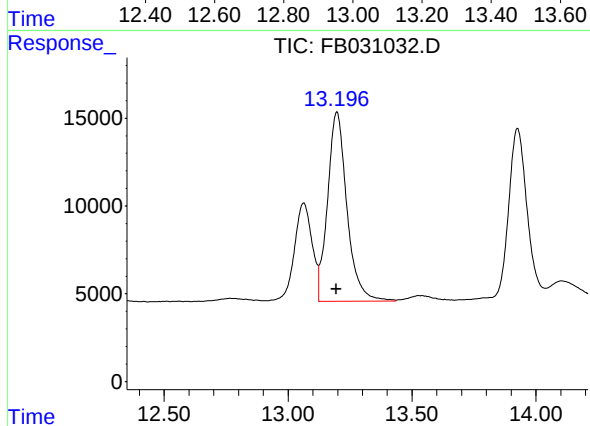

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 584751
Conc: 11.21 ng/ml

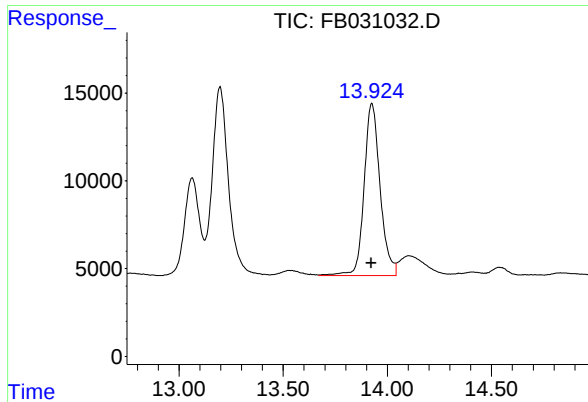

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.003 min
Response: 523379
Conc: 10.76 ng/ml

Instrument :
FID_B
ClientSampleId :

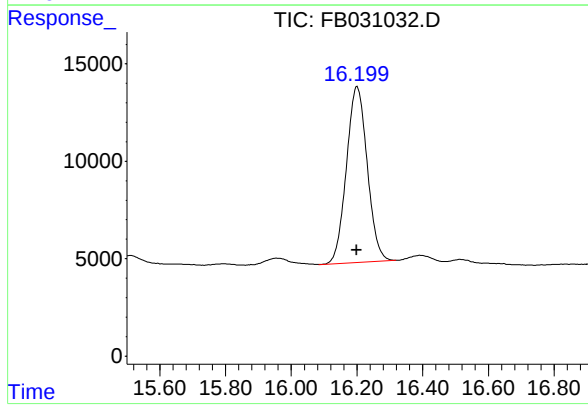

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.002 min
Response: 396462
Conc: 12.10 ng/ml