

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031014.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 10:27
 Operator : YP/AJ
 Sample : BSF1024S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1024S1

Integration File: Calibration.e
 Quant Time: Oct 25 04:01:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	536309	17.890 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.723	1004543	27.838 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	1321043	27.722 ng/ml
3) t n-Heptane	7.756	390749	8.663 ng/ml
4) t Benzene	7.896	511559	9.307 ng/ml
6) t Toluene	10.623	1455395	26.942 ng/ml
7) t Ethylbenzene	13.060	432416	9.123 ng/ml
8) t m-Xylene	13.194	929014	17.808 ng/ml
9) t O-Xylene	13.922	870185	17.888 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	670215	20.453 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031014.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 10:27
Operator : YP/AJ
Sample : BSF1024S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1024S1

Integration File: Calibration.e
Quant Time: Oct 25 04:01:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

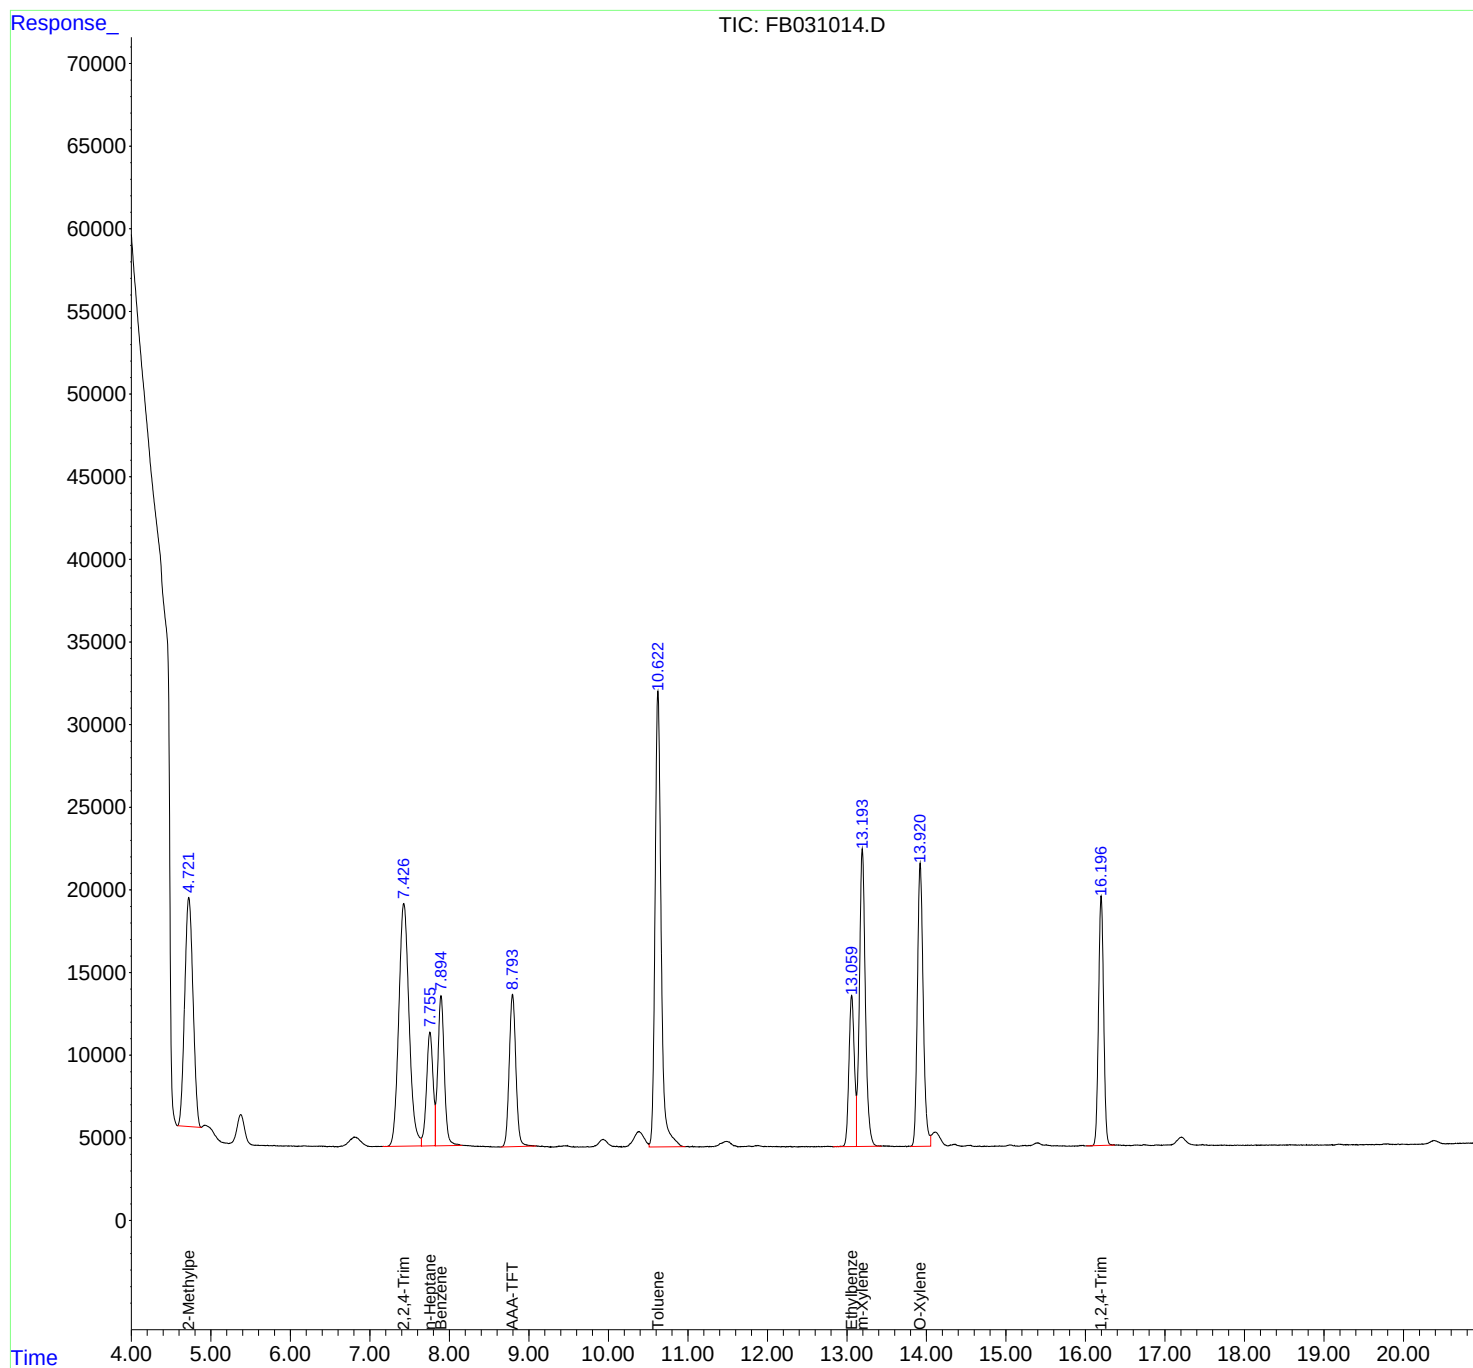


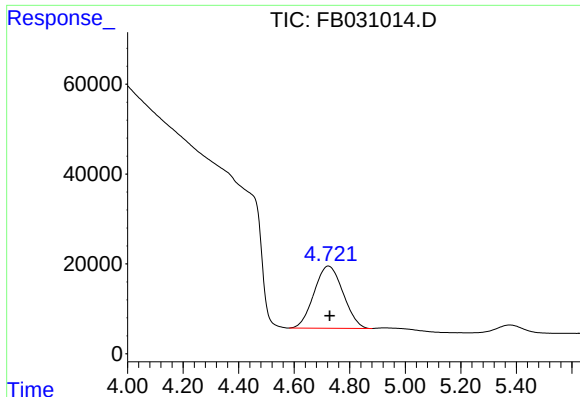

#1 2-Methylpentane


R.T.: 4.723 min
Delta R.T.: -0.005 min
Response: 1004543
Conc: 27.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S1

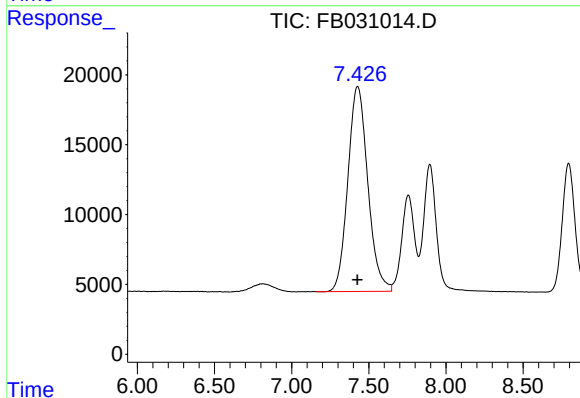


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: 0.000 min
Response: 1321043
Conc: 27.72 ng/ml

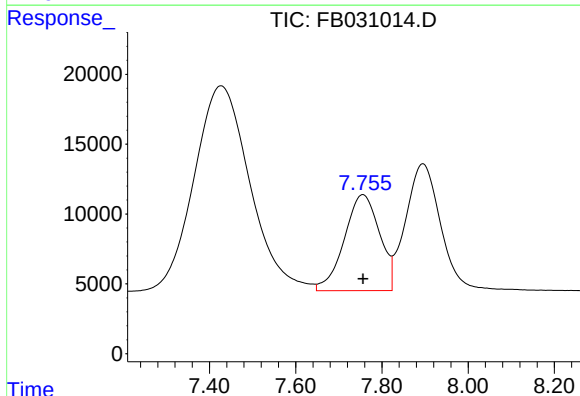


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 390749
Conc: 8.66 ng/ml

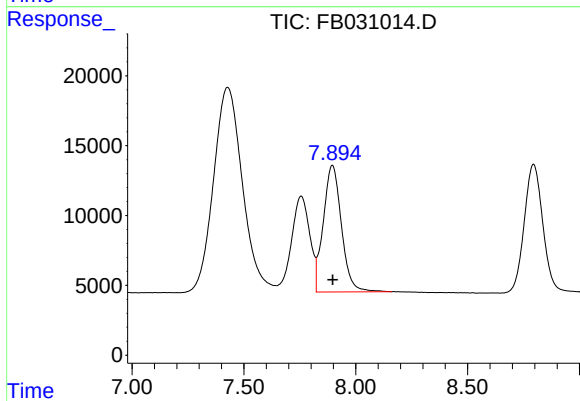

#4 Benzene


R.T.: 7.896 min
Delta R.T.: -0.002 min
Response: 511559
Conc: 9.31 ng/ml

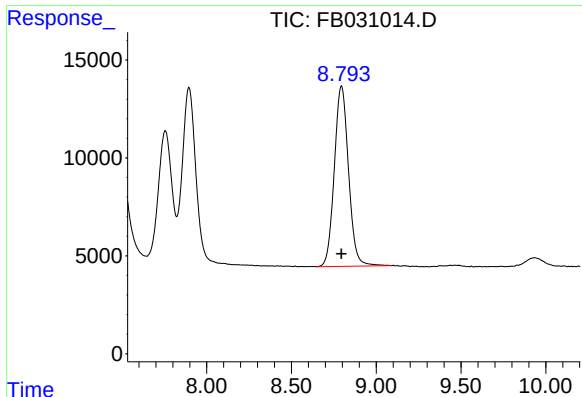

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 536309
Conc: 17.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S1

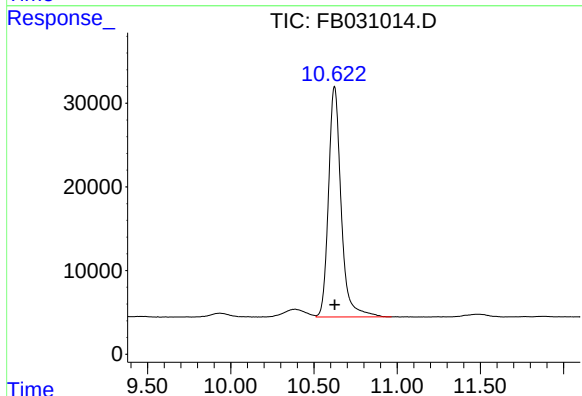


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.001 min
Response: 1455395
Conc: 26.94 ng/ml

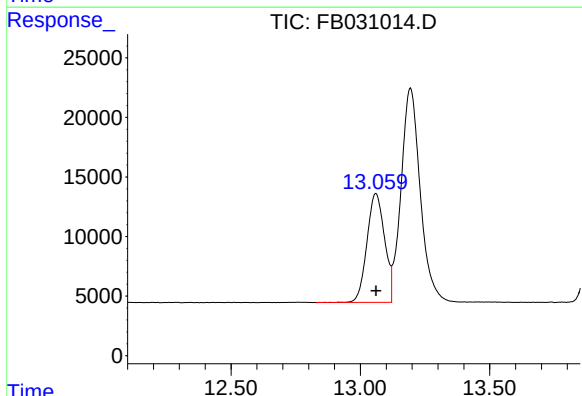


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.000 min
Response: 432416
Conc: 9.12 ng/ml

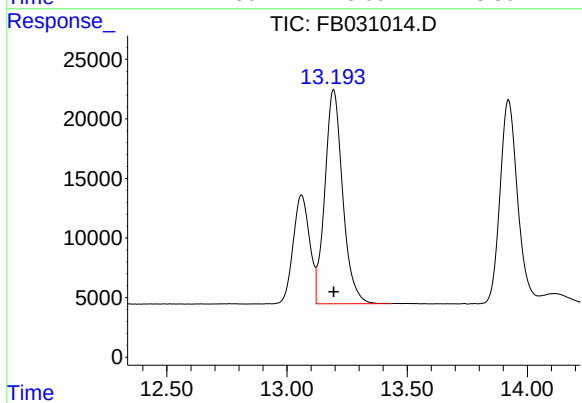

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.001 min
Response: 929014
Conc: 17.81 ng/ml

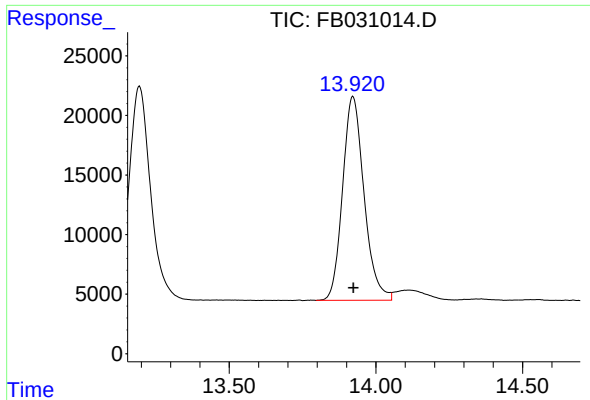

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.001 min
Response: 870185
Conc: 17.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S1

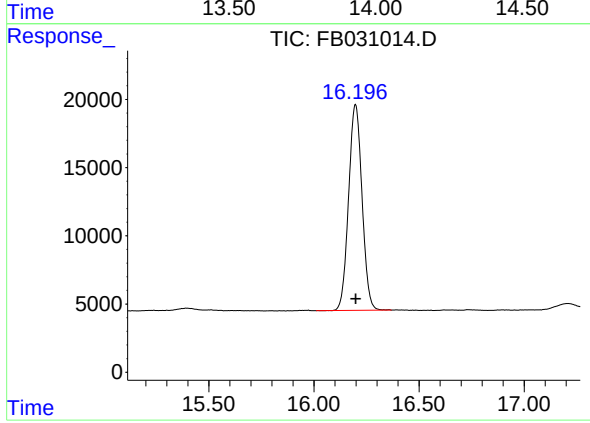

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 670215
Conc: 20.45 ng/ml