

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
 Data File : FB031033.D
 Signal(s) : FID2B.CH
 Acq On : 24 Oct 2024 19:34
 Operator : YP/AJ
 Sample : BSF1024S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1024S3

Integration File: Calibration.e
 Quant Time: Oct 25 04:03:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	637615	21.270 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.722	960140	26.608 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	1296647	27.210 ng/ml
3) t n-Heptane	7.756	383828	8.510 ng/ml
4) t Benzene	7.896	507467	9.233 ng/ml
6) t Toluene	10.624	1429200	26.457 ng/ml
7) t Ethylbenzene	13.061	436167	9.202 ng/ml
8) t m-Xylene	13.195	930699	17.840 ng/ml
9) t O-Xylene	13.922	864924	17.780 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	678982	20.721 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102424\
Data File : FB031033.D
Signal(s) : FID2B.CH
Acq On : 24 Oct 2024 19:34
Operator : YP/AJ
Sample : BSF1024S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1024S3

Integration File: Calibration.e
Quant Time: Oct 25 04:03:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

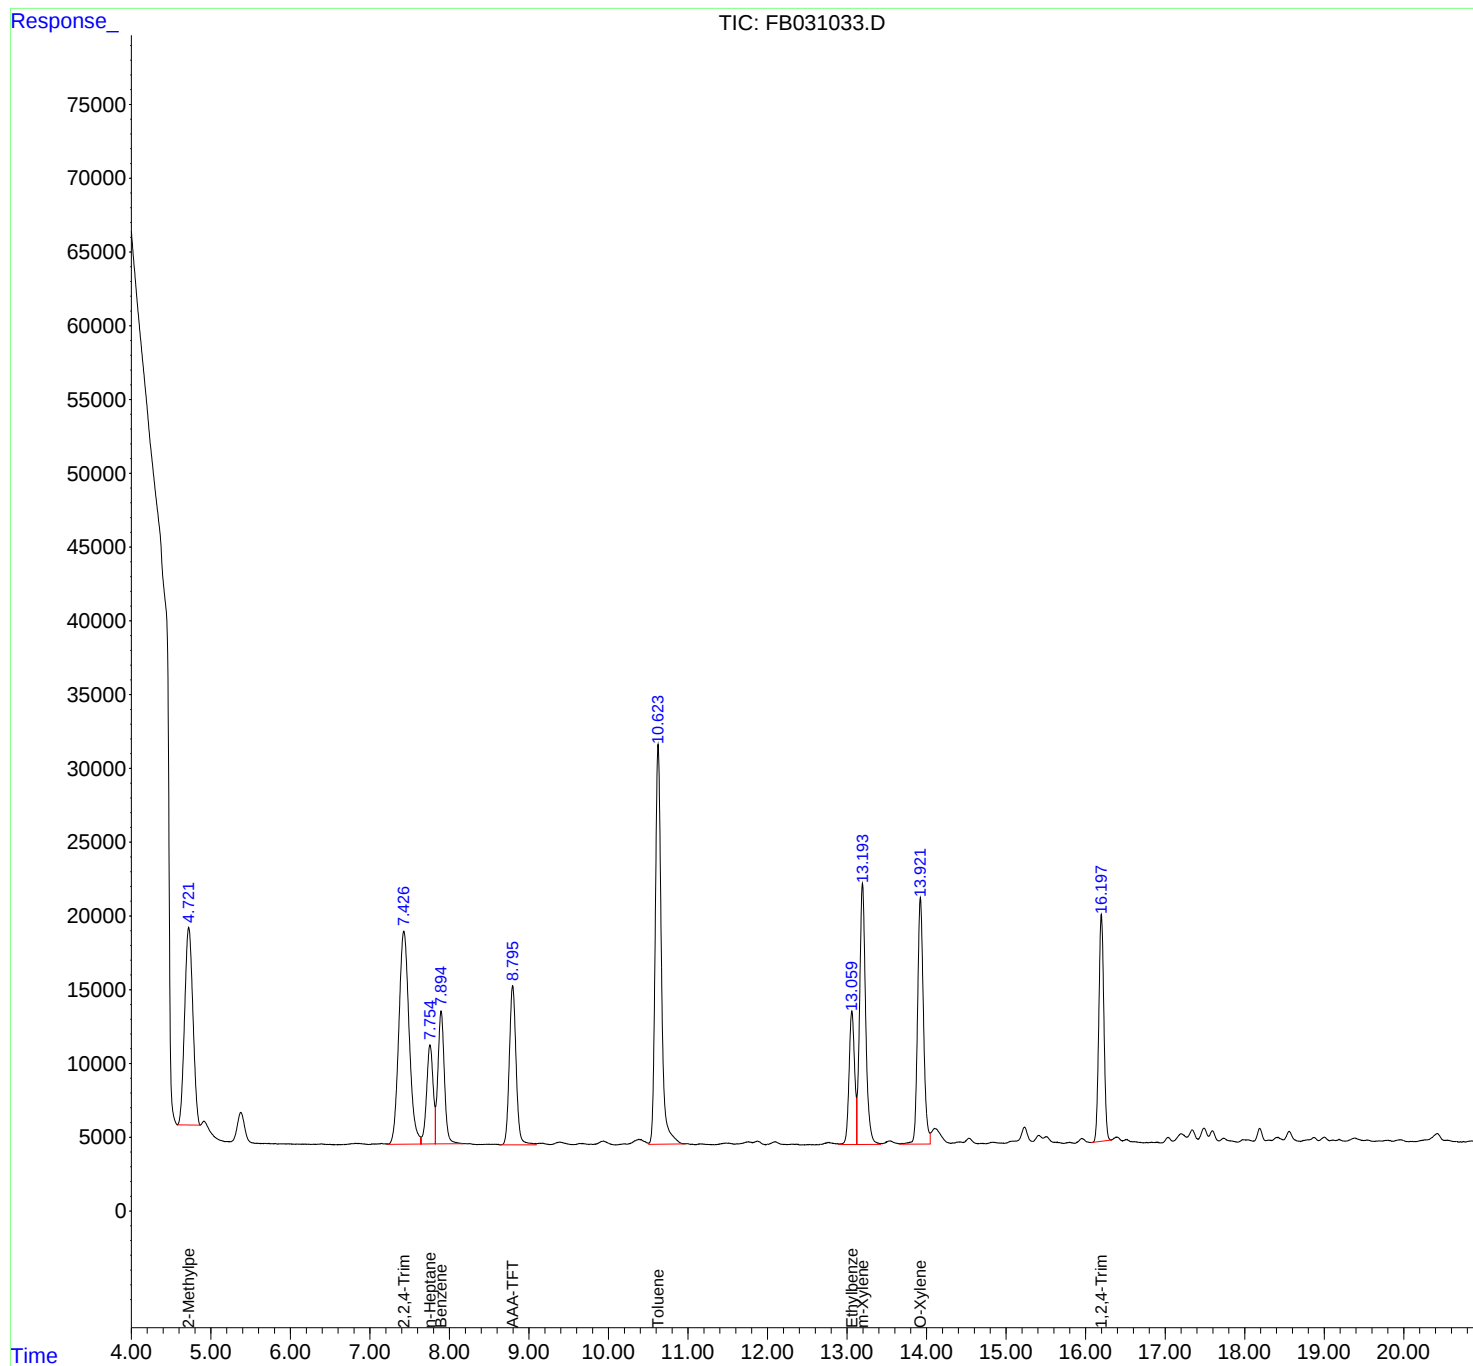


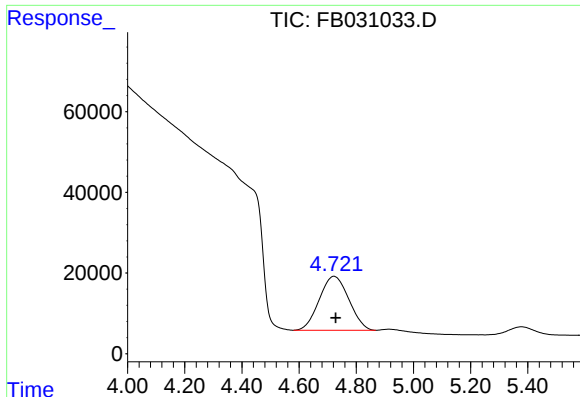

#1 2-Methylpentane


R.T.: 4.722 min
Delta R.T.: -0.006 min
Response: 960140
Conc: 26.61 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S3

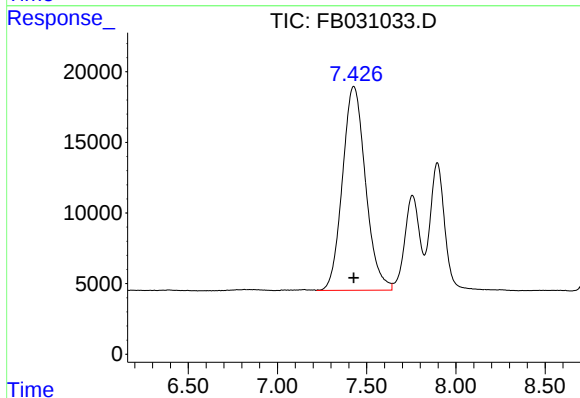


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.000 min
Response: 1296647
Conc: 27.21 ng/ml

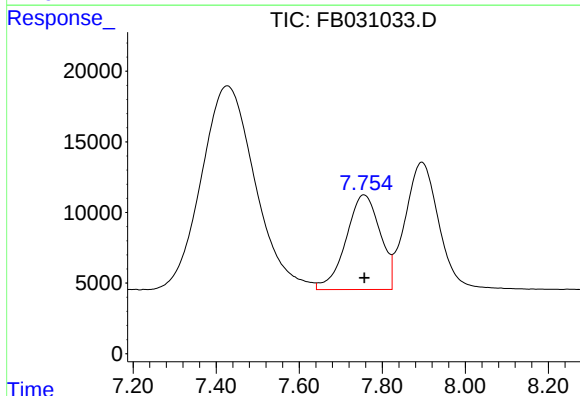


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 383828
Conc: 8.51 ng/ml

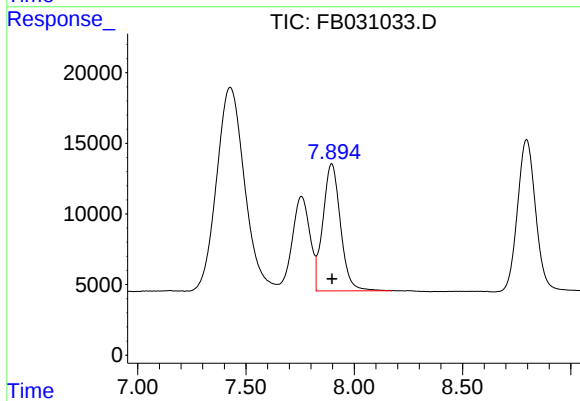

#4 Benzene


R.T.: 7.896 min
Delta R.T.: -0.002 min
Response: 507467
Conc: 9.23 ng/ml

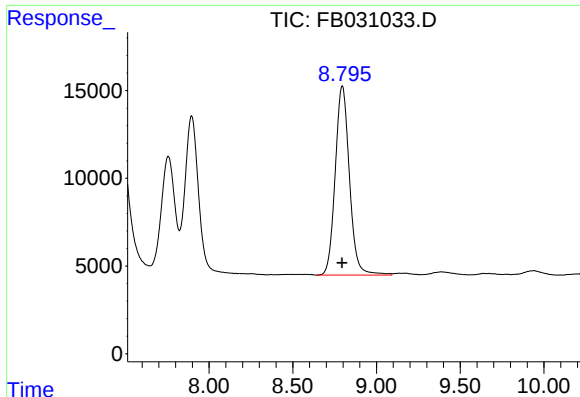

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 637615
Conc: 21.27 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S3

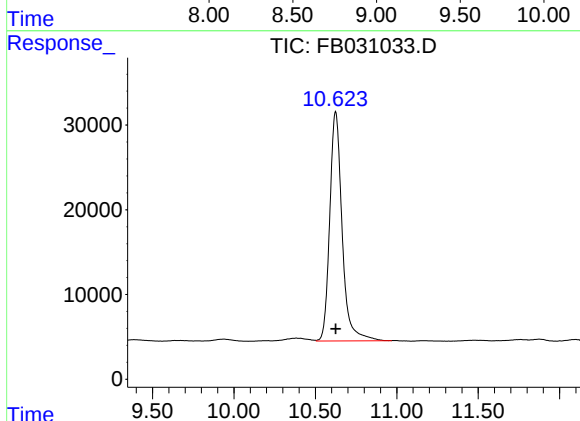


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 1429200
Conc: 26.46 ng/ml

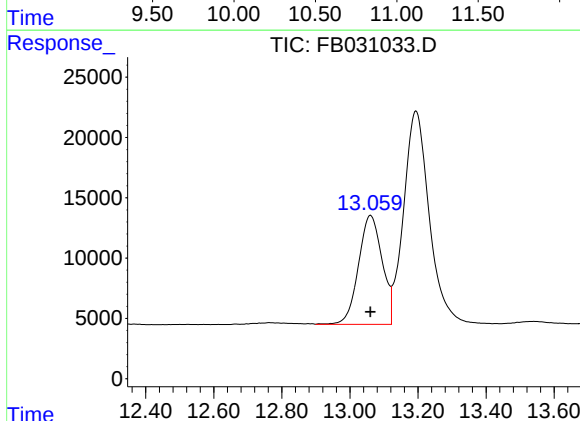


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.000 min
Response: 436167
Conc: 9.20 ng/ml

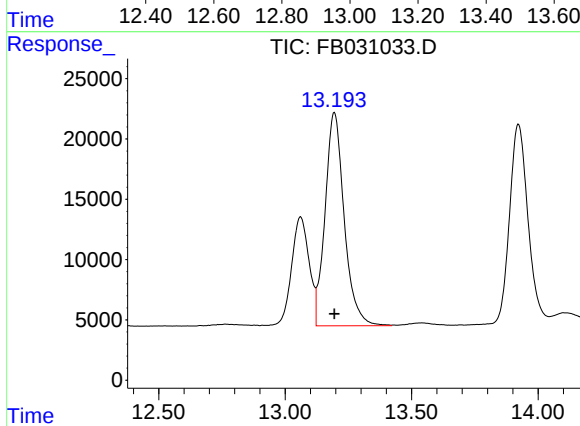

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.000 min
Response: 930699
Conc: 17.84 ng/ml

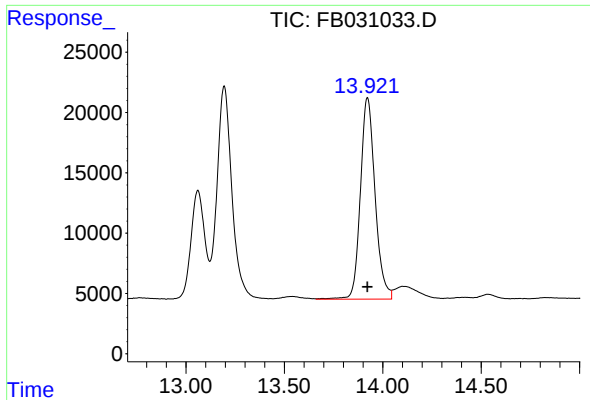

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.000 min
Response: 864924
Conc: 17.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1024S3

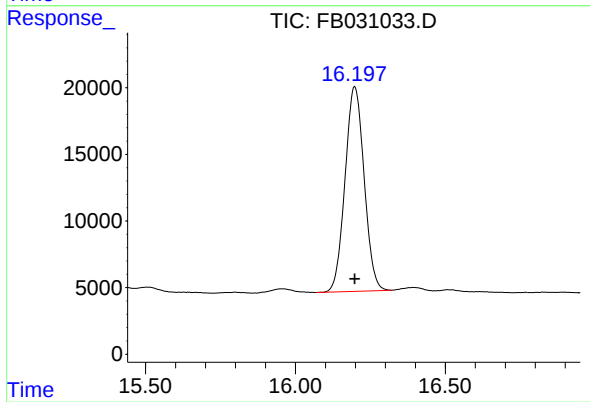

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 678982
Conc: 20.72 ng/ml