

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102519\
Data File : FB022830.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2019 14:26
Operator : DD/AJ
Sample : K5153-06
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 22:32:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	543702	21.487 ng/ml
Target Compounds			
6) t Toluene	10.624	4954	0.115 ng/ml
8) t m-Xylene	13.204	3025	0.079 ng/ml
9) t O-Xylene	13.914	2520	0.069 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	4517	0.159 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102519\
Data File : FB022830.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2019 14:26
Operator : DD/AJ
Sample : K5153-06
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 22:32:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

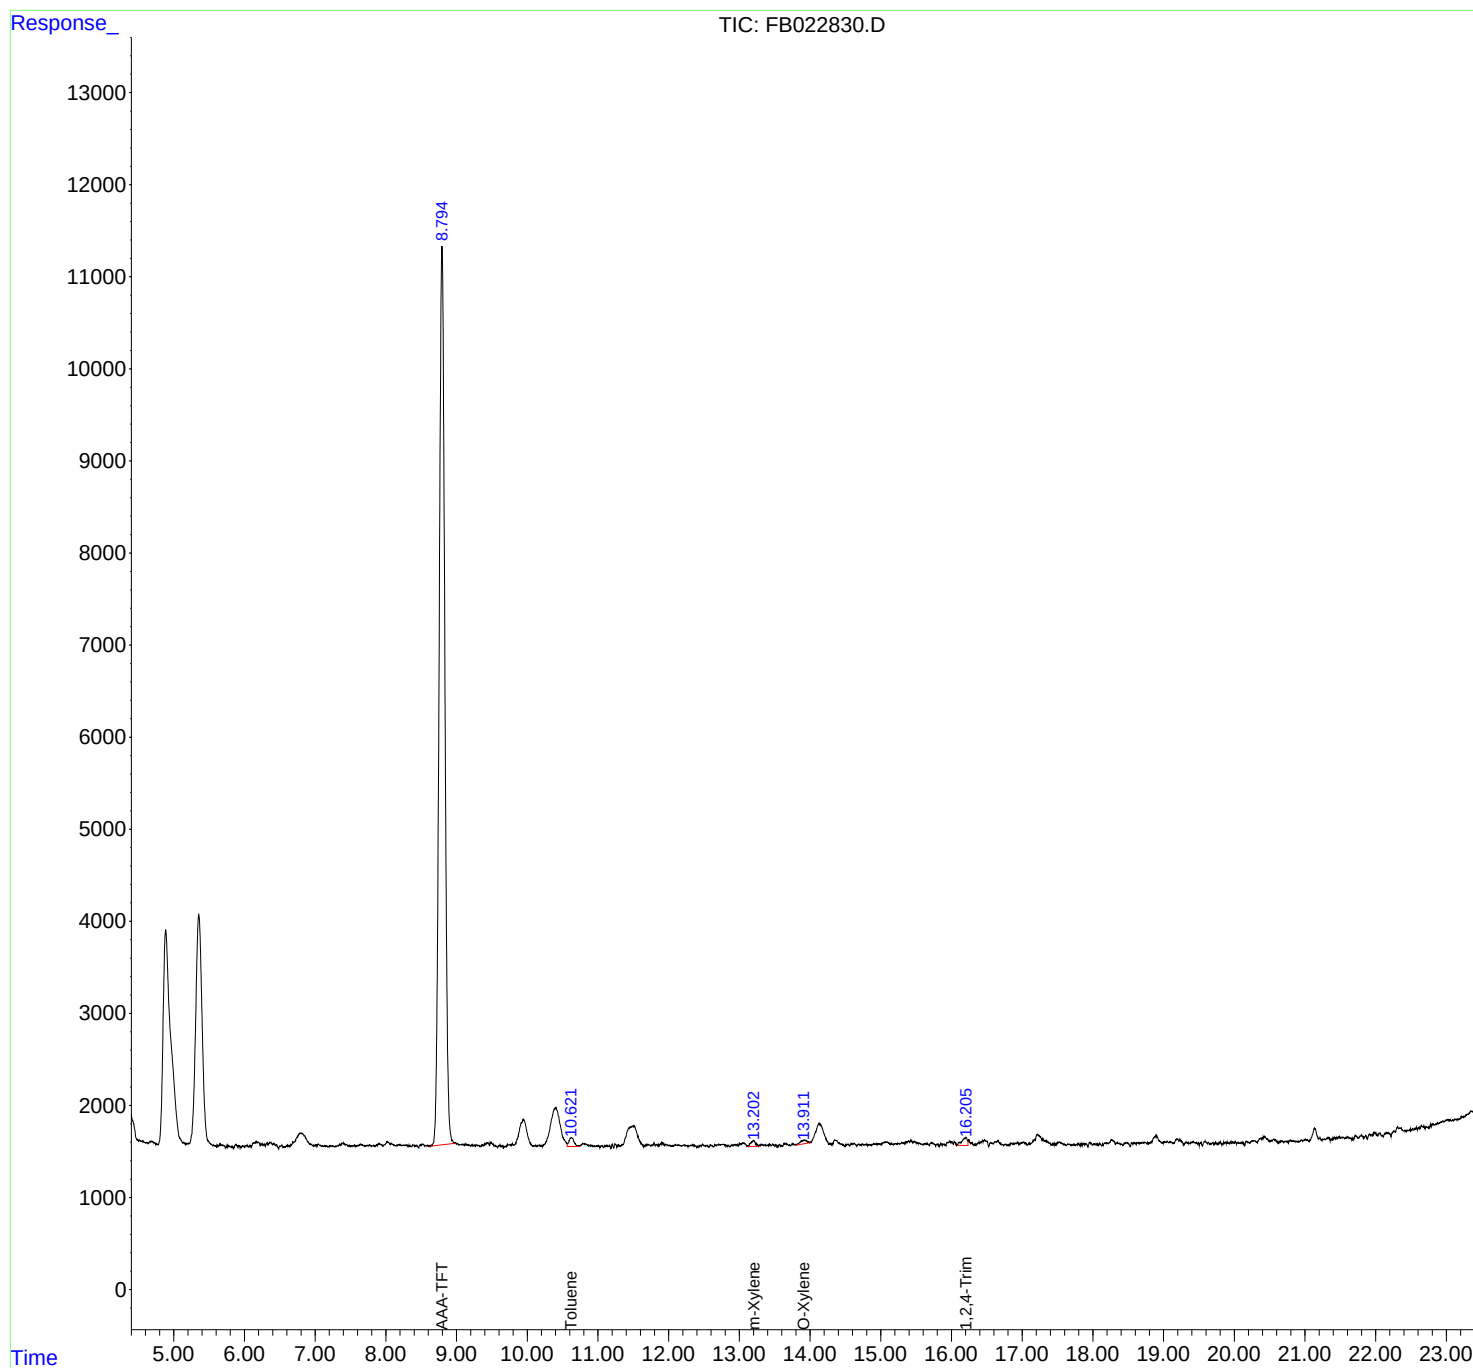

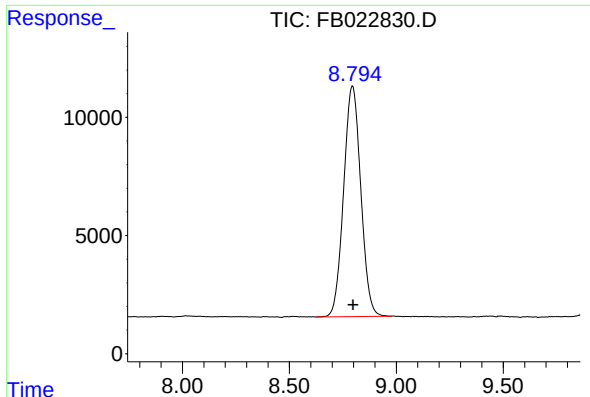


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 543702
Conc: 21.49 ng/ml

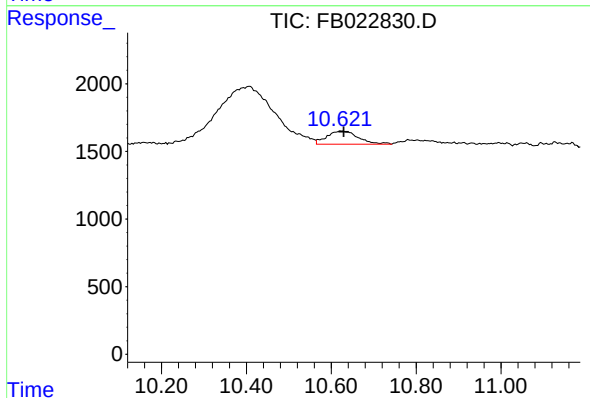


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.005 min
Response: 4954
Conc: 0.11 ng/ml

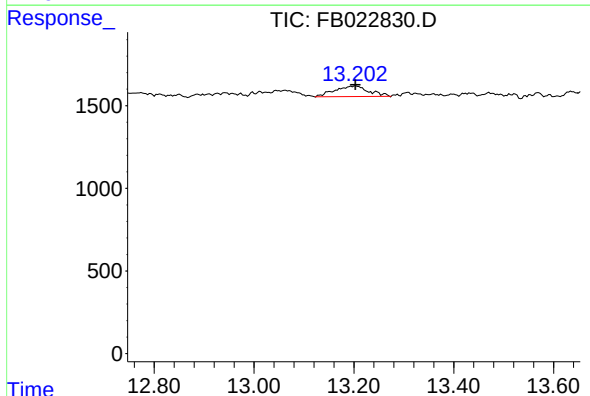


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.001 min
Response: 3025
Conc: 0.08 ng/ml

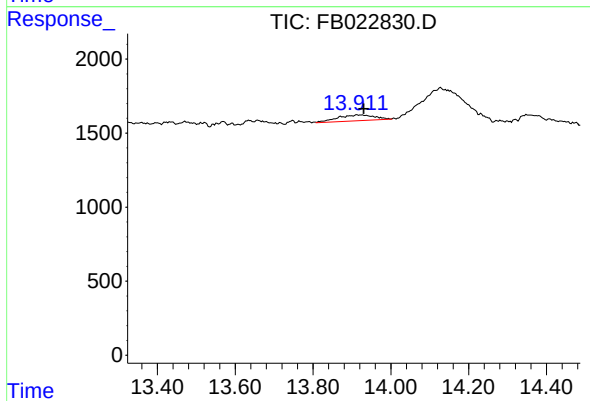

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.017 min
Response: 2520
Conc: 0.07 ng/ml

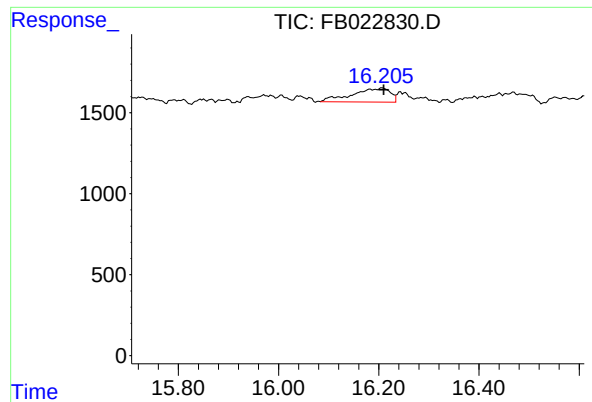

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 4517
Conc: 0.16 ng/ml