

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102519\
 Data File : FB022832.D
 Signal(s) : FID2B.CH
 Acq On : 25 Oct 2019 15:26
 Operator : DD/AJ
 Sample : K5153-06MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 25 22:33:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	527721	20.855 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	773085	22.748 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	636073	17.481 ng/ml
3) t n-Heptane	7.756	208326	5.710 ng/ml
4) t Benzene	7.890	393907	8.922 ng/ml
6) t Toluene	10.628	1126921	26.146 ng/ml
7) t Ethylbenzene	13.068	336805	8.293 ng/ml
8) t m-Xylene	13.201	627502	16.309 ng/ml
9) t O-Xylene	13.929	605062	16.613 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	446451	15.667 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102519\
Data File : FB022832.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2019 15:26
Operator : DD/AJ
Sample : K5153-06MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 22:33:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

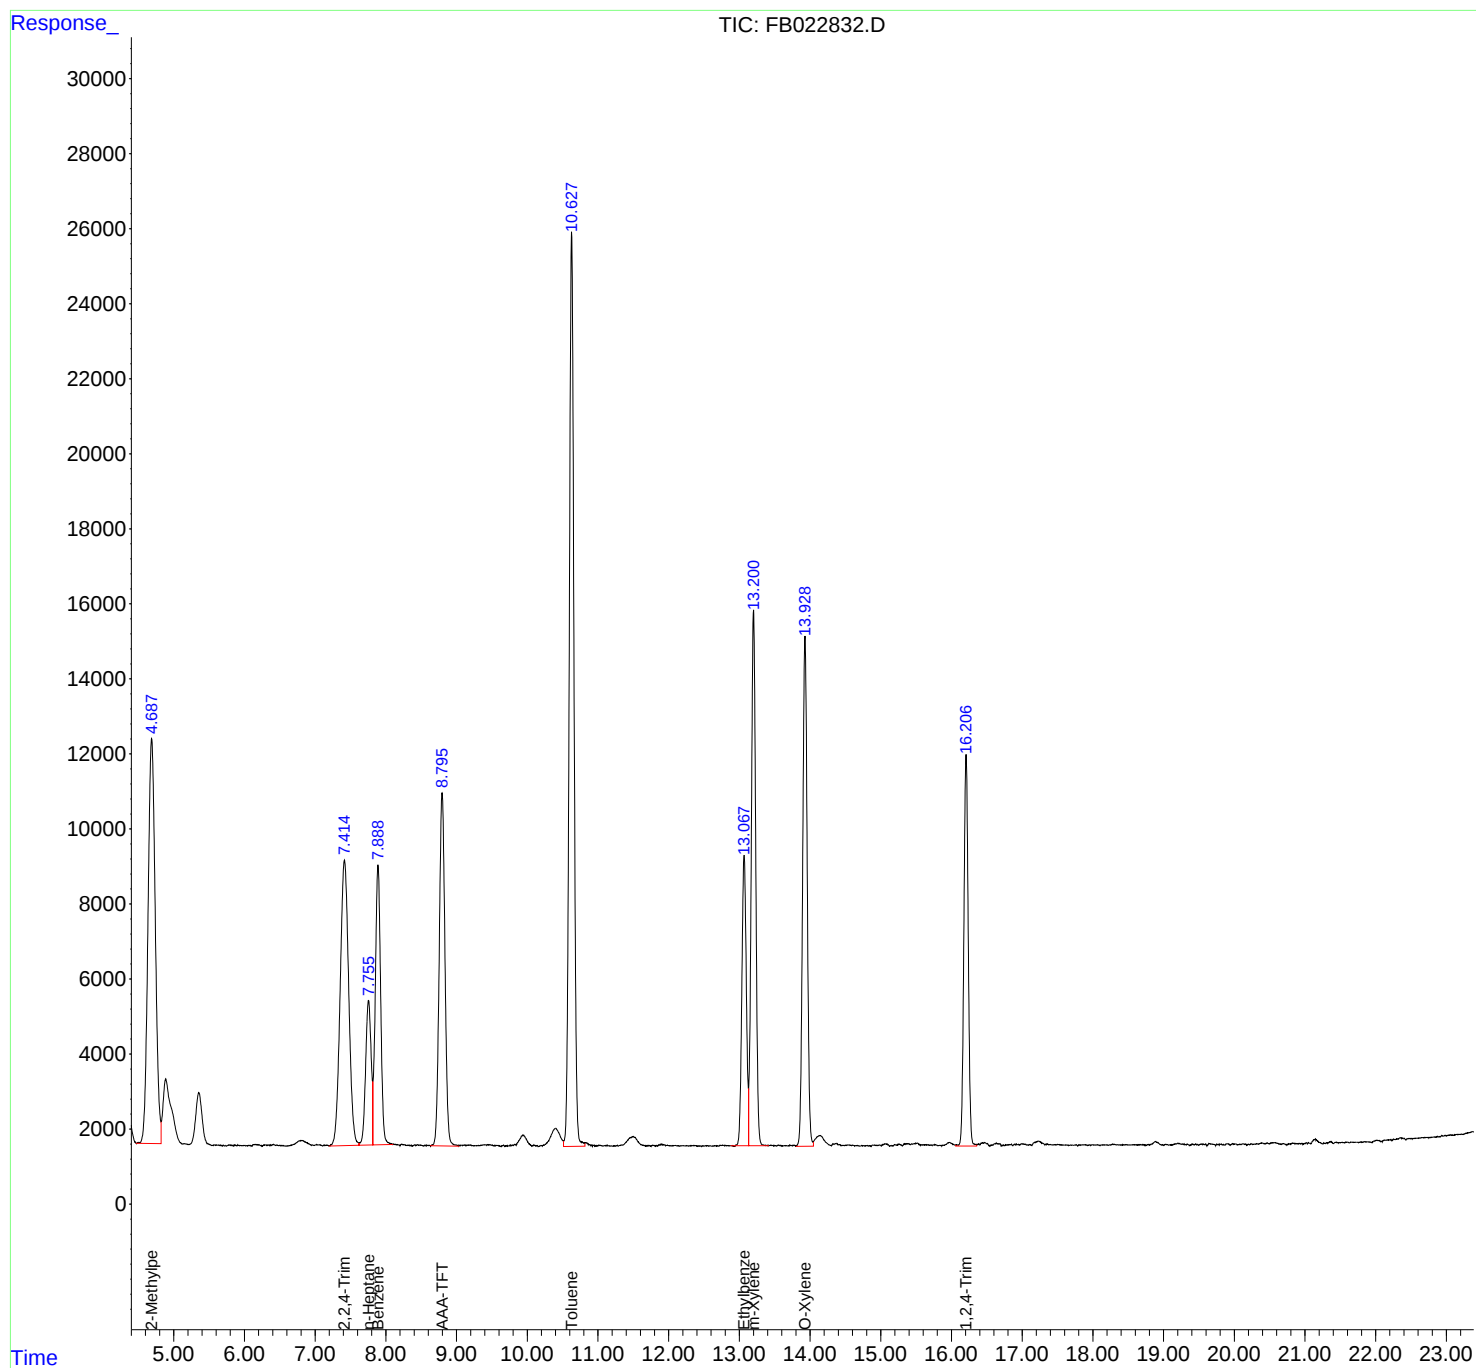

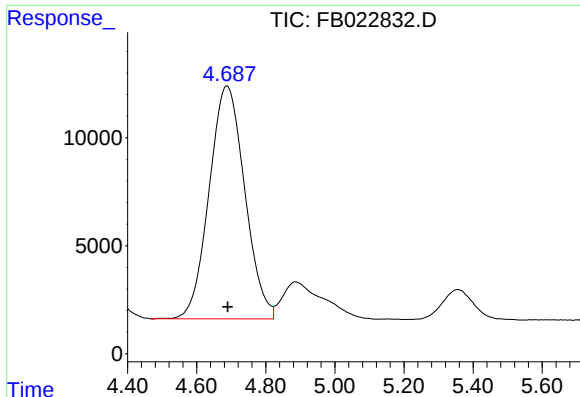


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 773085
Conc: 22.75 ng/ml

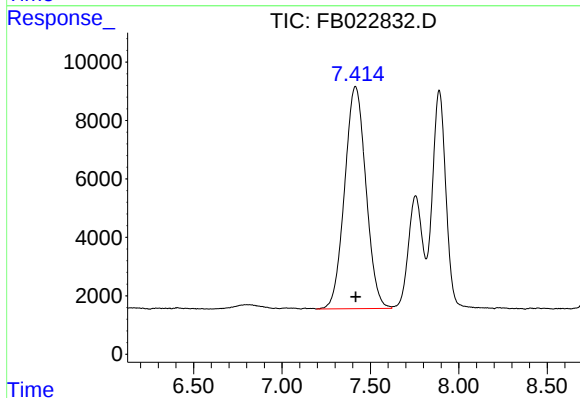


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 636073
Conc: 17.48 ng/ml

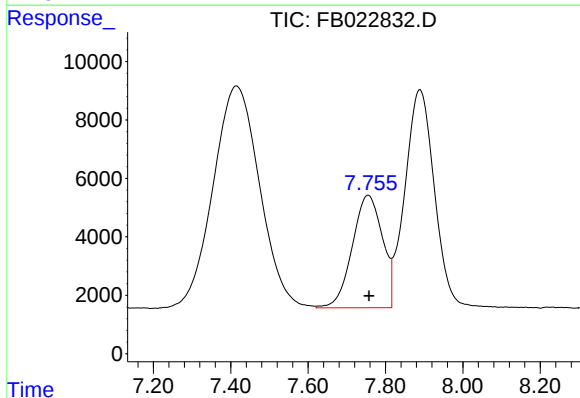


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.001 min
Response: 208326
Conc: 5.71 ng/ml

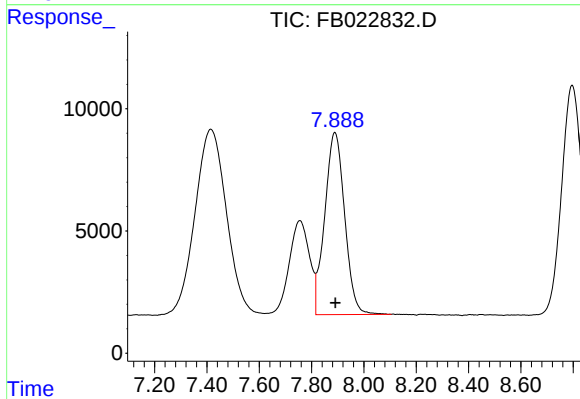


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 393907
Conc: 8.92 ng/ml

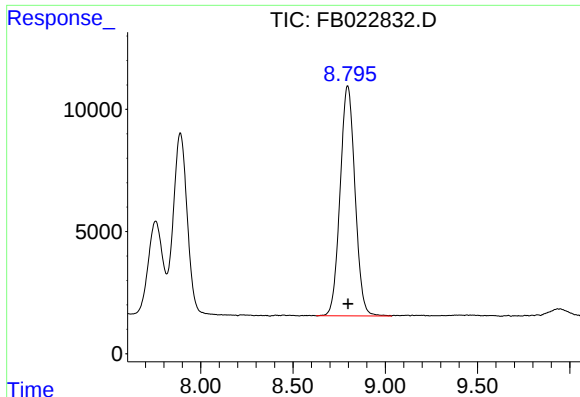


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.002 min
Response: 527721
Conc: 20.86 ng/ml

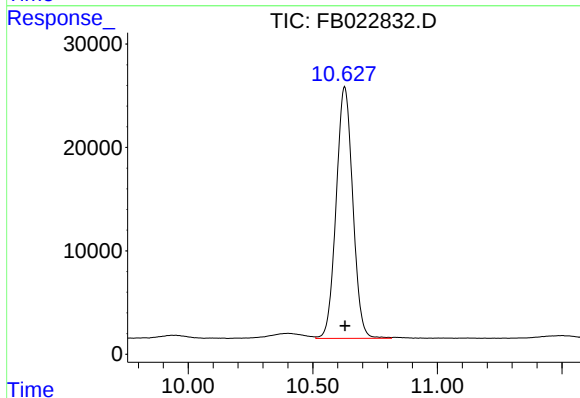


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.001 min
Response: 1126921
Conc: 26.15 ng/ml

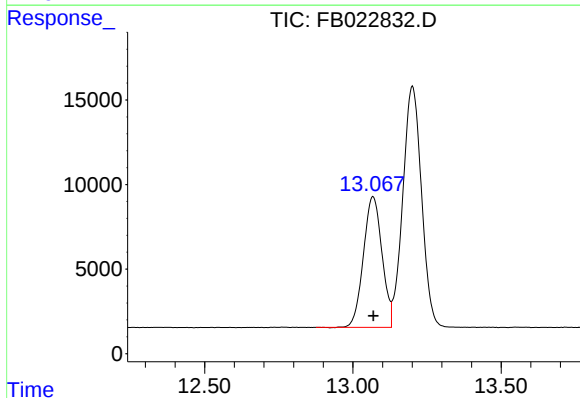


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 336805
Conc: 8.29 ng/ml

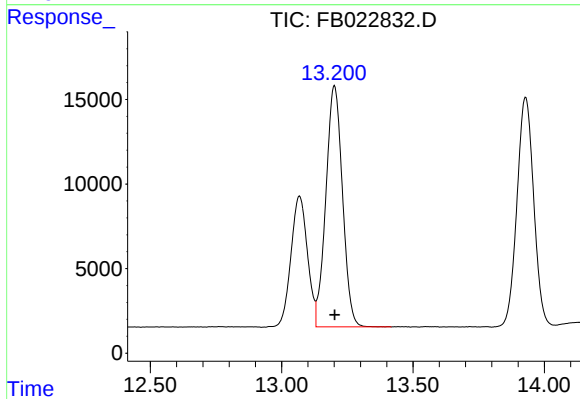


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 627502
Conc: 16.31 ng/ml

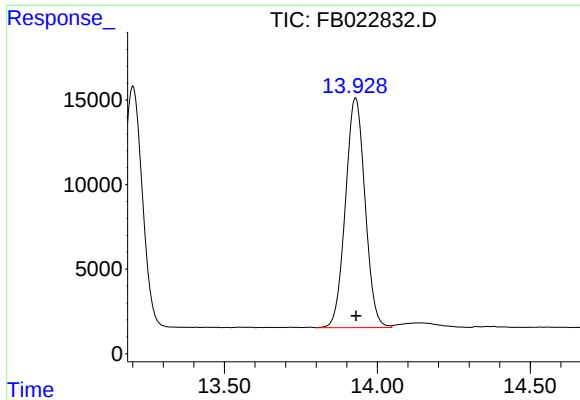

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 605062
Conc: 16.61 ng/ml

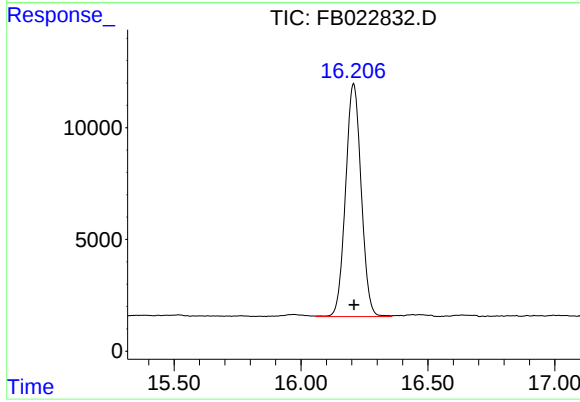

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 446451
Conc: 15.67 ng/ml