

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102519\
 Data File : FB022829.D
 Signal(s) : FID2B.CH
 Acq On : 25 Oct 2019 12:02
 Operator : DD/AJ
 Sample : BSF1025S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 25 22:32:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	502678	19.865 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	944242	27.784 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	1061100	29.161 ng/ml
3) t n-Heptane	7.754	345082	9.458 ng/ml
4) t Benzene	7.888	418263	9.473 ng/ml
6) t Toluene	10.626	1235822	28.673 ng/ml
7) t Ethylbenzene	13.067	398367	9.808 ng/ml
8) t m-Xylene	13.200	757862	19.697 ng/ml
9) t O-Xylene	13.927	724117	19.881 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	573965	20.142 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102519\
Data File : FB022829.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2019 12:02
Operator : DD/AJ
Sample : BSF1025S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 25 22:32:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

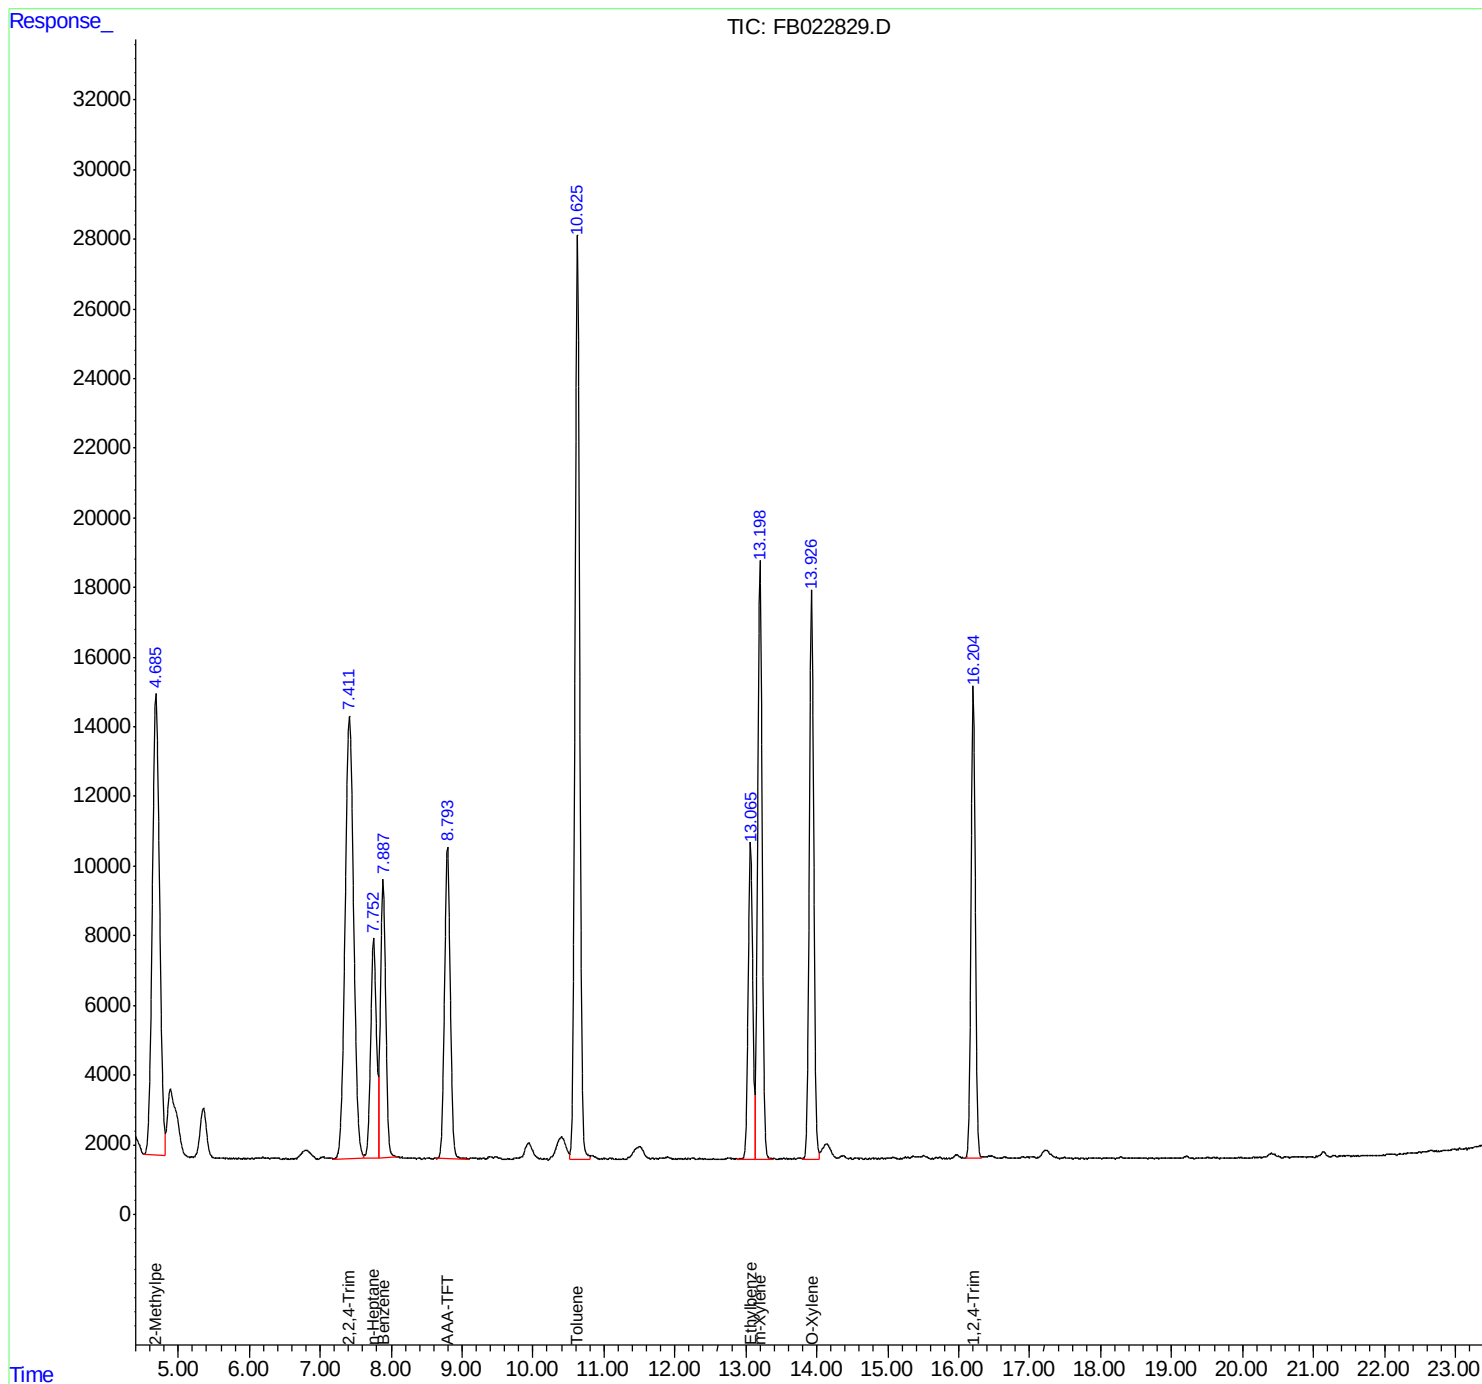

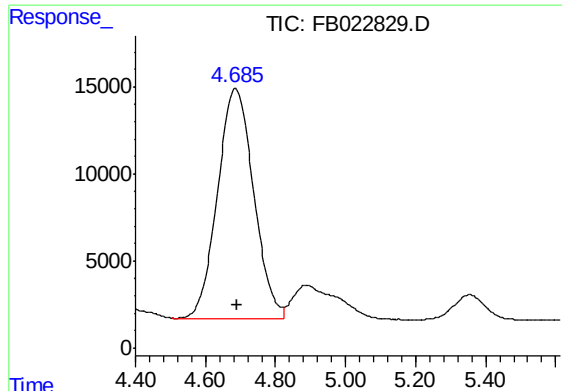


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.004 min
Response: 944242
Conc: 27.78 ng/ml

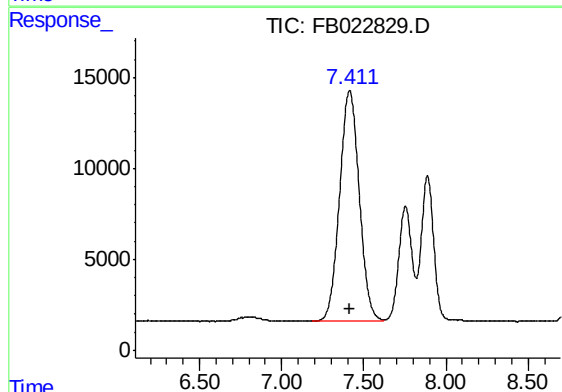


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.004 min
Response: 1061100
Conc: 29.16 ng/ml

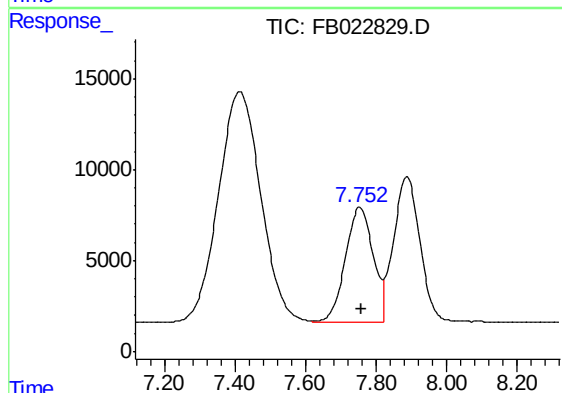


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.003 min
Response: 345082
Conc: 9.46 ng/ml

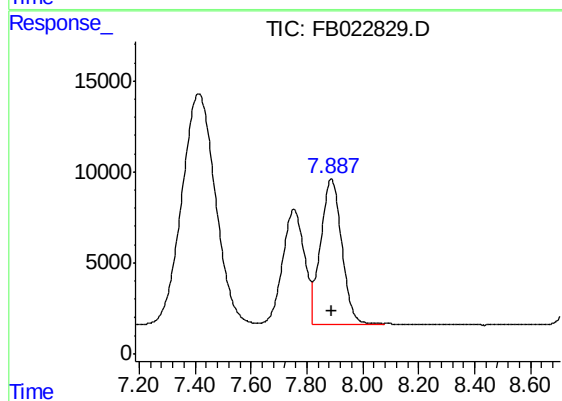


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.003 min
Response: 418263
Conc: 9.47 ng/ml

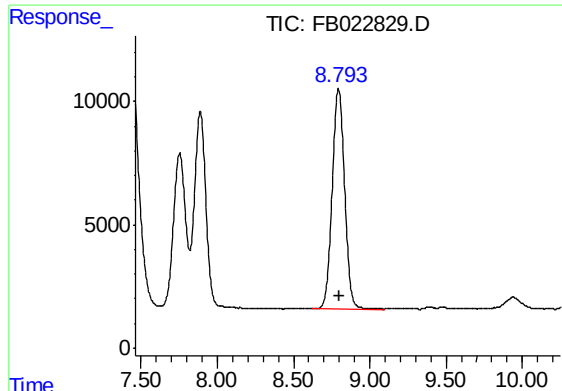


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 502678
Conc: 19.87 ng/ml

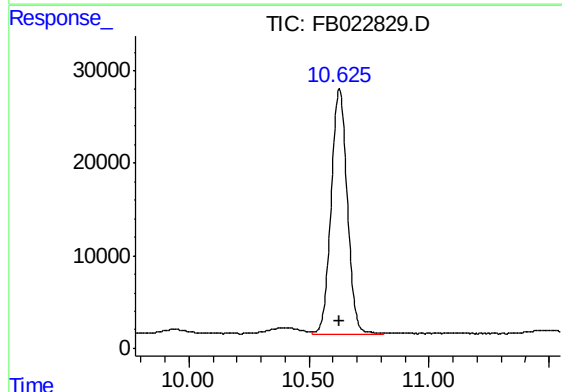


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.003 min
Response: 1235822
Conc: 28.67 ng/ml

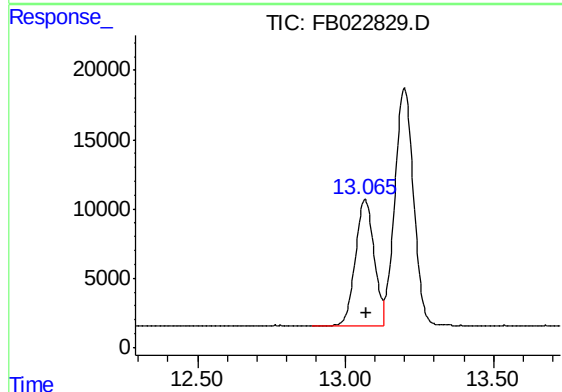


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.003 min
Response: 398367
Conc: 9.81 ng/ml

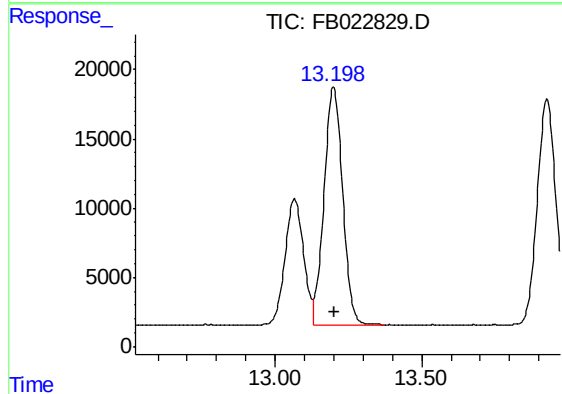


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 757862
Conc: 19.70 ng/ml

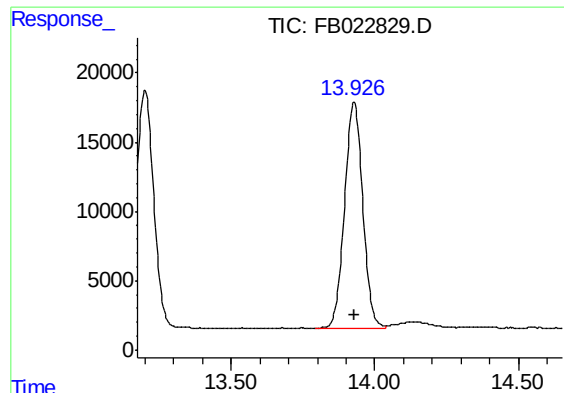

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.003 min
Response: 724117
Conc: 19.88 ng/ml

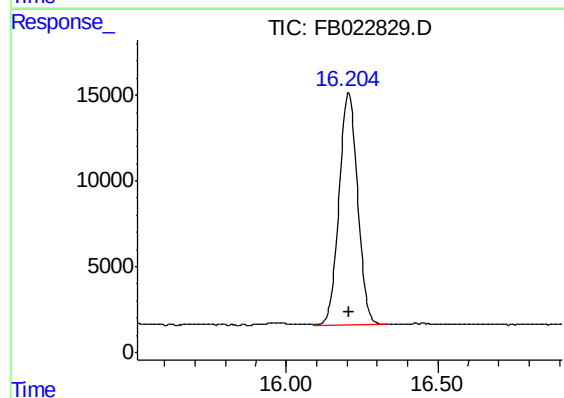

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.004 min
Response: 573965
Conc: 20.14 ng/ml