

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
Data File : FB028763.D
Signal(s) : FID2B.CH
Acq On : 26 Oct 2022 13:02
Operator : AJ/MA
Sample : N5256-12 50X
Misc : 2.85G/5.00 ML MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 26 13:21:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	219903	16.998 ng/ml
Target Compounds			
9) t O-Xylene	13.984	1434	0.074 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
Data File : FB028763.D
Signal(s) : FID2B.CH
Acq On : 26 Oct 2022 13:02
Operator : AJ/MA
Sample : N5256-12 50X
Misc : 2.85G/5.00 ML MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 26 13:21:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

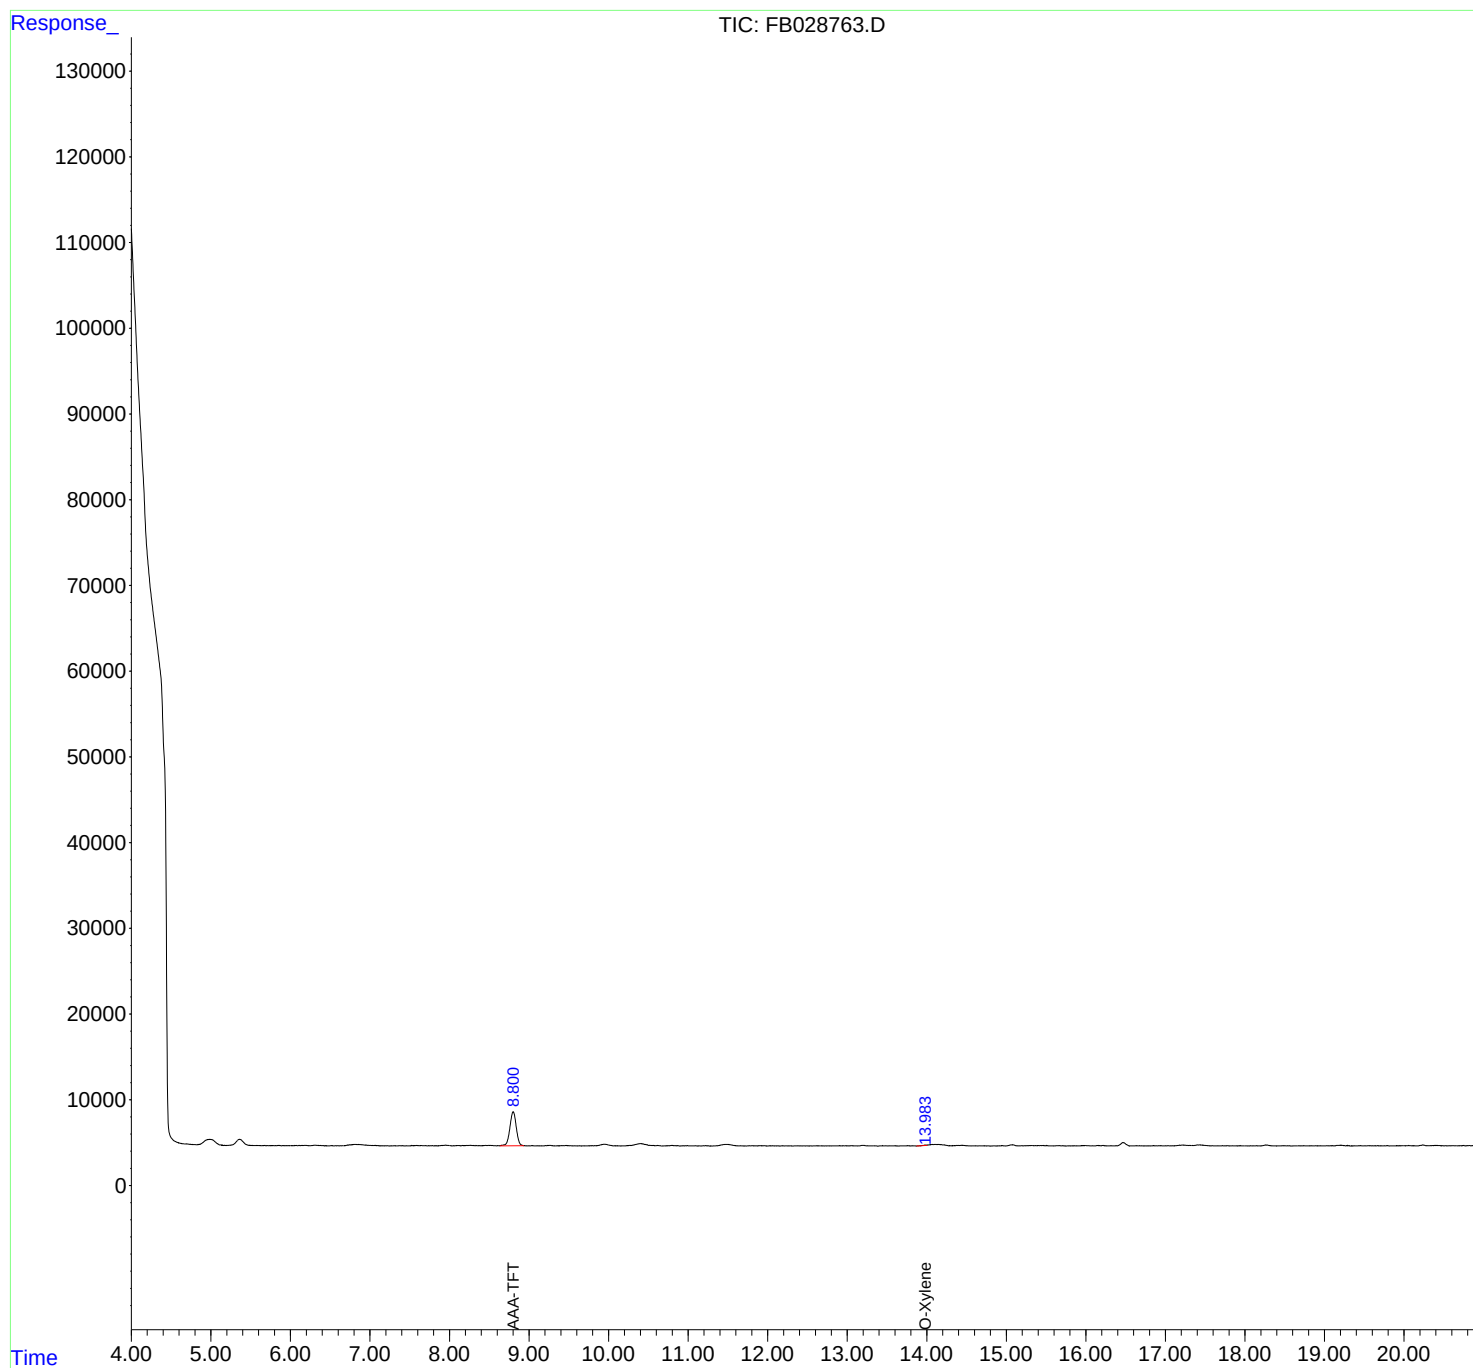

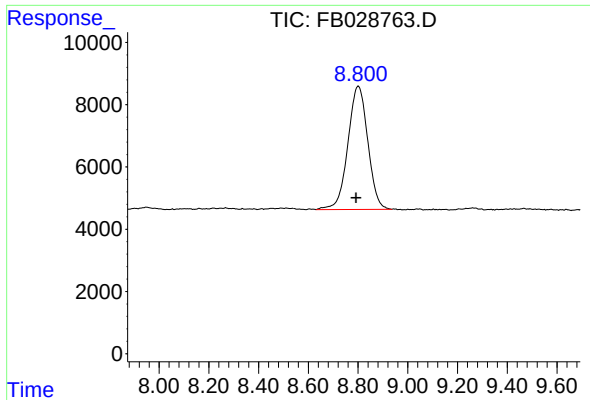


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.009 min
Response: 219903
Conc: 17.00 ng/ml

Instrument :

FID_B

ClientSampleId :

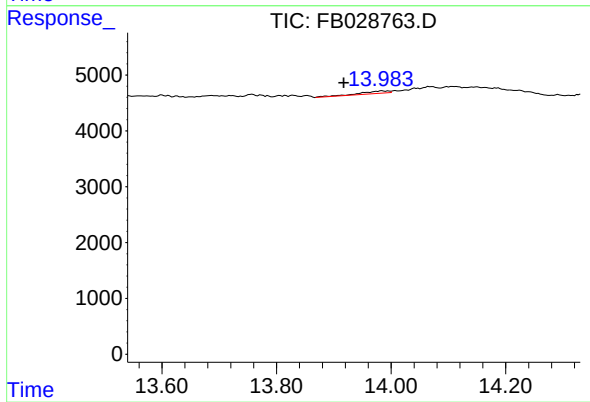

#9 O-Xylene

R.T.: 13.984 min
Delta R.T.: 0.067 min
Response: 1434
Conc: 0.07 ng/ml