

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
 Data File : FB028725.D
 Signal(s) : FID2B.CH
 Acq On : 25 Oct 2022 10:51
 Operator : AJ/MA
 Sample : BSF1025S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1025S1

Integration File: Calibration.e
 Quant Time: Oct 26 05:36:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	229323	17.726 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	444450	27.169 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	530826	29.373 ng/ml
3) t n-Heptane	7.755	144225	8.515 ng/ml
4) t Benzene	7.892	190126	8.656 ng/ml
6) t Toluene	10.625	541480	25.834 ng/ml
7) t Ethylbenzene	13.060	177583	8.948 ng/ml
8) t m-Xylene	13.193	358388	18.191 ng/ml
9) t O-Xylene	13.920	363594	18.689 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	382880	19.778 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
Data File : FB028725.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2022 10:51
Operator : AJ/MA
Sample : BSF1025S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1025S1

Integration File: Calibration.e
Quant Time: Oct 26 05:36:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

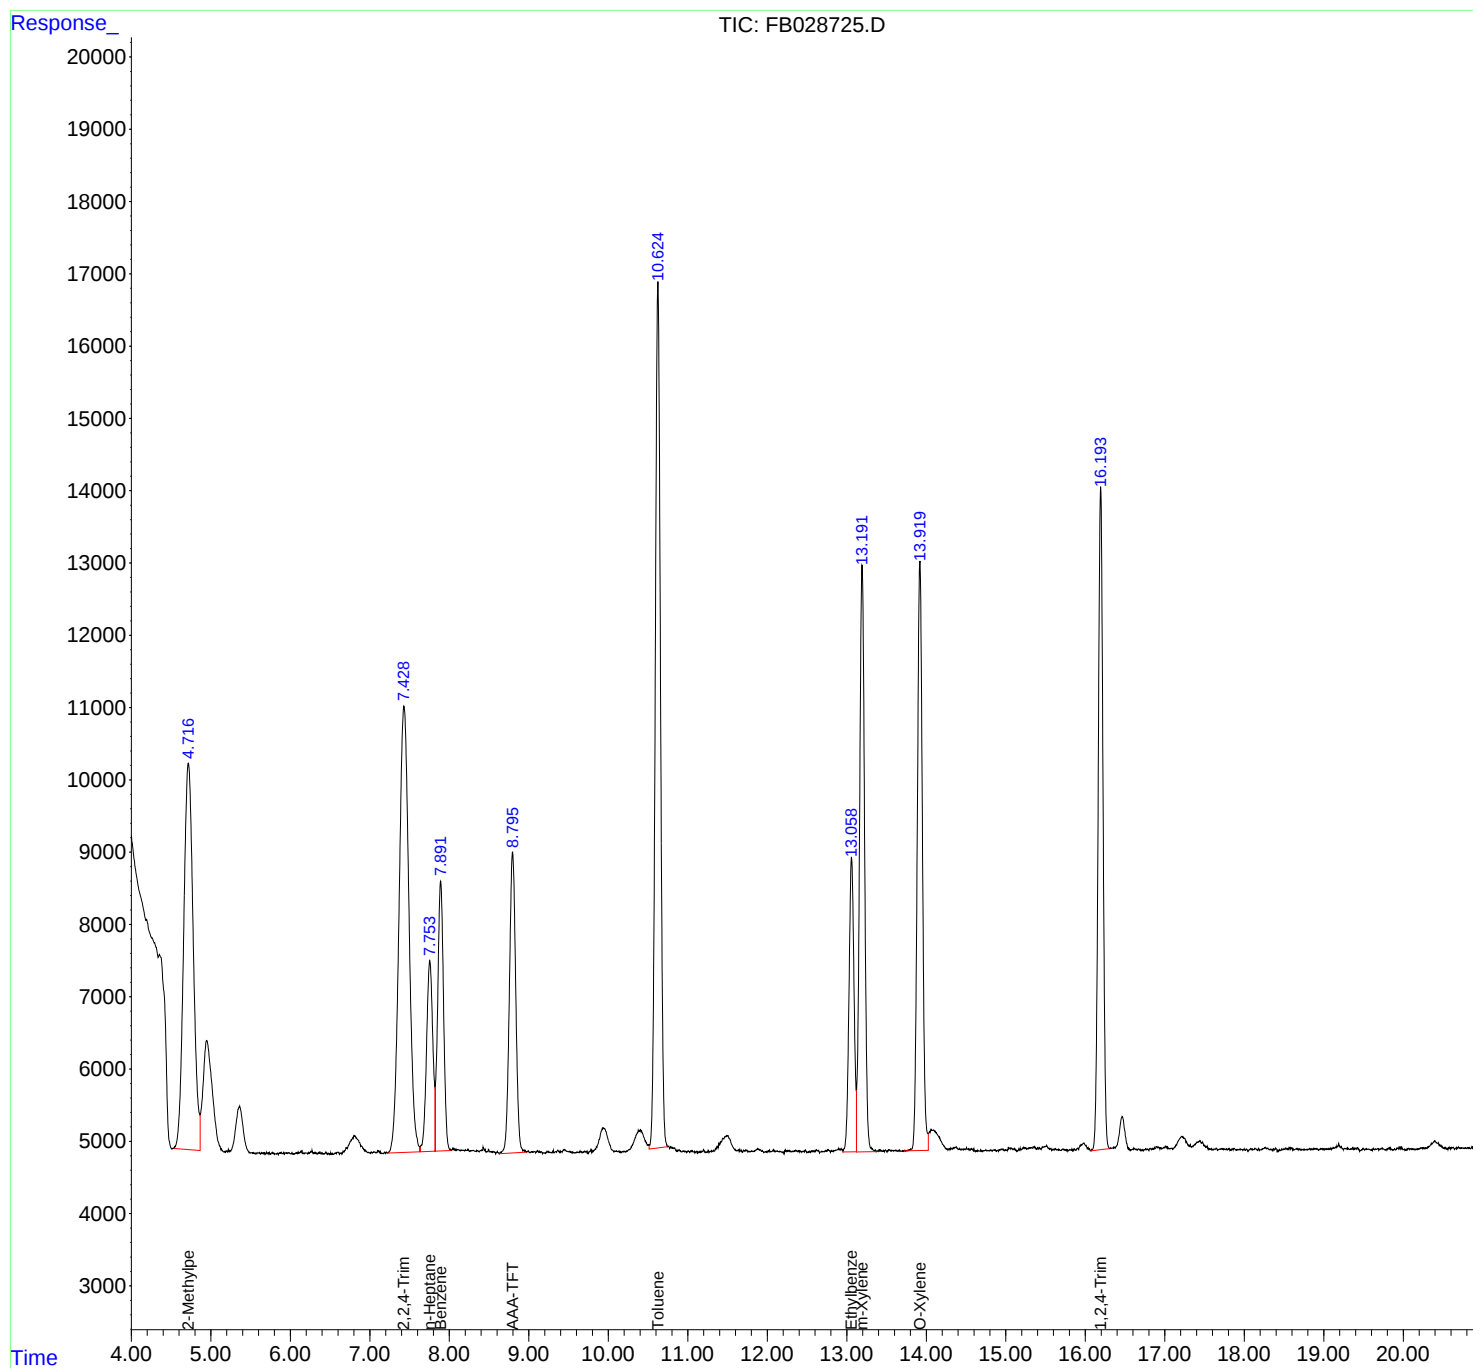


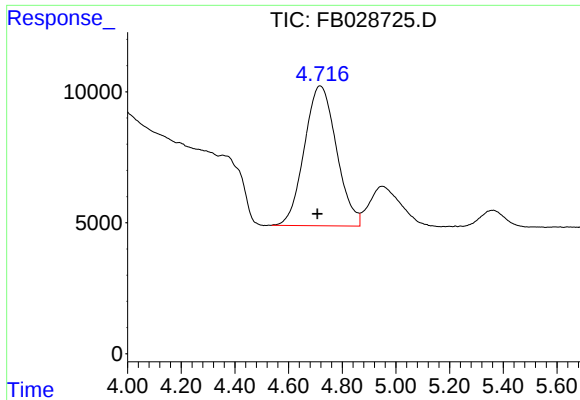

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.009 min
Response: 444450
Conc: 27.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S1

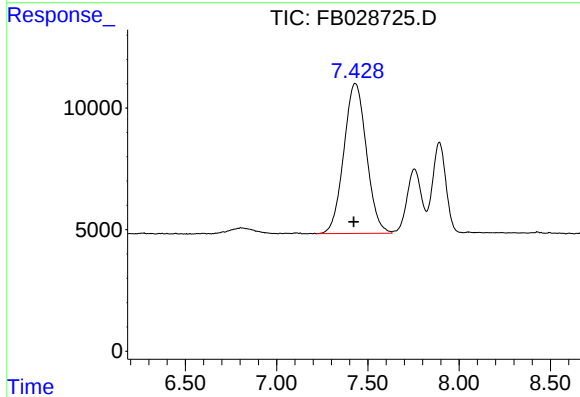


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.006 min
Response: 530826
Conc: 29.37 ng/ml

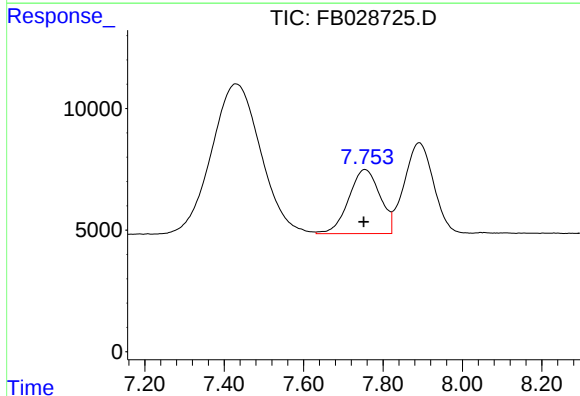


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.003 min
Response: 144225
Conc: 8.51 ng/ml

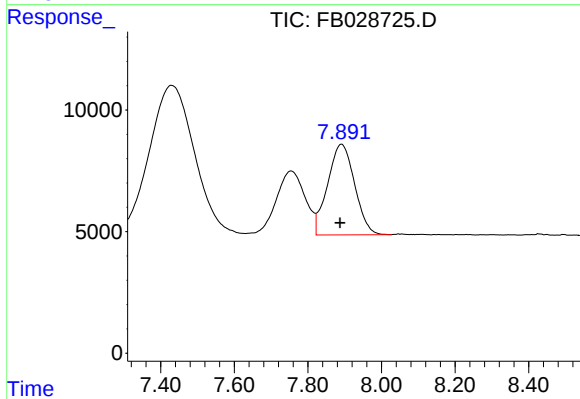

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.004 min
Response: 190126
Conc: 8.66 ng/ml

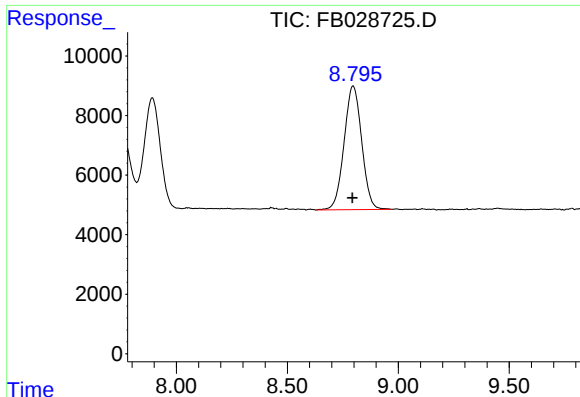

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.004 min
Response: 229323
Conc: 17.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S1

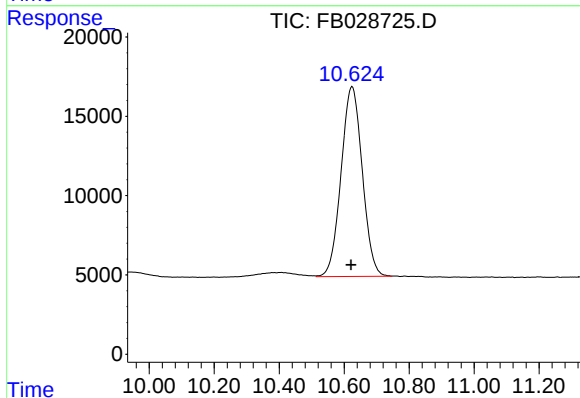


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.004 min
Response: 541480
Conc: 25.83 ng/ml

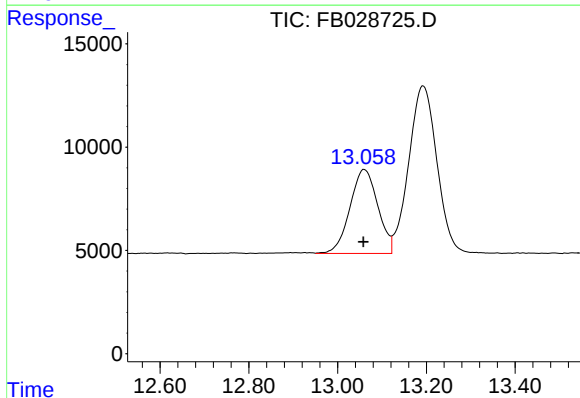


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.002 min
Response: 177583
Conc: 8.95 ng/ml

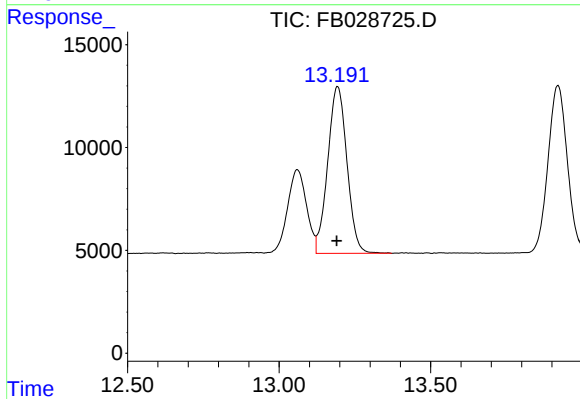

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.003 min
Response: 358388
Conc: 18.19 ng/ml

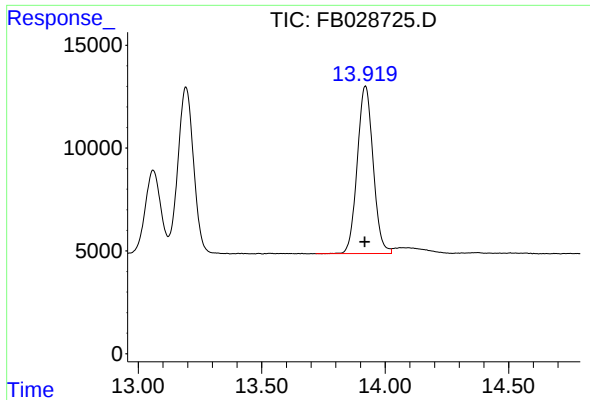

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.003 min
Response: 363594
Conc: 18.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S1

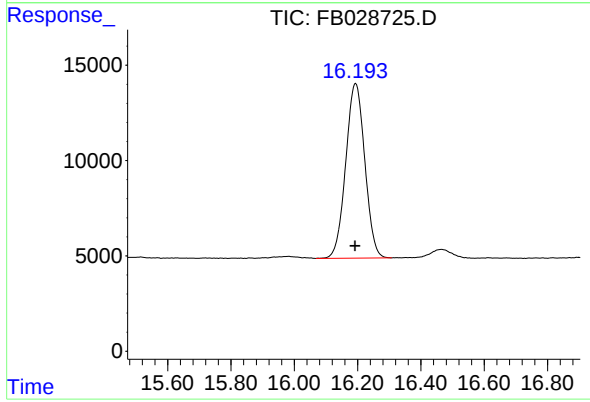

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 382880
Conc: 19.78 ng/ml