

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
 Data File : FB028731.D
 Signal(s) : FID2B.CH
 Acq On : 25 Oct 2022 15:02
 Operator : AJ/MA
 Sample : N5217-24MS
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-E3-COMPMS

Integration File: Calibration.e
 Quant Time: Oct 26 05:36:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	243073	18.789 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	364168	22.261 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	460964	25.507 ng/ml
3) t n-Heptane	7.754	144276	8.518 ng/ml
4) t Benzene	7.892	201578	9.177 ng/ml
6) t Toluene	10.626	579476	27.647 ng/ml
7) t Ethylbenzene	13.063	184584	9.301 ng/ml
8) t m-Xylene	13.196	357867	18.165 ng/ml
9) t O-Xylene	13.923	347780	17.876 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	298912	15.440 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
Data File : FB028731.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2022 15:02
Operator : AJ/MA
Sample : N5217-24MS
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-E3-COMPMS

Integration File: Calibration.e
Quant Time: Oct 26 05:36:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

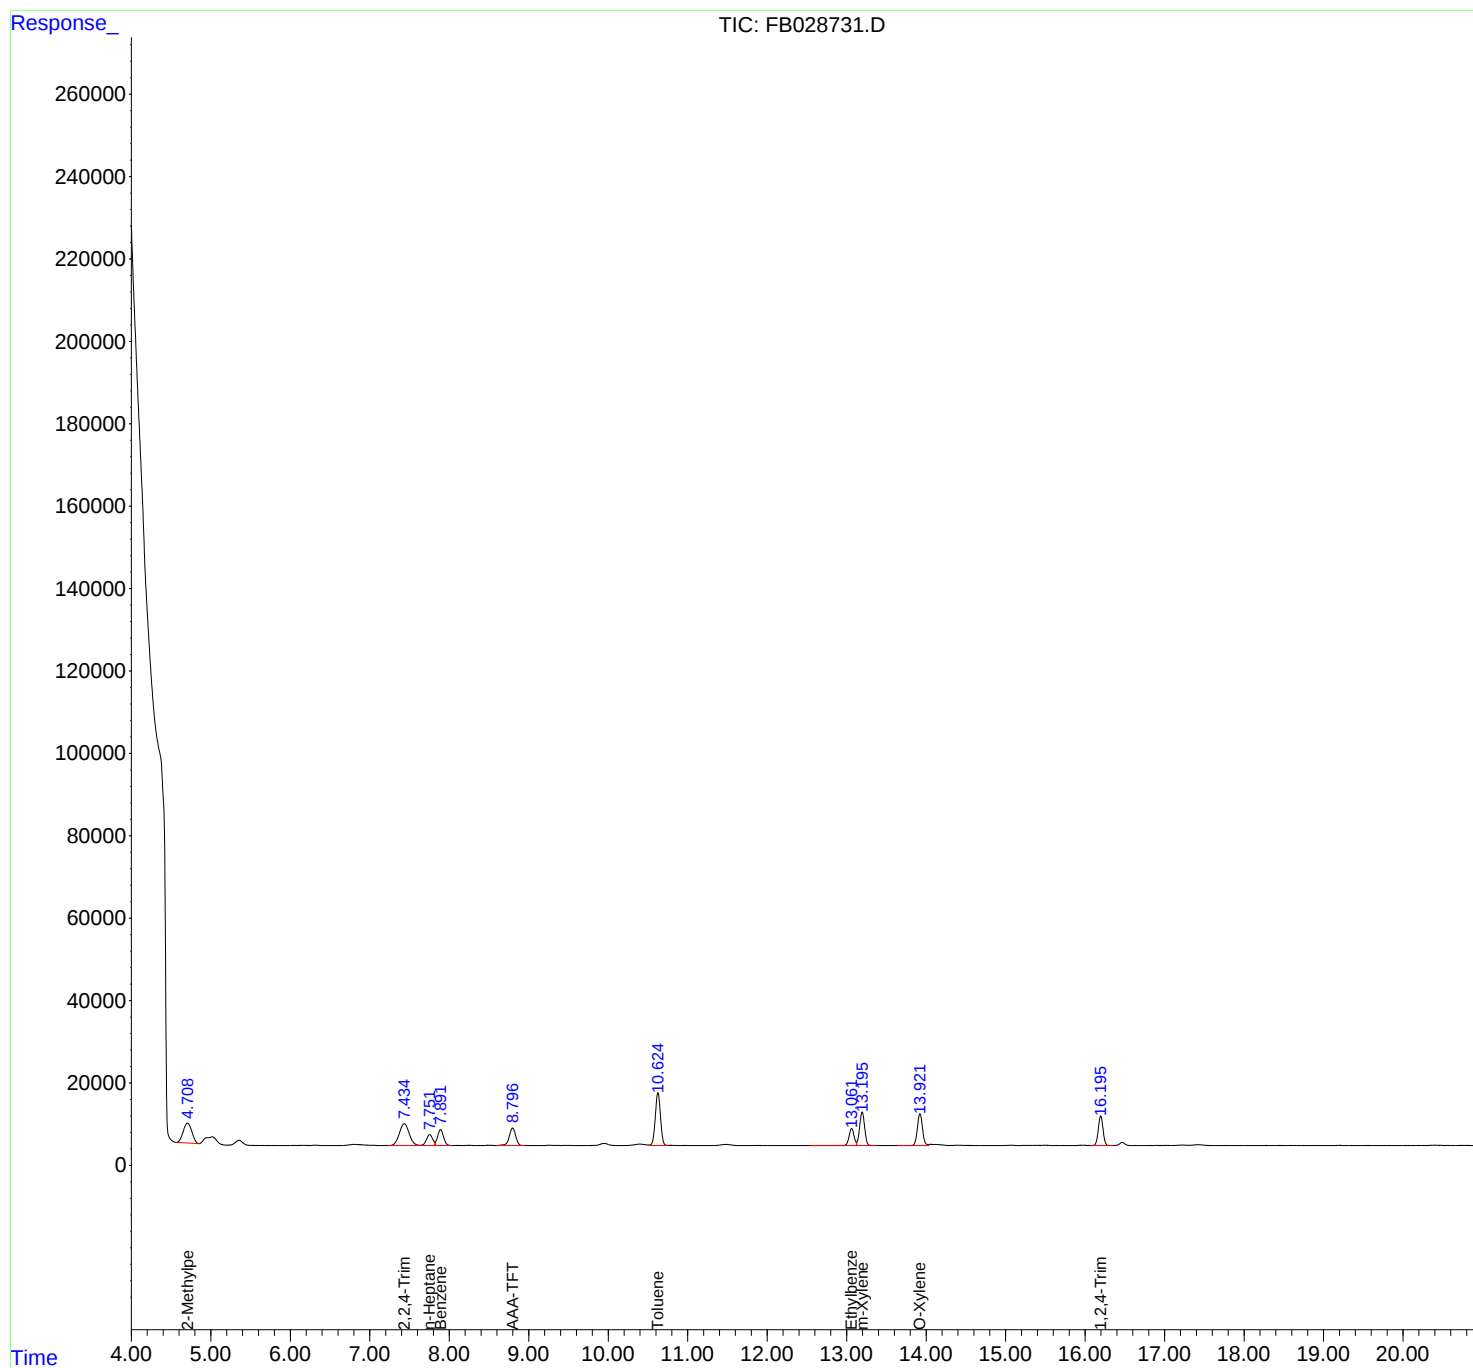


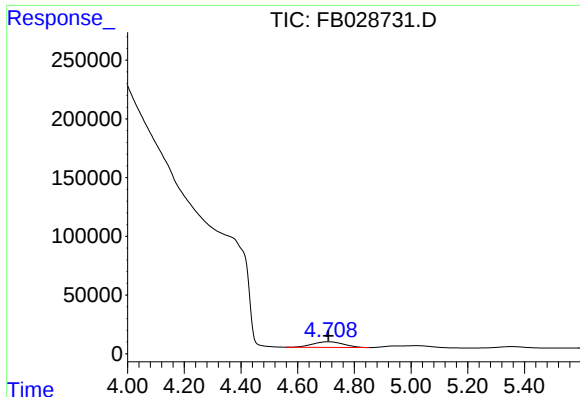

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.001 min
Response: 364168
Conc: 22.26 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-E3-COMPMS

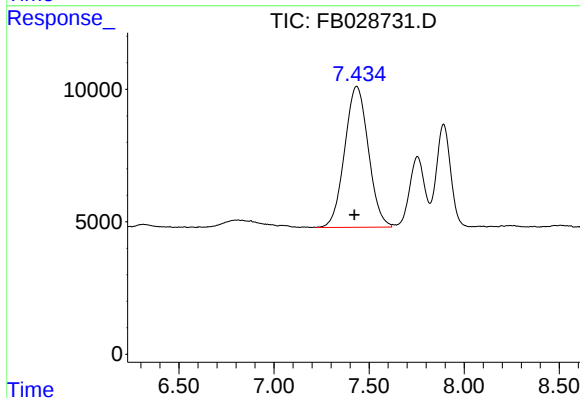


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.012 min
Response: 460964
Conc: 25.51 ng/ml

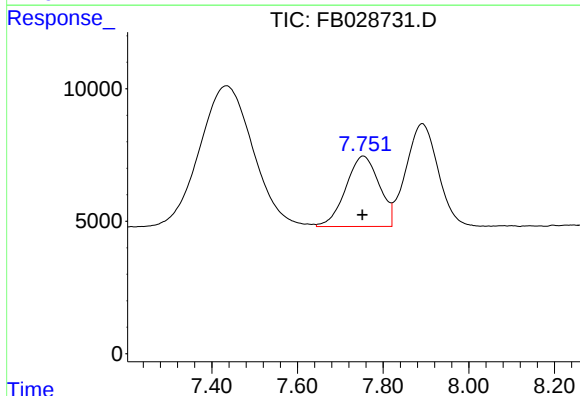


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.002 min
Response: 144276
Conc: 8.52 ng/ml

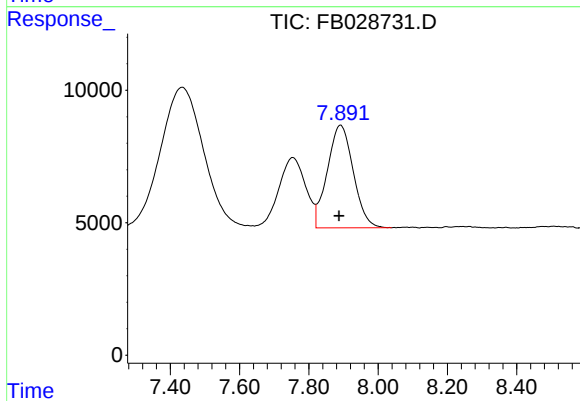

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.004 min
Response: 201578
Conc: 9.18 ng/ml

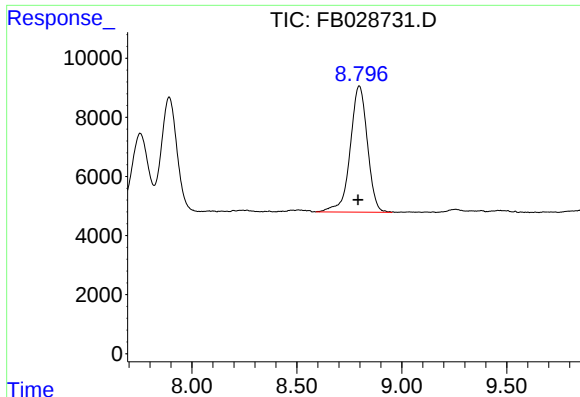

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.005 min
Response: 243073
Conc: 18.79 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-E3-COMPMS

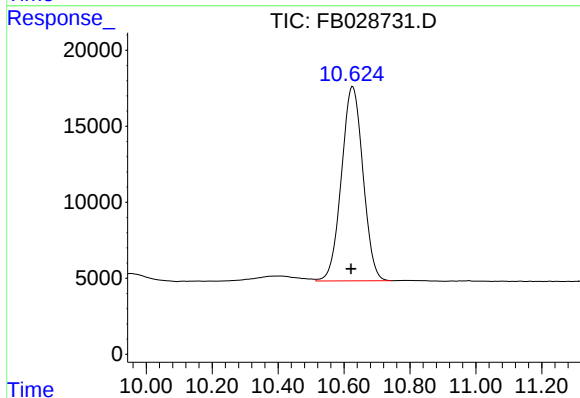


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.005 min
Response: 579476
Conc: 27.65 ng/ml

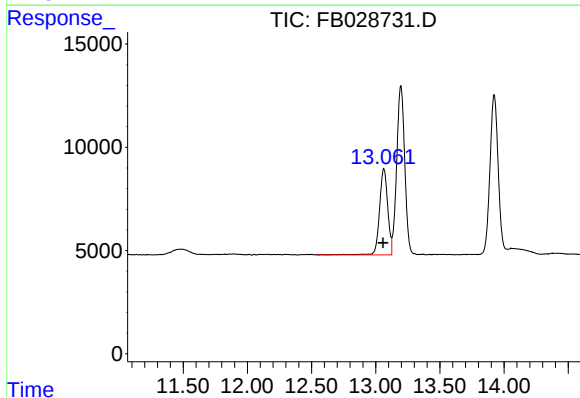


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.005 min
Response: 184584
Conc: 9.30 ng/ml

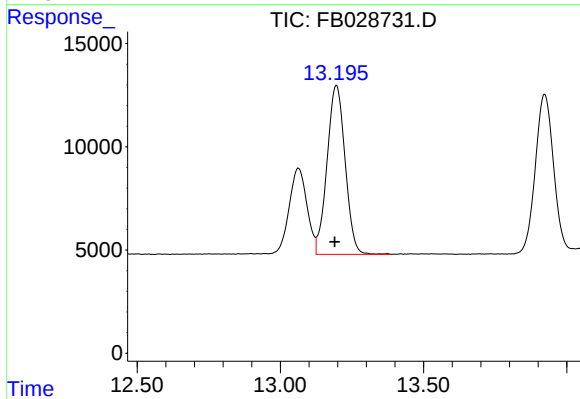

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: 0.005 min
Response: 357867
Conc: 18.17 ng/ml

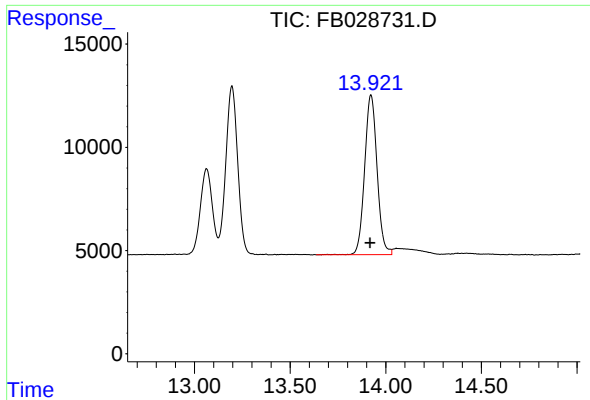

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.005 min
Response: 347780
Conc: 17.88 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-E3-COMPMS

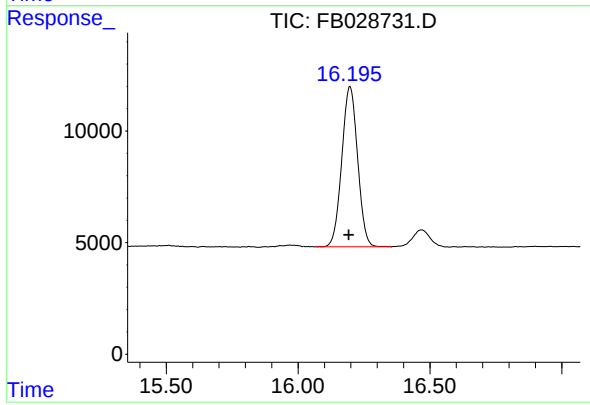

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.005 min
Response: 298912
Conc: 15.44 ng/ml