

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
 Data File : FB028732.D
 Signal(s) : FID2B.CH
 Acq On : 25 Oct 2022 15:40
 Operator : AJ/MA
 Sample : N5217-24MSD
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-E3-COMPMSD

Integration File: Calibration.e
 Quant Time: Oct 26 05:36:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	290192	22.431 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	391388	23.925 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	484820	26.827 ng/ml
3) t n-Heptane	7.756	157376	9.291 ng/ml
4) t Benzene	7.893	200100	9.110 ng/ml
6) t Toluene	10.627	579943	27.669 ng/ml
7) t Ethylbenzene	13.064	180737	9.107 ng/ml
8) t m-Xylene	13.197	352711	17.903 ng/ml
9) t O-Xylene	13.924	338859	17.418 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	292917	15.131 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
Data File : FB028732.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2022 15:40
Operator : AJ/MA
Sample : N5217-24MSD
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-E3-COMPMSD

Integration File: Calibration.e
Quant Time: Oct 26 05:36:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

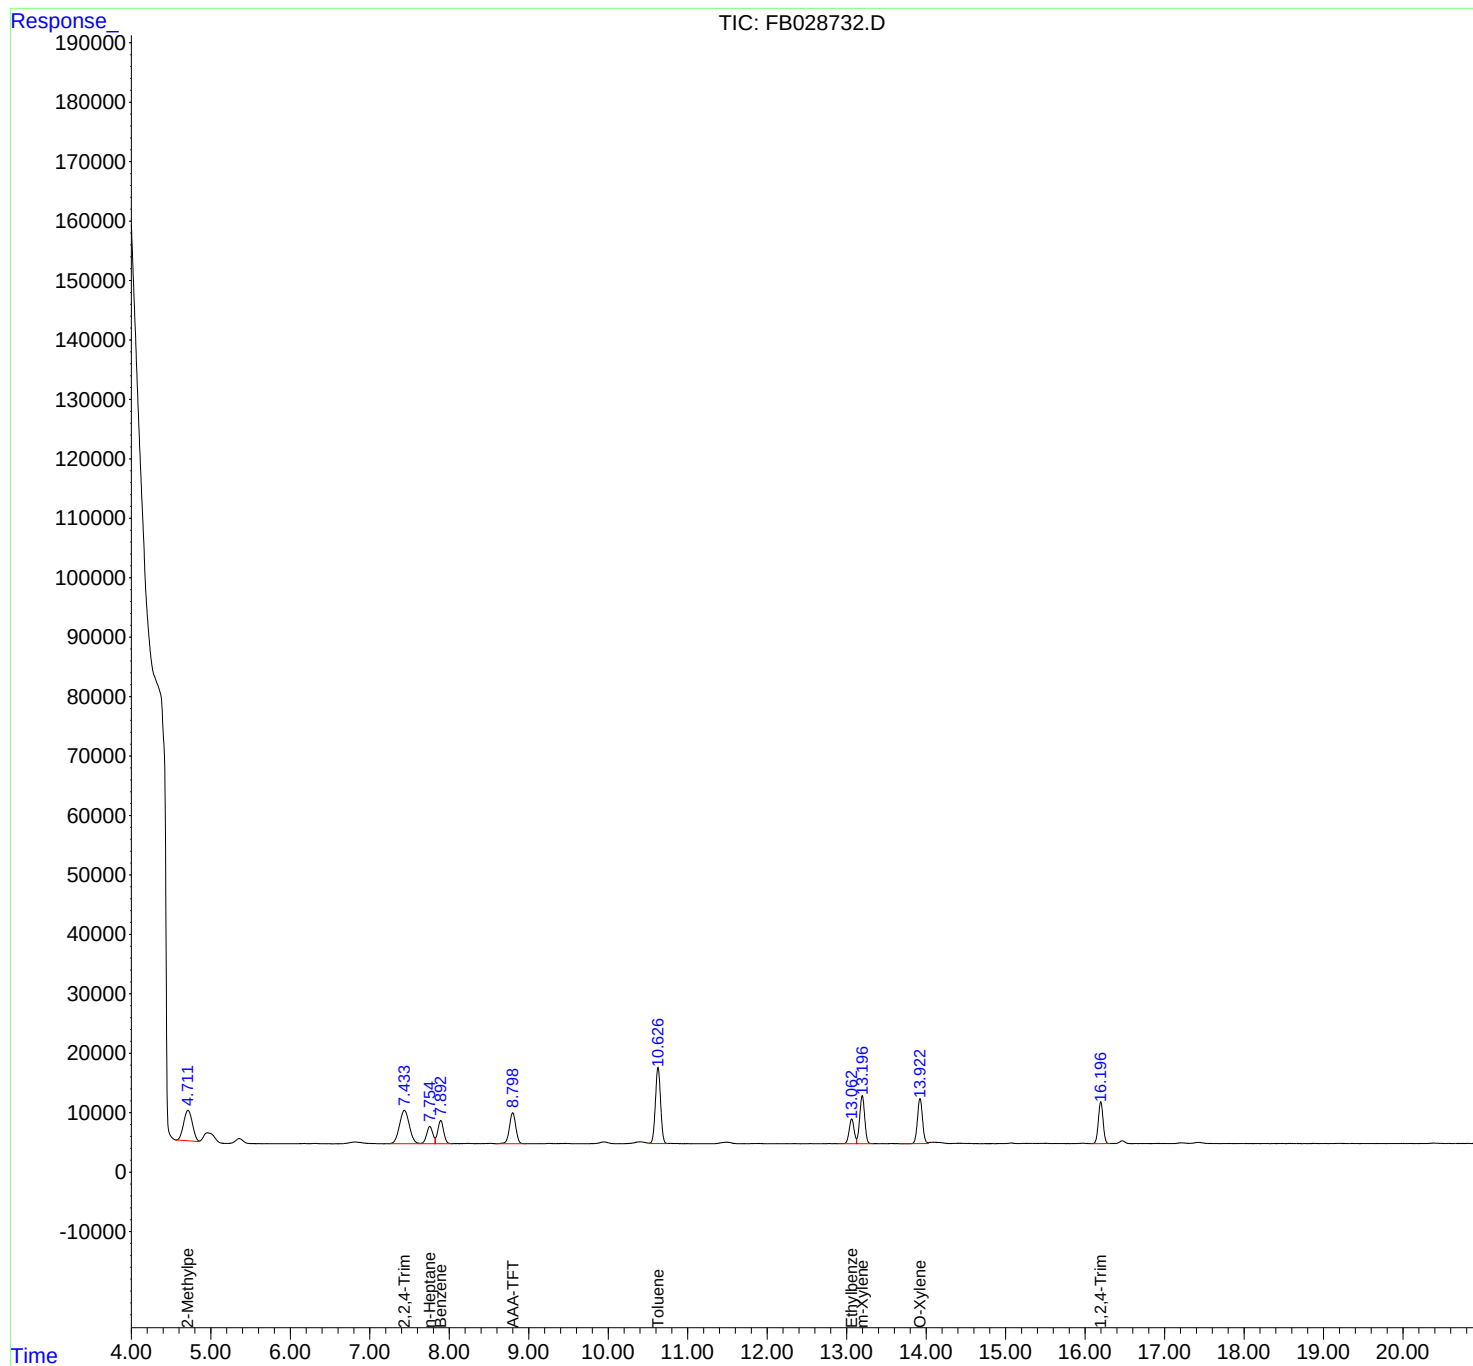


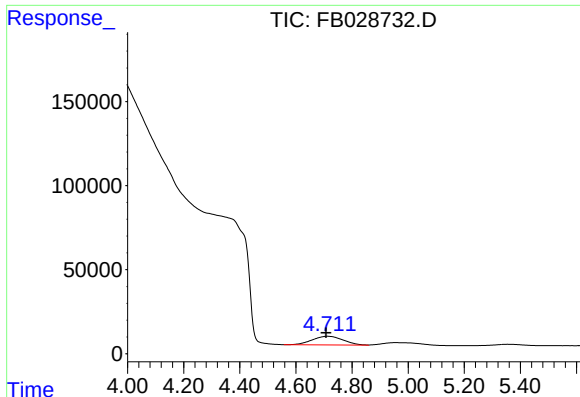

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.005 min
Response: 391388
Conc: 23.92 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-E3-COMPMSD

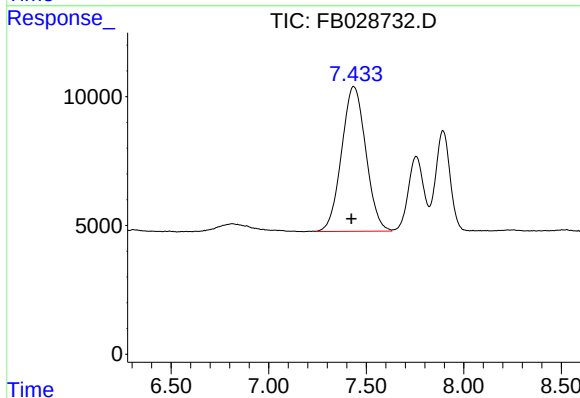


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.011 min
Response: 484820
Conc: 26.83 ng/ml

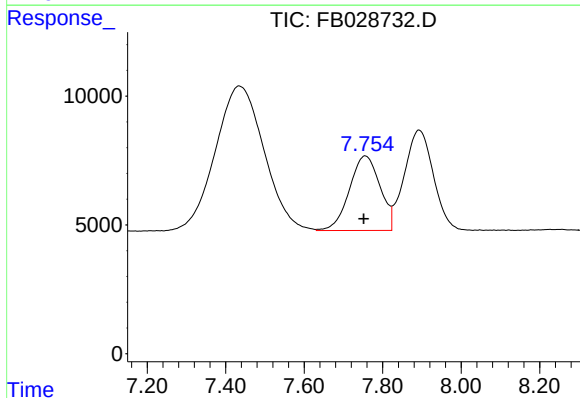


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.004 min
Response: 157376
Conc: 9.29 ng/ml

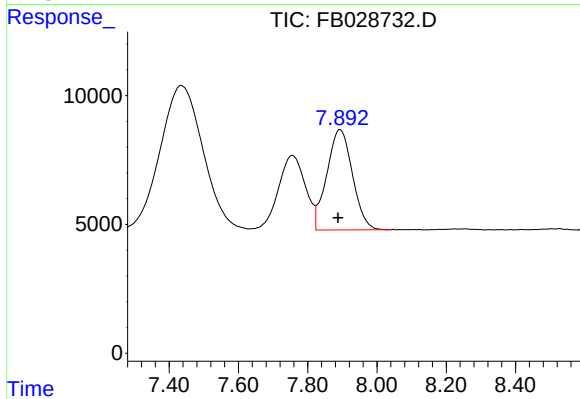

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.006 min
Response: 200100
Conc: 9.11 ng/ml

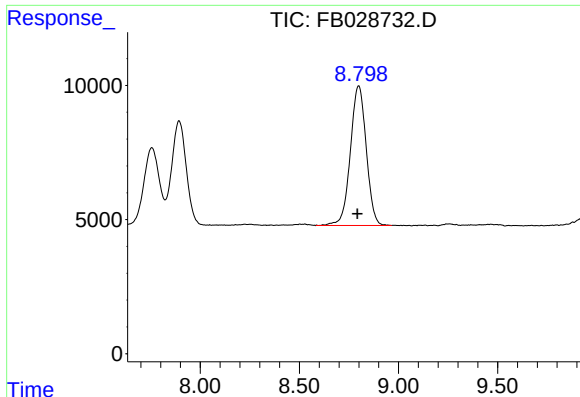

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.007 min
Response: 290192
Conc: 22.43 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-E3-COMPMSD

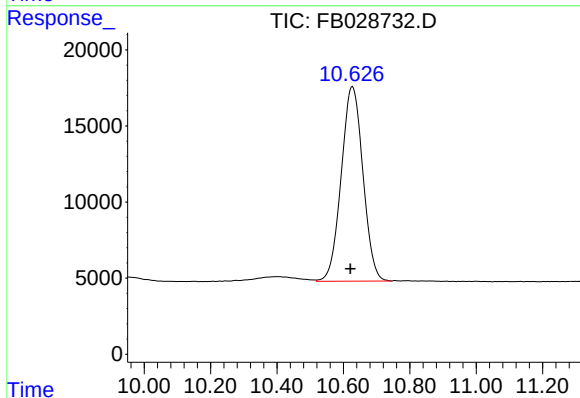


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.006 min
Response: 579943
Conc: 27.67 ng/ml

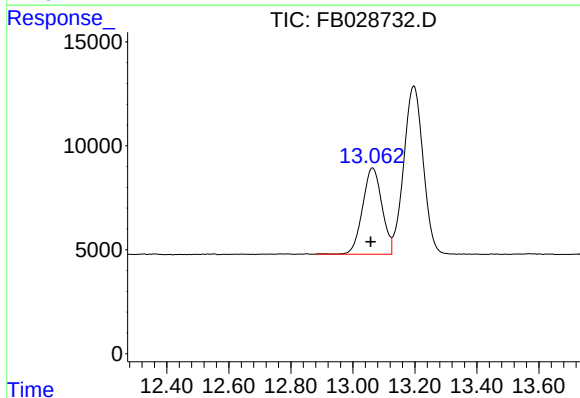


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.006 min
Response: 180737
Conc: 9.11 ng/ml

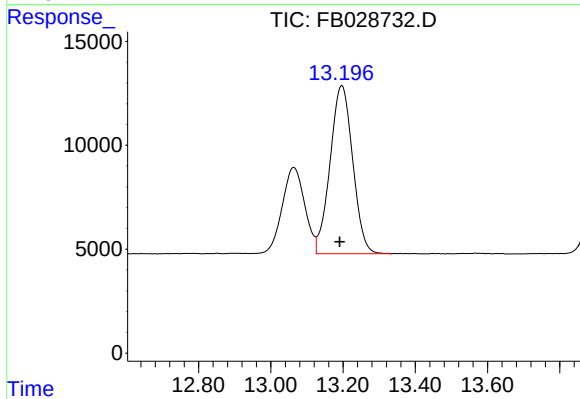

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.007 min
Response: 352711
Conc: 17.90 ng/ml

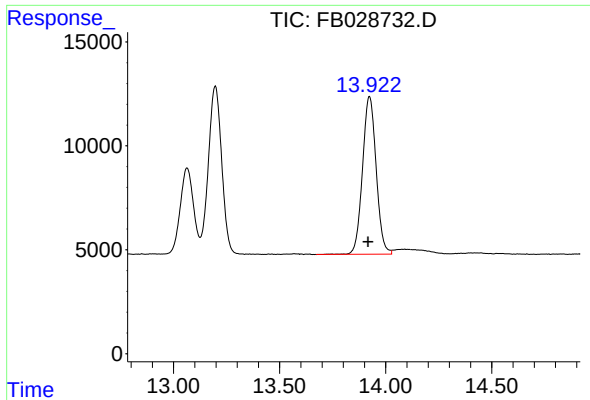

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.006 min
Response: 338859
Conc: 17.42 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-E3-COMPMSD

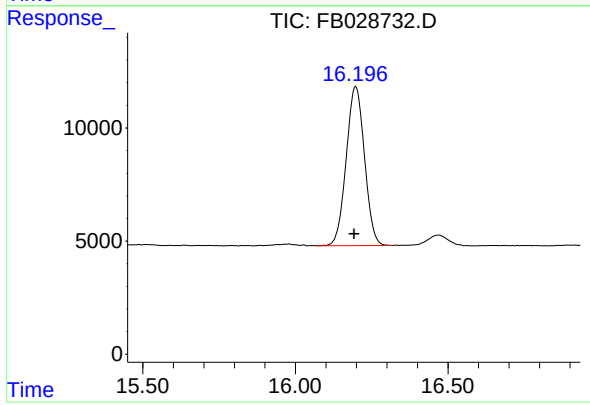

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.005 min
Response: 292917
Conc: 15.13 ng/ml