

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
 Data File : FB028744.D
 Signal(s) : FID2B.CH
 Acq On : 25 Oct 2022 23:49
 Operator : AJ/MA
 Sample : BSF1025S2
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1025S2

Integration File: Calibration.e
 Quant Time: Oct 26 05:37:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
 Quant Title :
 QLast Update : Wed Oct 05 12:47:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	276614	21.381 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.720	502903	30.742 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	568826	31.475 ng/ml
3) t n-Heptane	7.758	175283	10.348 ng/ml
4) t Benzene	7.896	217887	9.920 ng/ml
6) t Toluene	10.628	635744	30.331 ng/ml
7) t Ethylbenzene	13.065	203554	10.256 ng/ml
8) t m-Xylene	13.197	395196	20.060 ng/ml
9) t O-Xylene	13.924	383792	19.727 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	357657	18.475 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
Data File : FB028744.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2022 23:49
Operator : AJ/MA
Sample : BSF1025S2
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1025S2

Integration File: Calibration.e
Quant Time: Oct 26 05:37:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

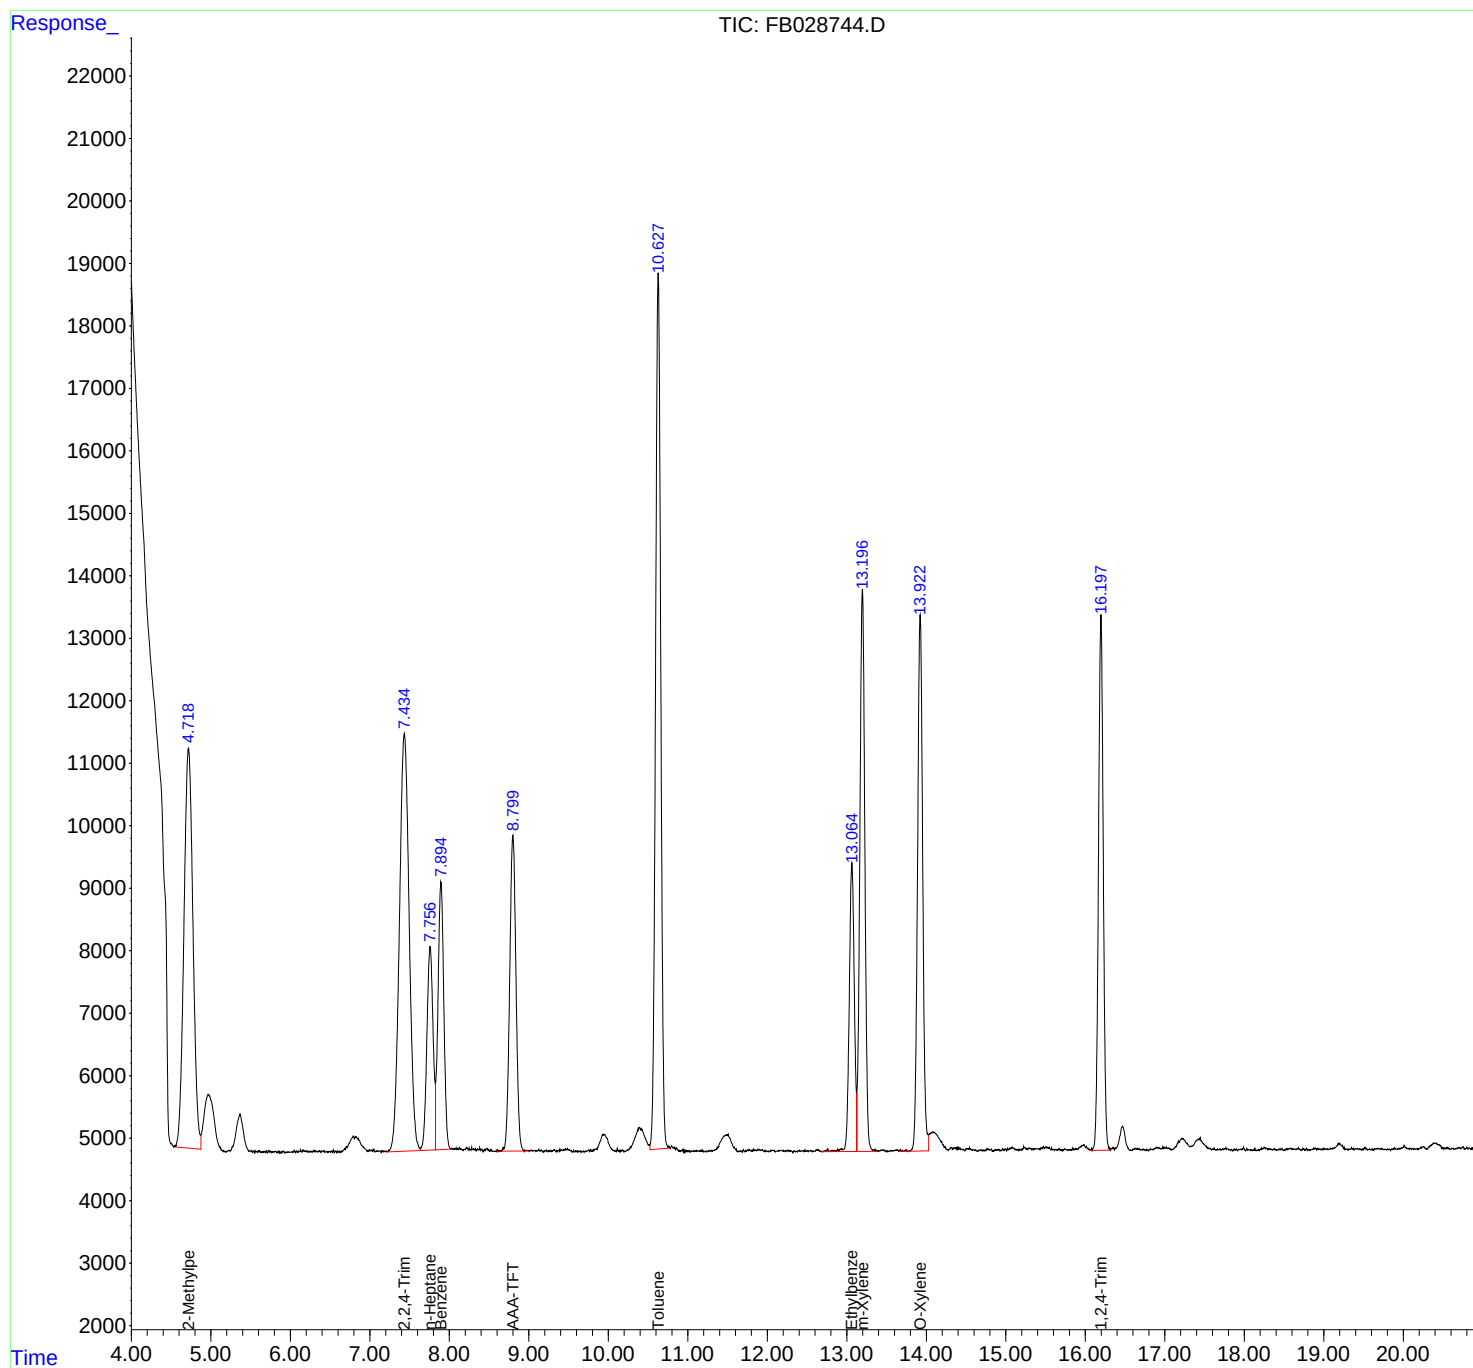


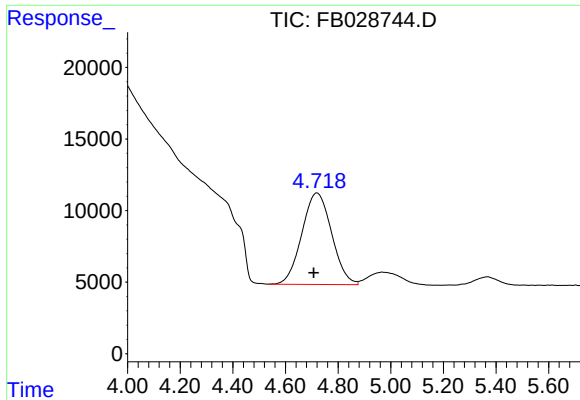

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.012 min
Response: 502903
Conc: 30.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S2

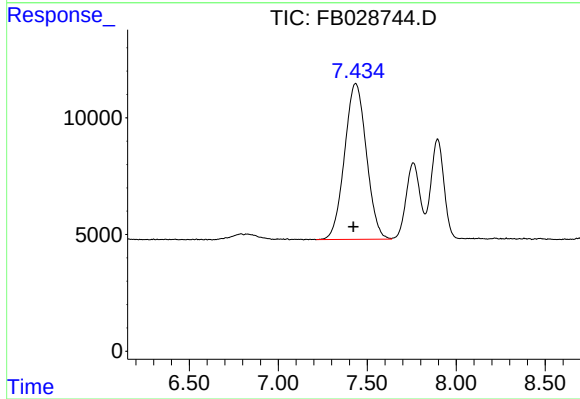


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.012 min
Response: 568826
Conc: 31.48 ng/ml

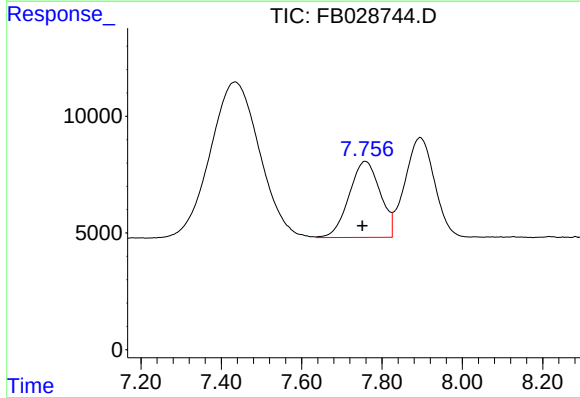


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.007 min
Response: 175283
Conc: 10.35 ng/ml

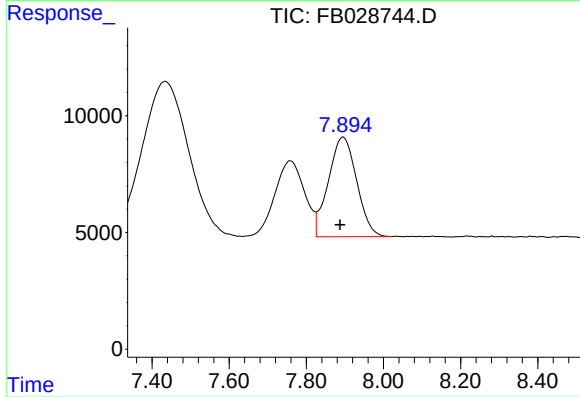

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.008 min
Response: 217887
Conc: 9.92 ng/ml

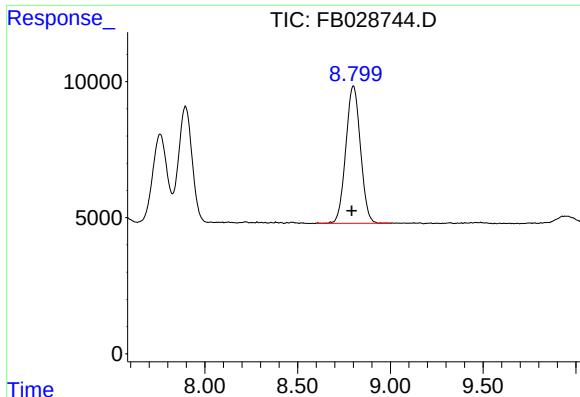

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.008 min
Response: 276614
Conc: 21.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S2

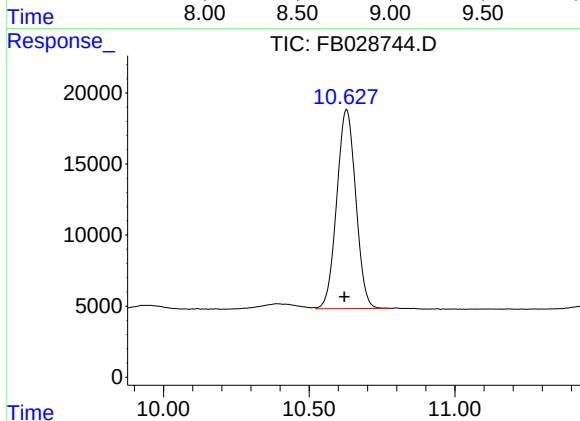


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.007 min
Response: 635744
Conc: 30.33 ng/ml

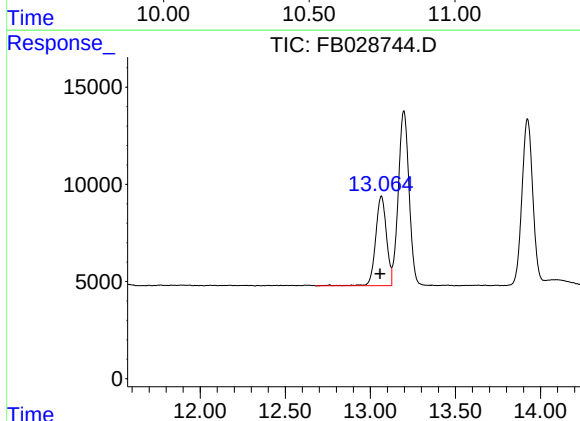


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.007 min
Response: 203554
Conc: 10.26 ng/ml

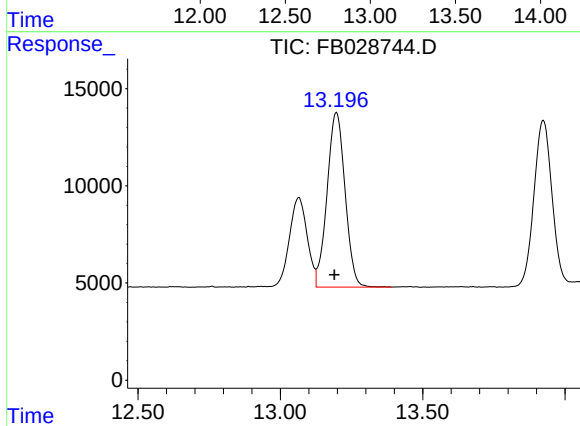

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.007 min
Response: 395196
Conc: 20.06 ng/ml

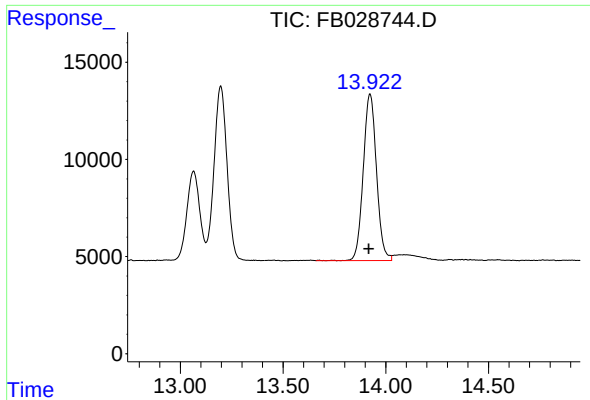

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.006 min
Response: 383792
Conc: 19.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S2

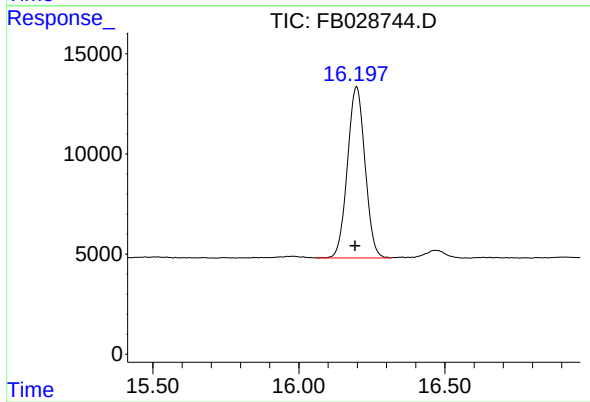

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.005 min
Response: 357657
Conc: 18.47 ng/ml