

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
Data File : FB028755.D
Signal(s) : FID2B.CH
Acq On : 26 Oct 2022 7:19
Operator : AJ/MA
Sample : BSF1025S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1025S3

Integration File: Calibration.e
Quant Time: Oct 26 07:40:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	212947	16.460 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	445941	27.260 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	506225	28.011 ng/ml
3) t n-Heptane	7.755	147933	8.734 ng/ml
4) t Benzene	7.893	188288	8.572 ng/ml
6) t Toluene	10.627	551641	26.319 ng/ml
7) t Ethylbenzene	13.063	175238	8.830 ng/ml
8) t m-Xylene	13.195	345276	17.526 ng/ml
9) t O-Xylene	13.922	340787	17.517 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	331356	17.116 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102522\
Data File : FB028755.D
Signal(s) : FID2B.CH
Acq On : 26 Oct 2022 7:19
Operator : AJ/MA
Sample : BSF1025S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1025S3

Integration File: Calibration.e
Quant Time: Oct 26 07:40:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100522.M
Quant Title :
QLast Update : Wed Oct 05 12:47:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

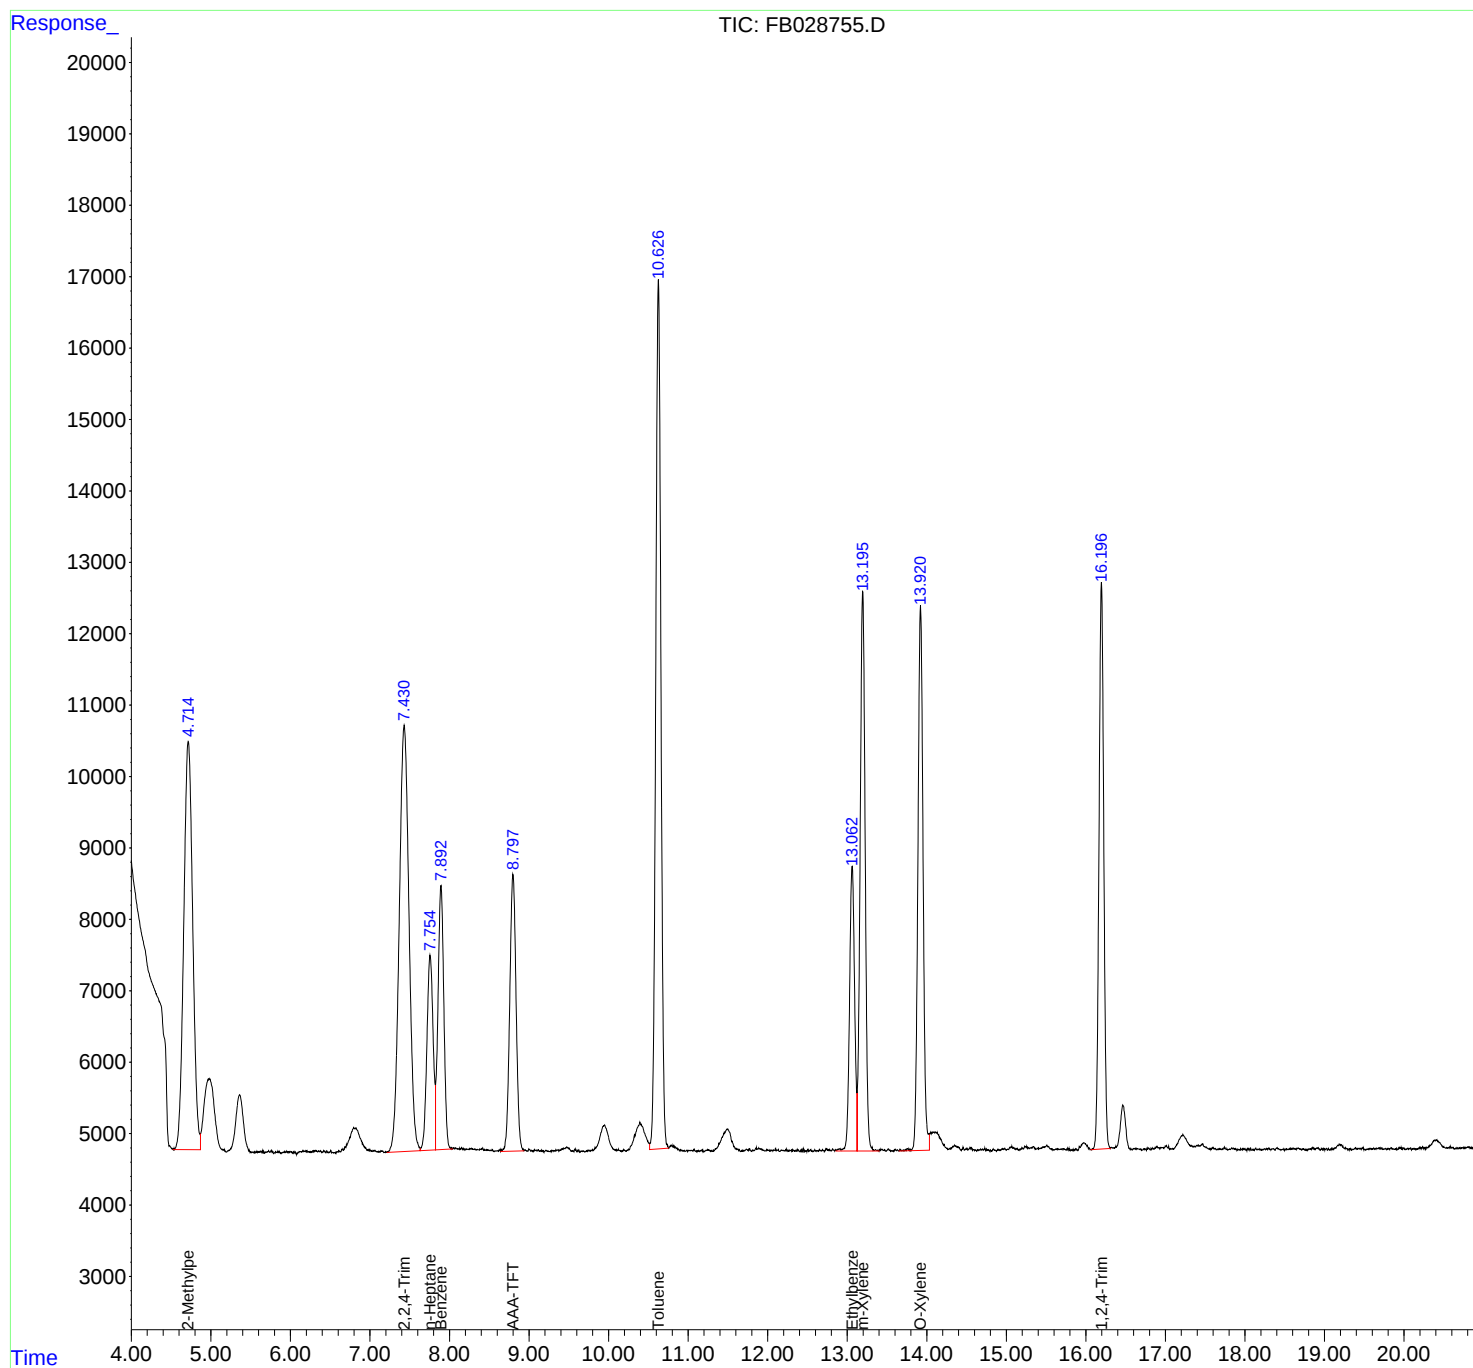


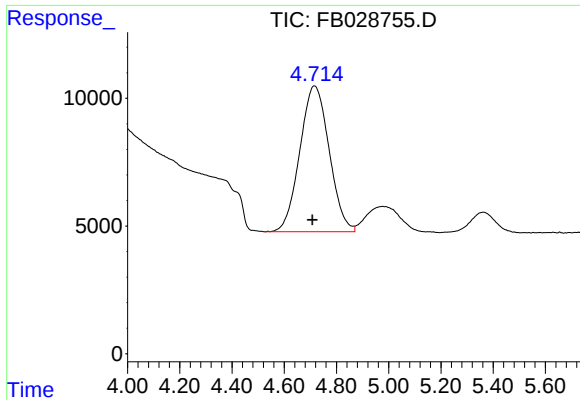

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.008 min
Response: 445941
Conc: 27.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S3

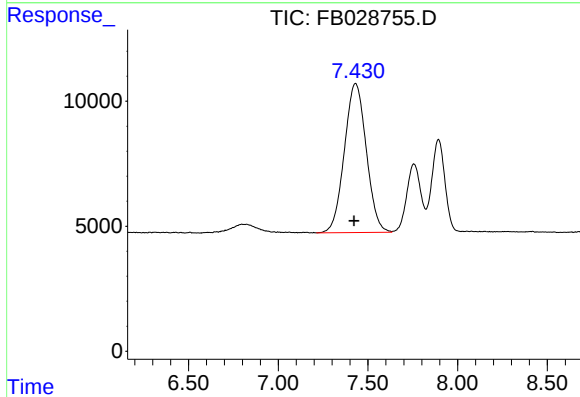


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.008 min
Response: 506225
Conc: 28.01 ng/ml

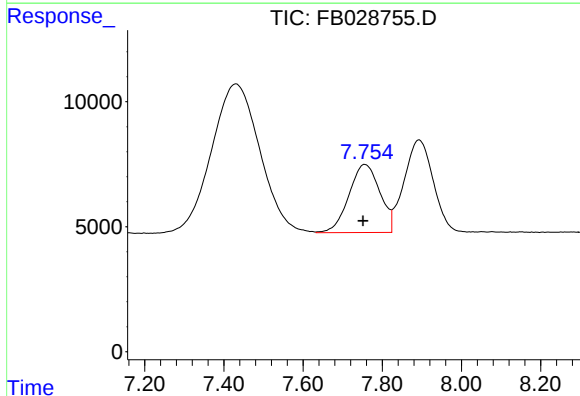


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.004 min
Response: 147933
Conc: 8.73 ng/ml

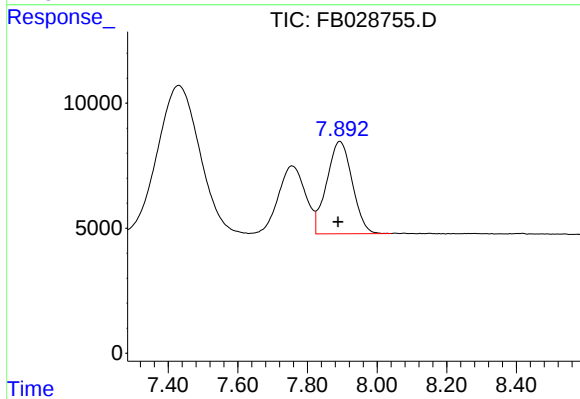

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.006 min
Response: 188288
Conc: 8.57 ng/ml

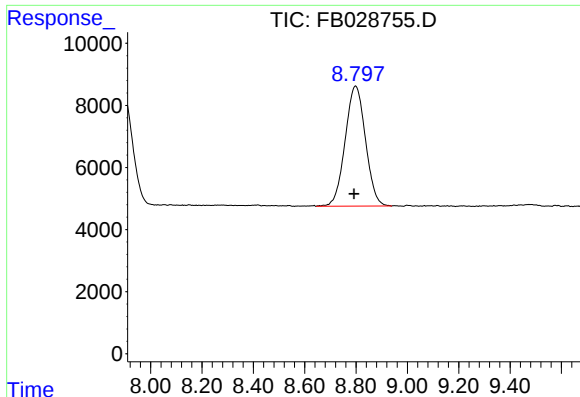

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.006 min
Response: 212947
Conc: 16.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S3

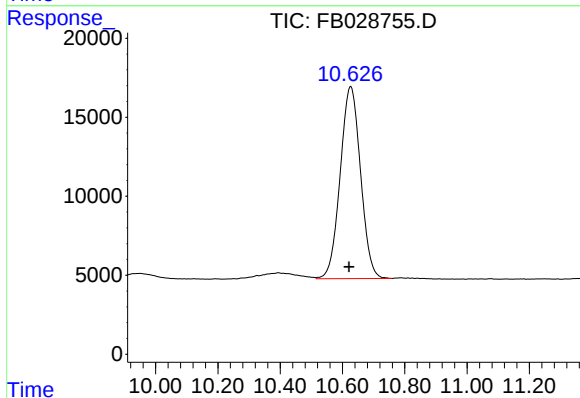


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.006 min
Response: 551641
Conc: 26.32 ng/ml

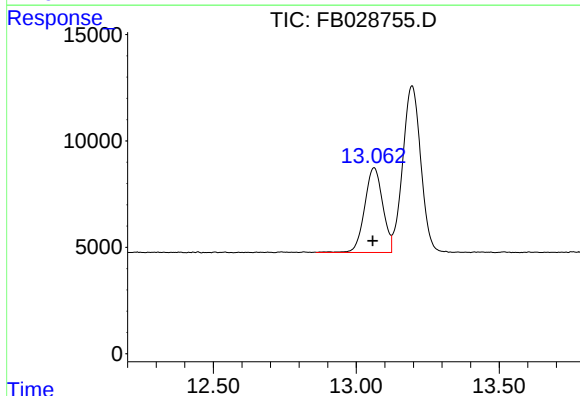


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.005 min
Response: 175238
Conc: 8.83 ng/ml

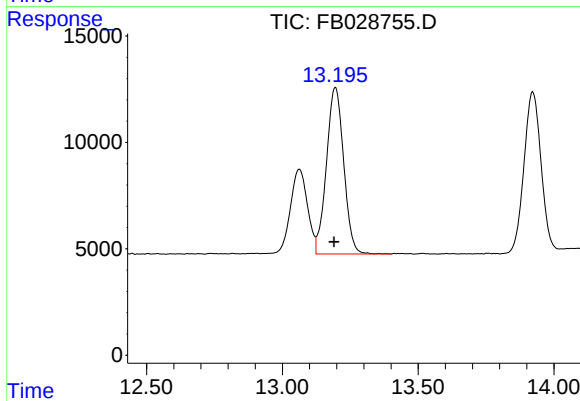

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.005 min
Response: 345276
Conc: 17.53 ng/ml

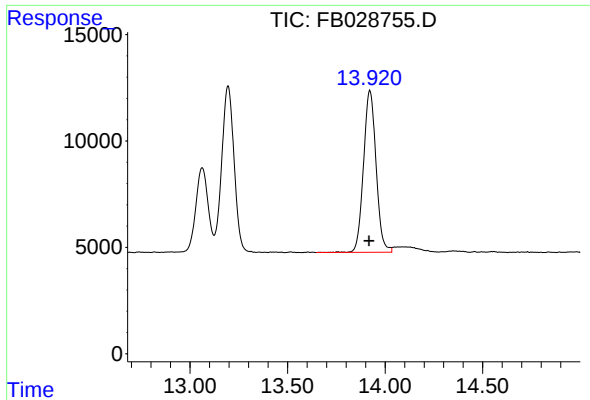

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.005 min
Response: 340787
Conc: 17.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S3

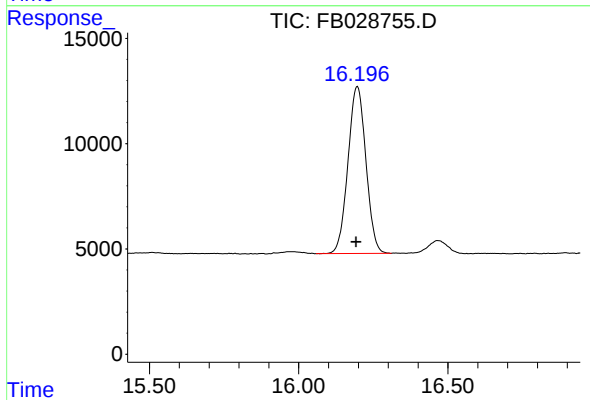

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.004 min
Response: 331356
Conc: 17.12 ng/ml