

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102524\
 Data File : FB031038.D
 Signal(s) : FID2B.CH
 Acq On : 25 Oct 2024 10:29
 Operator : YP/AJ
 Sample : BSF1025S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1025S1

Integration File: Calibration.e
 Quant Time: Oct 26 00:02:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
 Quant Title :
 QLast Update : Fri Oct 04 11:53:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	600927	20.046 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.723	973152	26.968 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	1274461	26.744 ng/ml
3) t n-Heptane	7.755	342922	7.603 ng/ml
4) t Benzene	7.894	489954	8.914 ng/ml
6) t Toluene	10.623	1388725	25.708 ng/ml
7) t Ethylbenzene	13.060	421917	8.901 ng/ml
8) t m-Xylene	13.193	911207	17.467 ng/ml
9) t O-Xylene	13.922	852949	17.534 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	665969	20.324 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102524\
Data File : FB031038.D
Signal(s) : FID2B.CH
Acq On : 25 Oct 2024 10:29
Operator : YP/AJ
Sample : BSF1025S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1025S1

Integration File: Calibration.e
Quant Time: Oct 26 00:02:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB100424.M
Quant Title :
QLast Update : Fri Oct 04 11:53:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

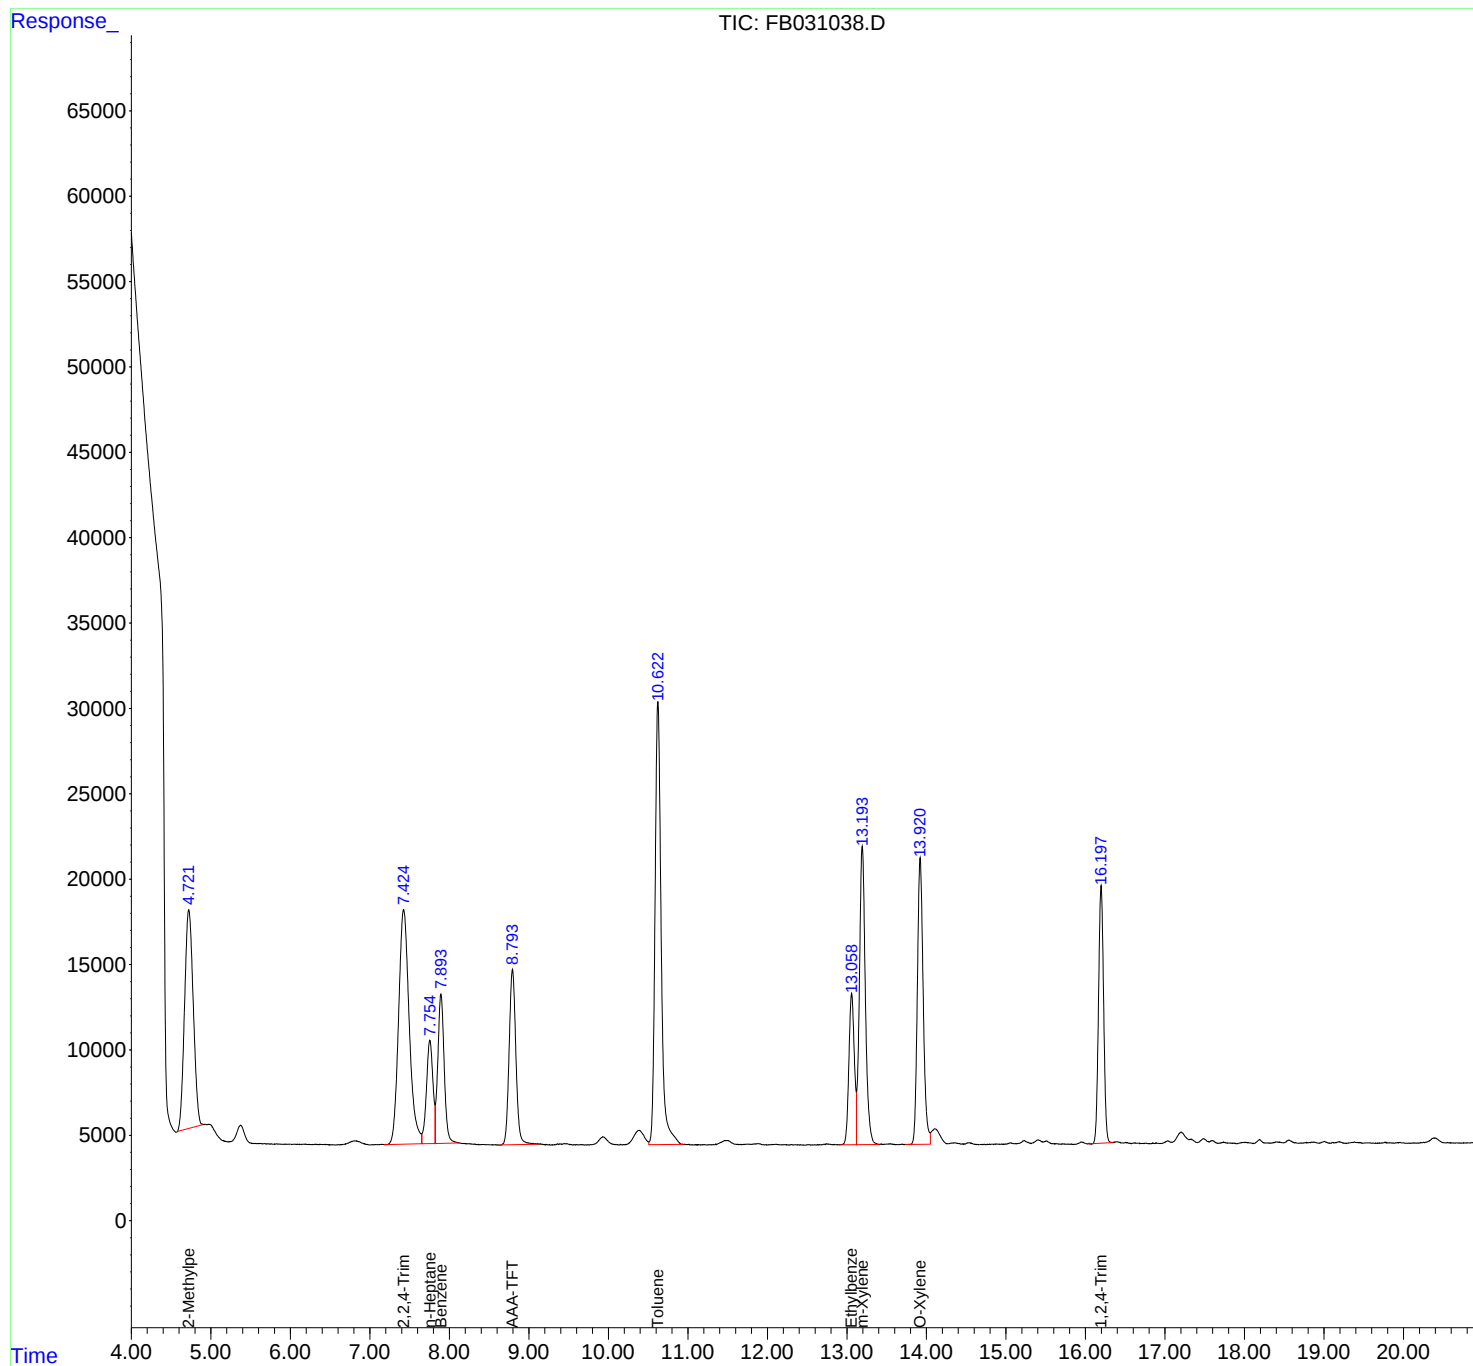


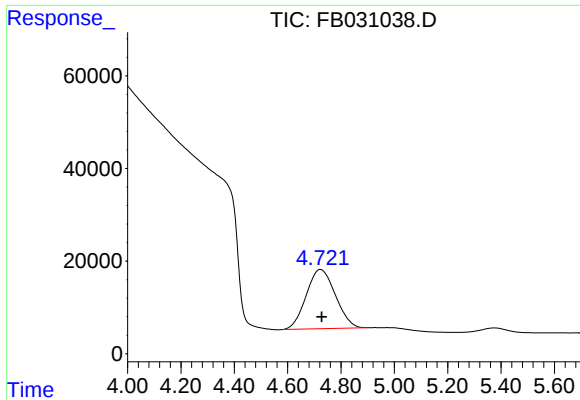

#1 2-Methylpentane


R.T.: 4.723 min
Delta R.T.: -0.005 min
Response: 973152
Conc: 26.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S1

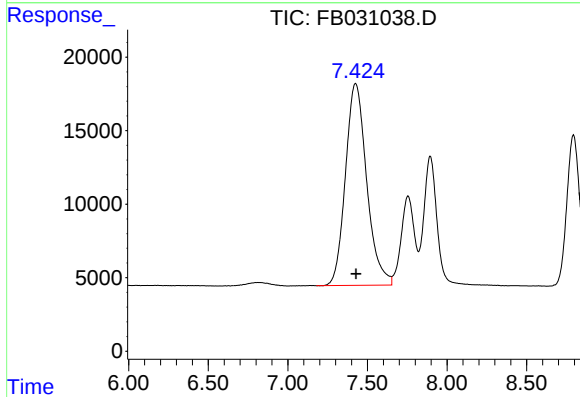


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.003 min
Response: 1274461
Conc: 26.74 ng/ml

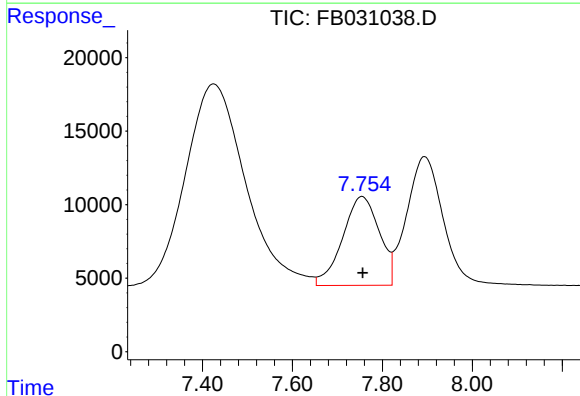


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.001 min
Response: 342922
Conc: 7.60 ng/ml

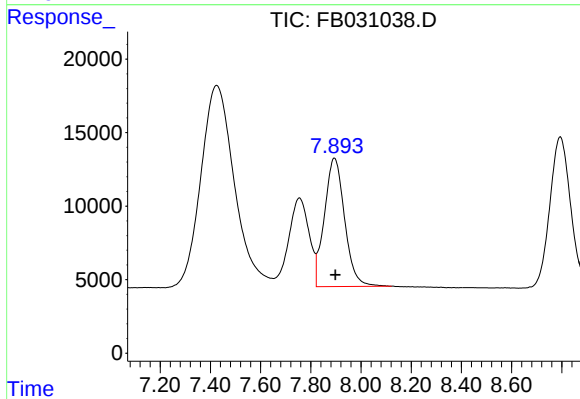

#4 Benzene


R.T.: 7.894 min
Delta R.T.: -0.003 min
Response: 489954
Conc: 8.91 ng/ml

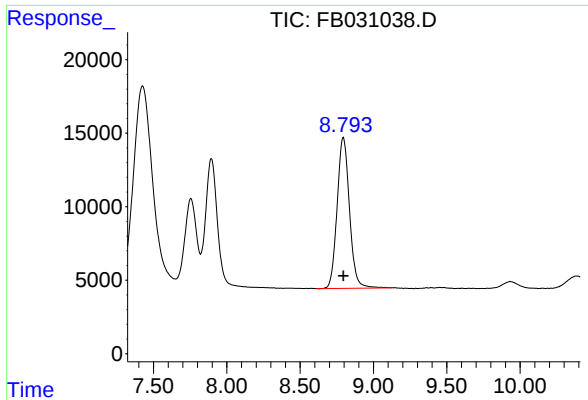

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.001 min
Response: 600927
Conc: 20.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S1

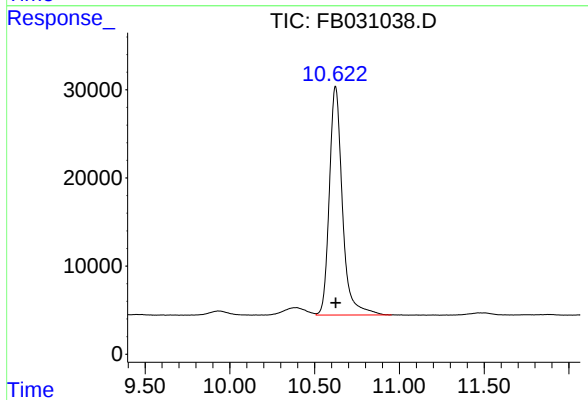


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.002 min
Response: 1388725
Conc: 25.71 ng/ml

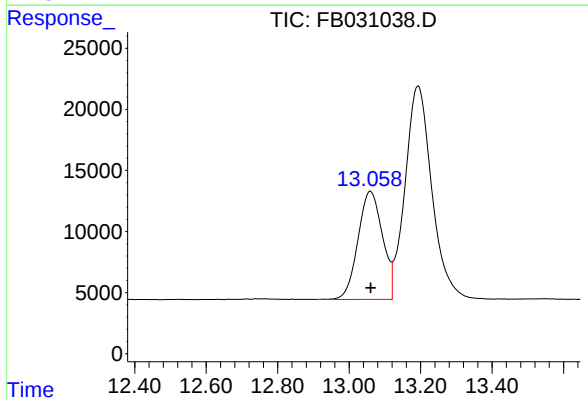


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.000 min
Response: 421917
Conc: 8.90 ng/ml

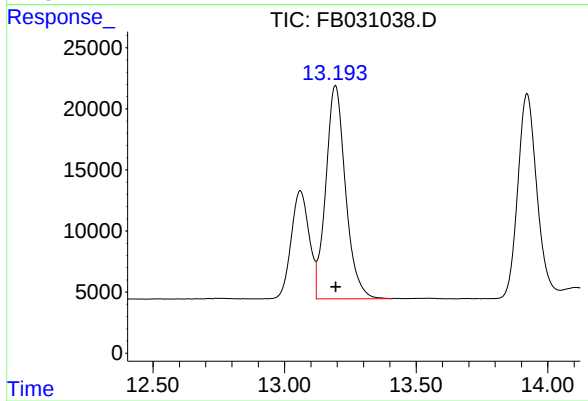

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.002 min
Response: 911207
Conc: 17.47 ng/ml

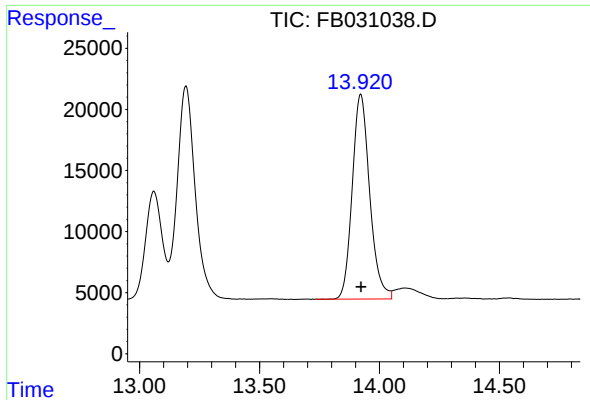

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.001 min
Response: 852949
Conc: 17.53 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1025S1

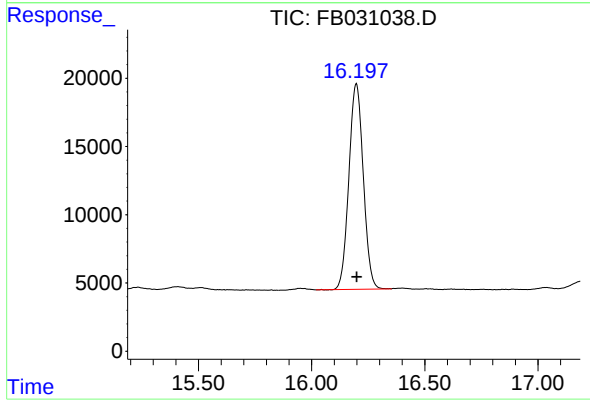

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.000 min
Response: 665969
Conc: 20.32 ng/ml