

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102618\  
Data File : FB018358.D  
Signal(s) : FID2B.CH  
Acq On : 26 Oct 2018 12:37  
Operator : MJ/SJ  
Sample : J5675-02  
Misc : 5.01g/5.00mL DI Water  
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Oct 29 04:04:15 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB101218.M  
Quant Title :  
QLast Update : Fri Oct 12 08:04:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 9.108  | 175110   | 20.331 ng/ml |
|                             |        |          |              |
| Target Compounds            |        |          |              |
| 9) t O-Xylene               | 14.346 | 1592     | 0.089 ng/ml  |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB102618\  
Data File : FB018358.D  
Signal(s) : FID2B.CH  
Acq On : 26 Oct 2018 12:37  
Operator : MJ/SJ  
Sample : J5675-02  
Misc : 5.01g/5.00mL DI Water  
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Oct 29 04:04:15 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB101218.M  
Quant Title :  
QLast Update : Fri Oct 12 08:04:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

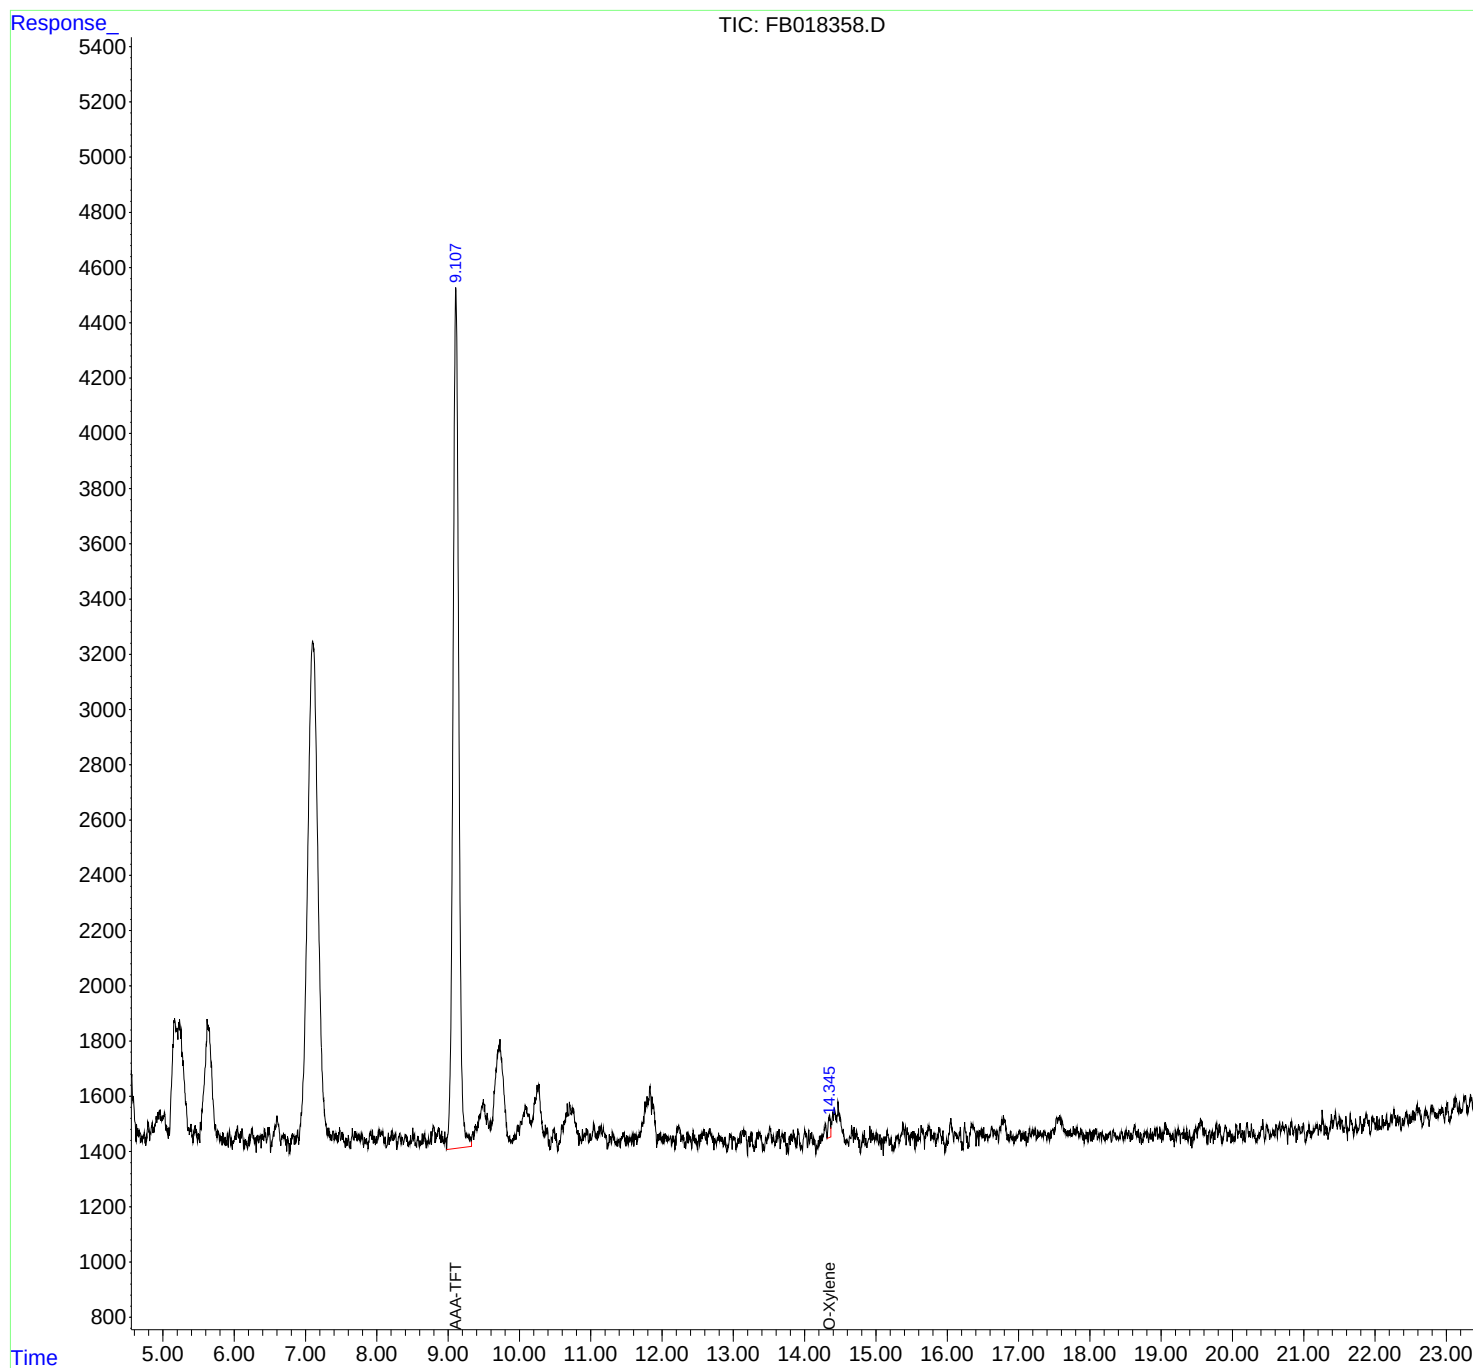

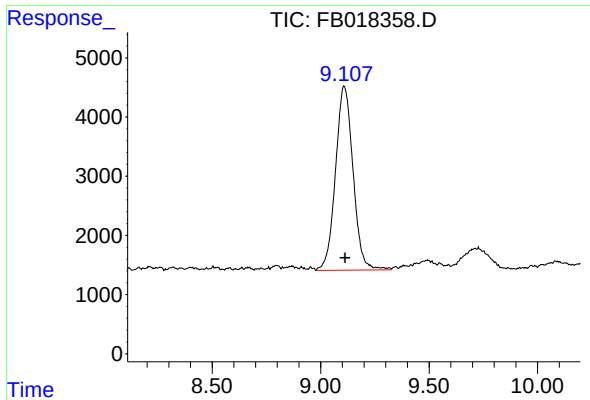

#5 AAA-TFT

R.T.: 9.108 min  
Delta R.T.: -0.004 min  
Response: 175110  
Conc: 20.33 ng/ml

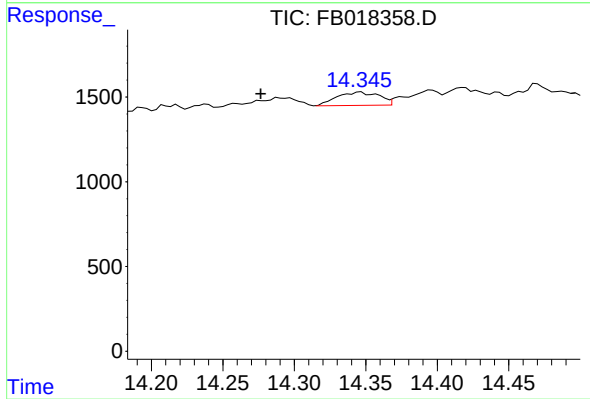

#9 O-Xylene

R.T.: 14.346 min  
Delta R.T.: 0.070 min  
Response: 1592  
Conc: 0.09 ng/ml