

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB102618\
 Data File : FB018352.D
 Signal(s) : FID2B.CH
 Acq On : 26 Oct 2018 9:35
 Operator : MJ/SJ
 Sample : BSF1026S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 04:03:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.110	173906	20.192 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.961	467772	30.585 ng/ml
2) t	2,2,4-Trimethylpentane	7.725	447539	30.287 ng/ml
3) t	n-Heptane	8.064	145666	10.279 ng/ml
4) t	Benzene	8.204	182548	9.799 ng/ml
6) t	Toluene	10.959	456086	29.926 ng/ml
7) t	Ethylbenzene	13.408	149447	9.420 ng/ml
8) t	m-Xylene	13.541	318148	19.121 ng/ml
9) t	O-Xylene	14.273	337883	18.951 ng/ml
10) t	1,2,4-Trimethylbenzene	16.556	405055	19.911 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB102618\
Data File : FB018352.D
Signal(s) : FID2B.CH
Acq On : 26 Oct 2018 9:35
Operator : MJ/SJ
Sample : BSF1026S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 04:03:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

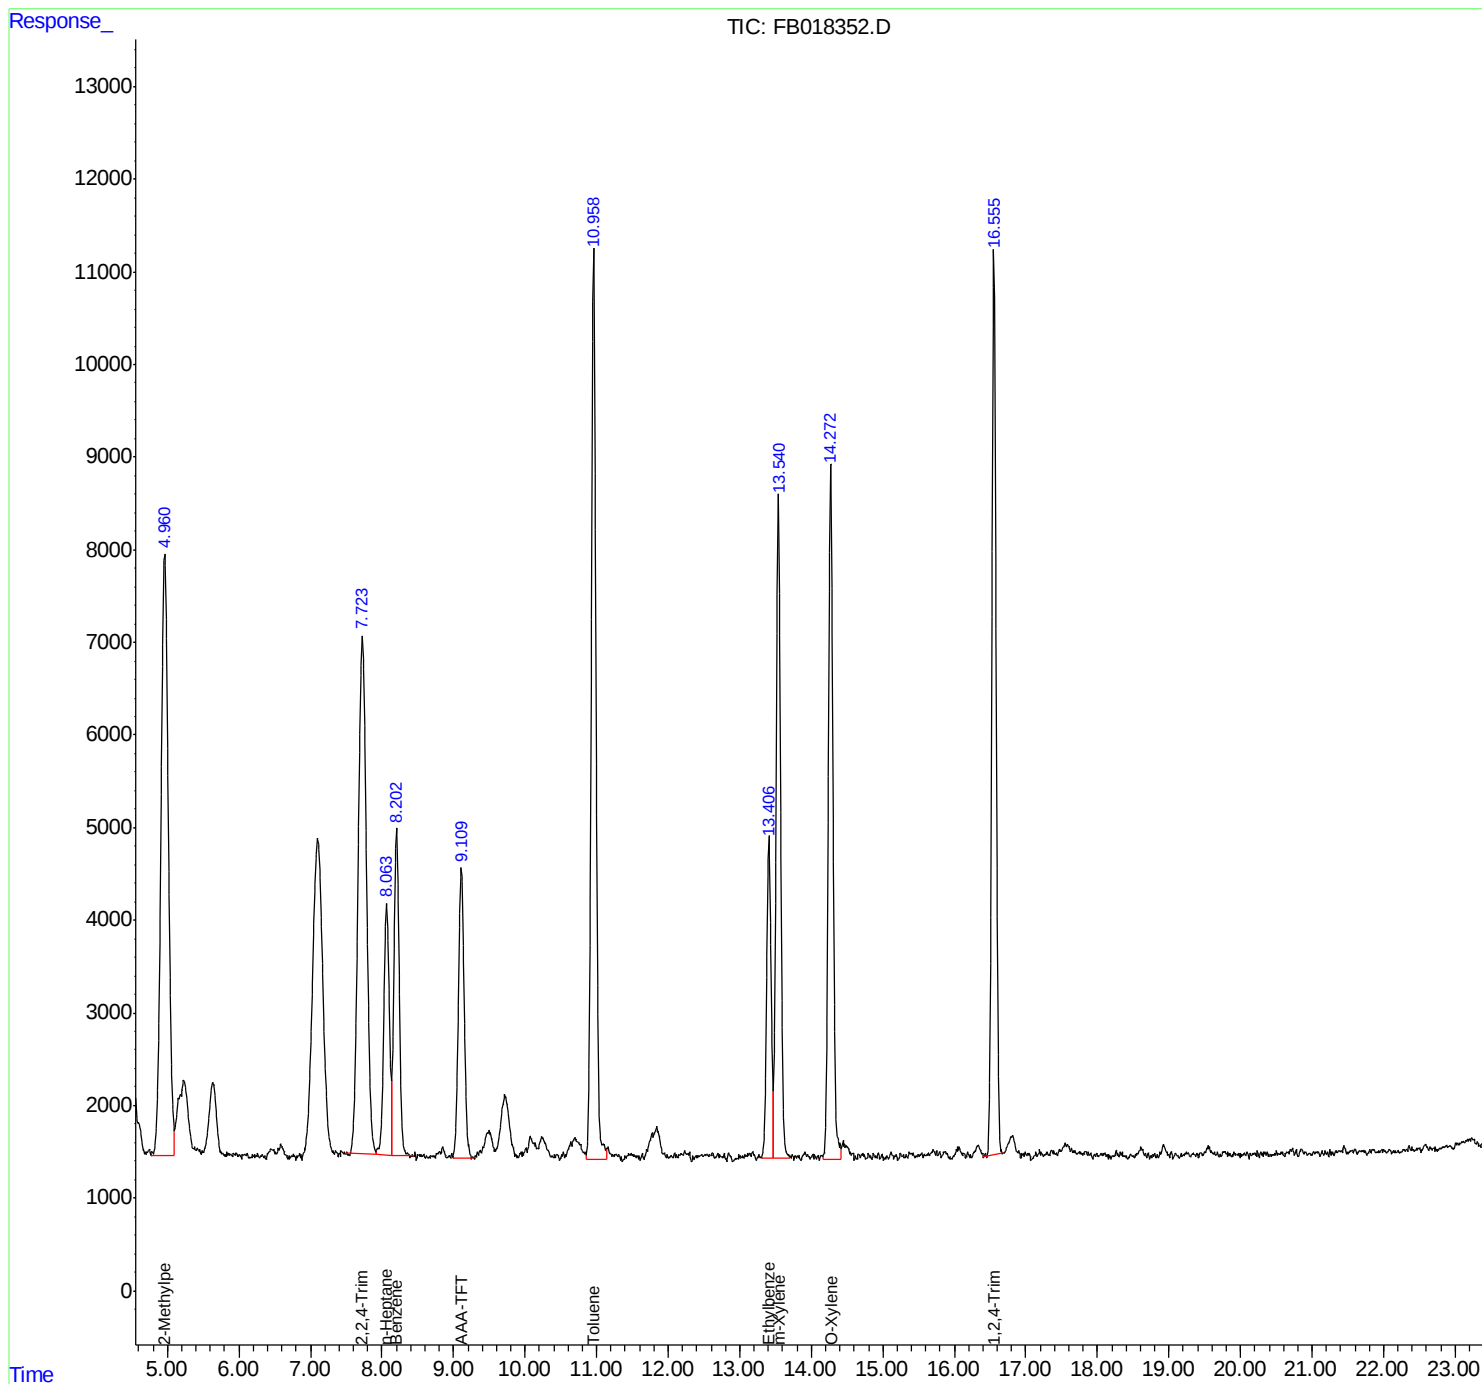

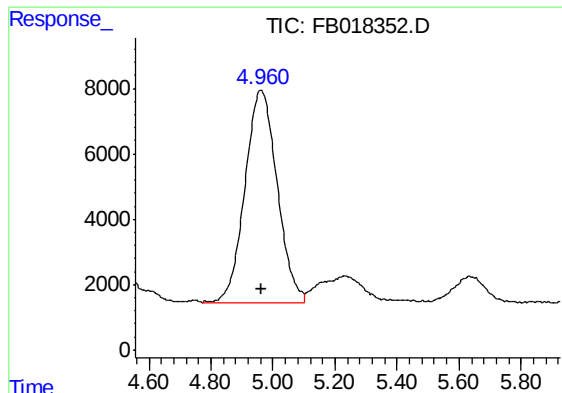


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: -0.004 min
Response: 467772
Conc: 30.58 ng/ml

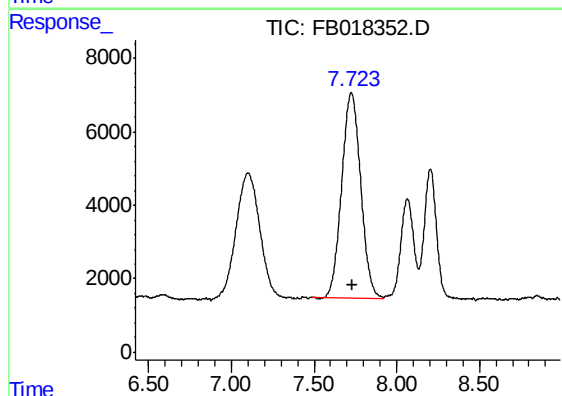


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.003 min
Response: 447539
Conc: 30.29 ng/ml

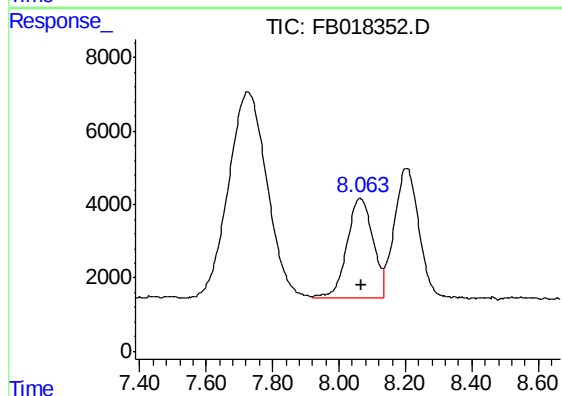


#3 n-Heptane

R.T.: 8.064 min
Delta R.T.: -0.003 min
Response: 145666
Conc: 10.28 ng/ml

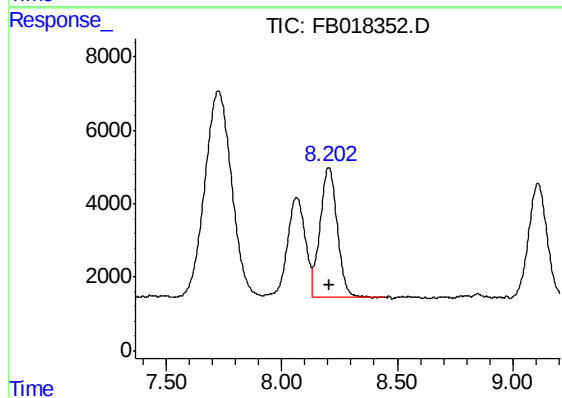


#4 Benzene

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 182548
Conc: 9.80 ng/ml

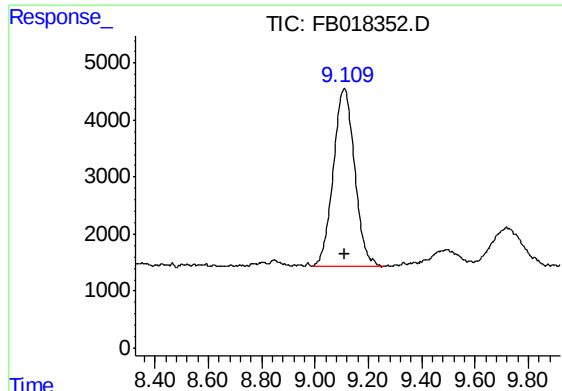


#5 AAA-TFT

R.T.: 9.110 min
Delta R.T.: -0.002 min
Response: 173906
Conc: 20.19 ng/ml

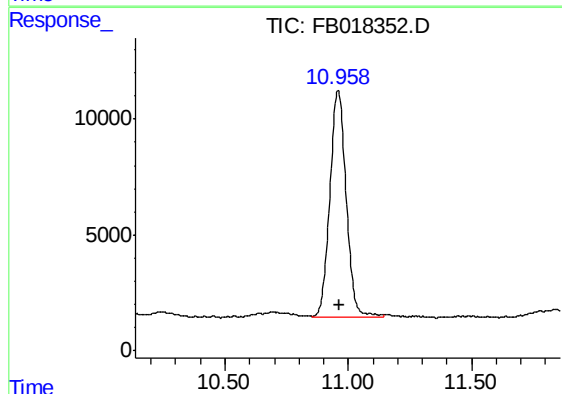


#6 Toluene

R.T.: 10.959 min
Delta R.T.: -0.003 min
Response: 456086
Conc: 29.93 ng/ml

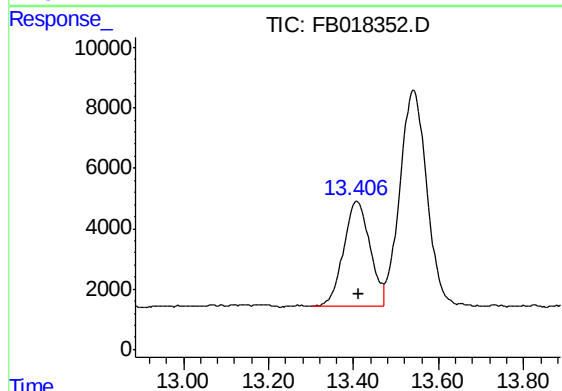


#7 Ethylbenzene

R.T.: 13.408 min
Delta R.T.: -0.004 min
Response: 149447
Conc: 9.42 ng/ml

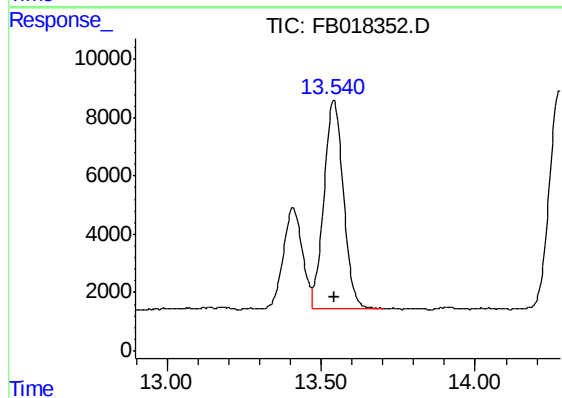


#8 m-Xylene

R.T.: 13.541 min
Delta R.T.: -0.003 min
Response: 318148
Conc: 19.12 ng/ml

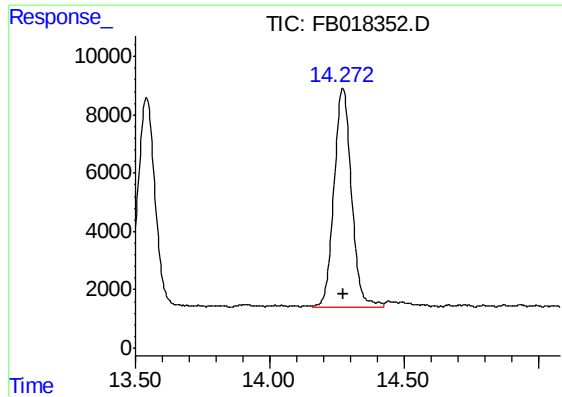

#9 O-Xylene

R.T.: 14.273 min
Delta R.T.: -0.003 min
Response: 337883
Conc: 18.95 ng/ml

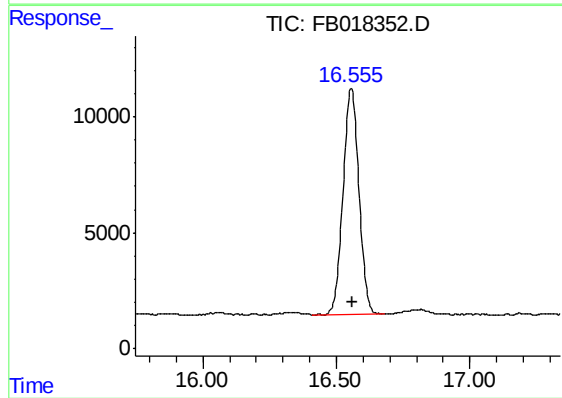

#10 1,2,4-Trimethylbenzene

R.T.: 16.556 min
Delta R.T.: -0.004 min
Response: 405055
Conc: 19.91 ng/ml