

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB102618\
 Data File : FB018365.D
 Signal(s) : FID2B.CH
 Acq On : 26 Oct 2018 16:10
 Operator : MJ/SJ
 Sample : J5688-02MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 16 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 04:04:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
 Quant Title :
 QLast Update : Fri Oct 12 08:04:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	180410	20.947 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.965	360136	23.547 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	319858	21.646 ng/ml
3) t n-Heptane	8.070	89646	6.326 ng/ml
4) t Benzene	8.207	177992	9.555 ng/ml
6) t Toluene	10.961	419505	27.525 ng/ml
7) t Ethylbenzene	13.411	131861	8.311 ng/ml
8) t m-Xylene	13.543	230710	13.866 ng/ml
9) t O-Xylene	14.275	303372	17.015 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	257289	12.647 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB102618\
Data File : FB018365.D
Signal(s) : FID2B.CH
Acq On : 26 Oct 2018 16:10
Operator : MJ/SJ
Sample : J5688-02MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 16 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 04:04:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101218.M
Quant Title :
QLast Update : Fri Oct 12 08:04:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

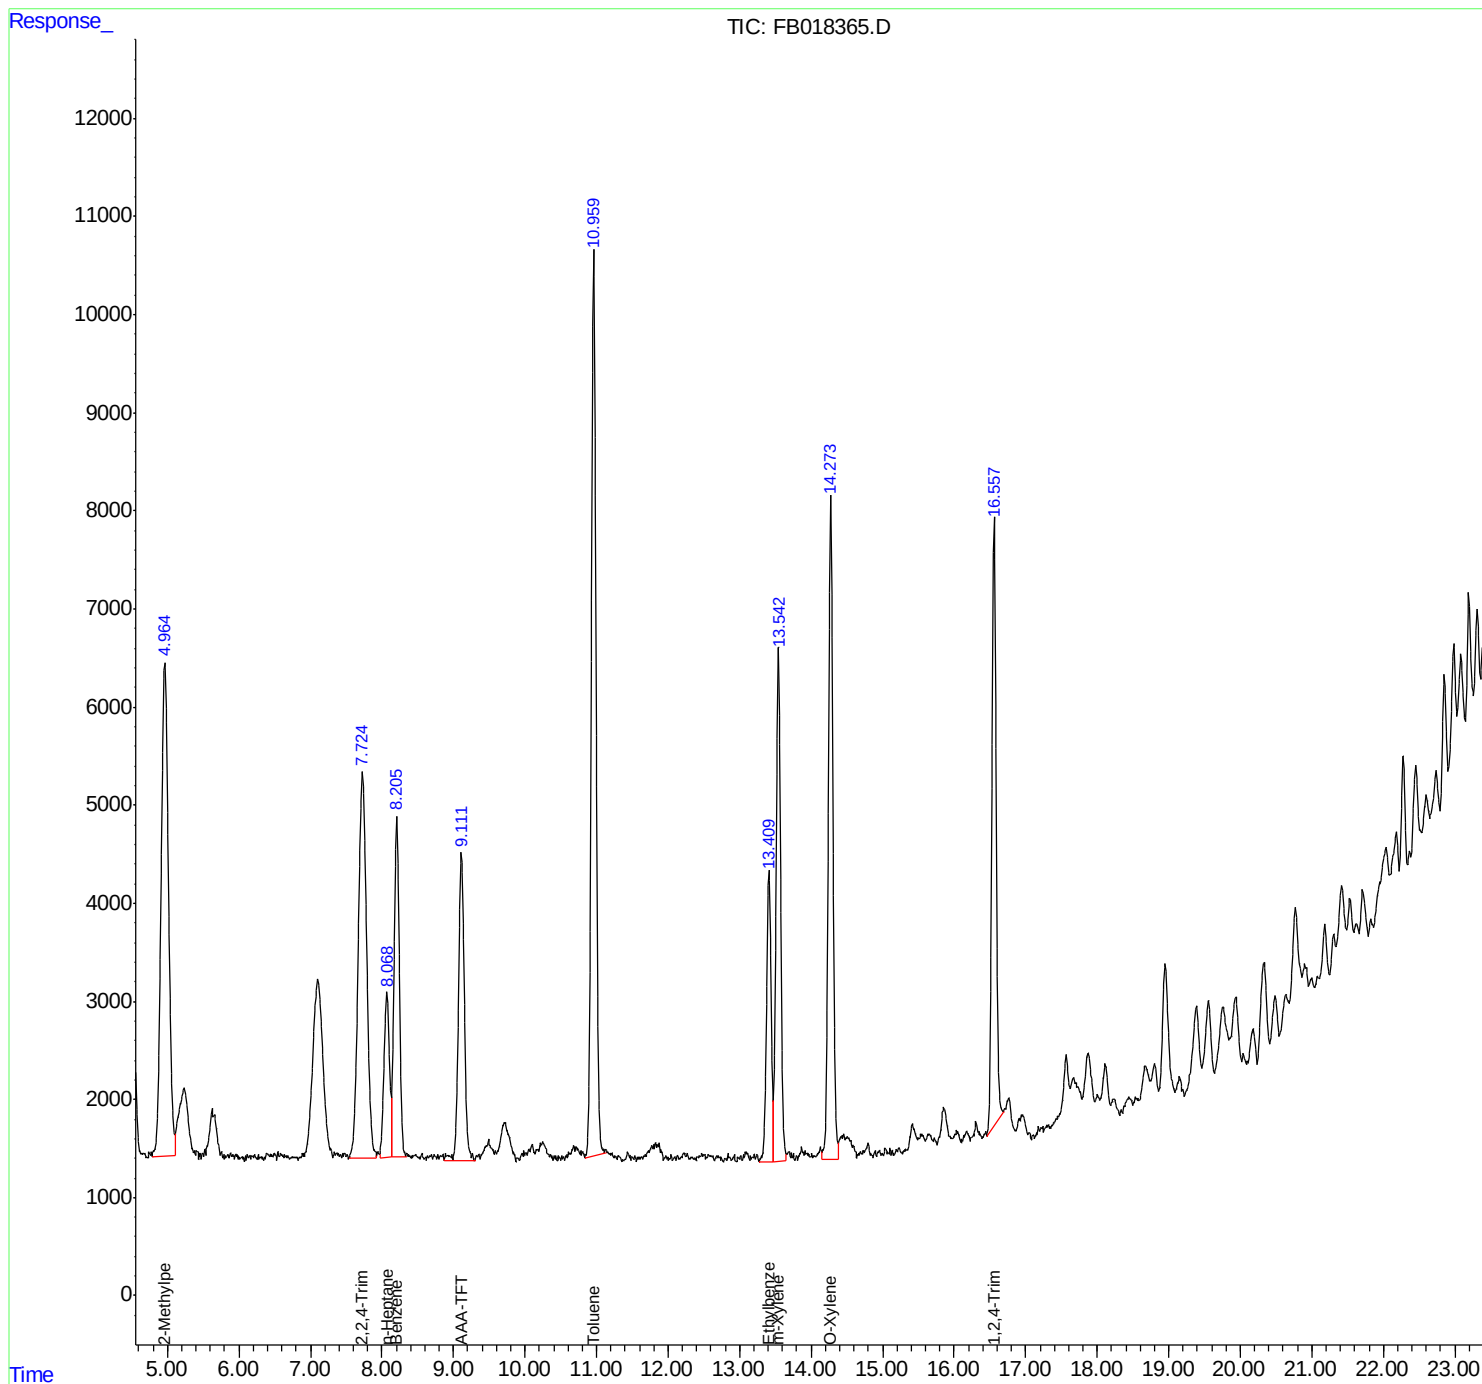

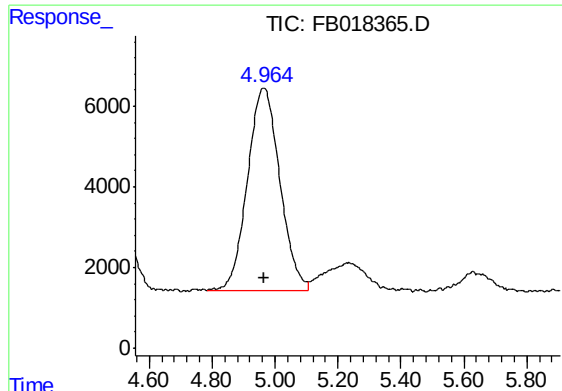


#1 2-Methylpentane

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 360136
Conc: 23.55 ng/ml

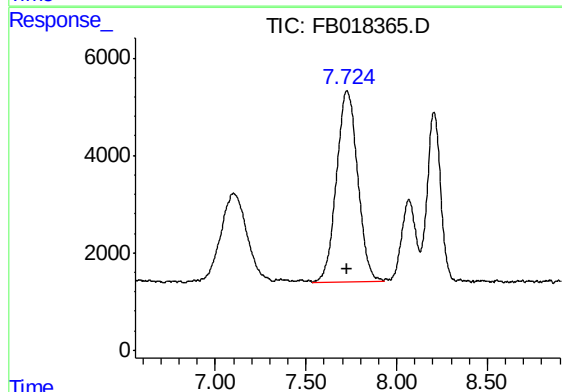


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: -0.002 min
Response: 319858
Conc: 21.65 ng/ml

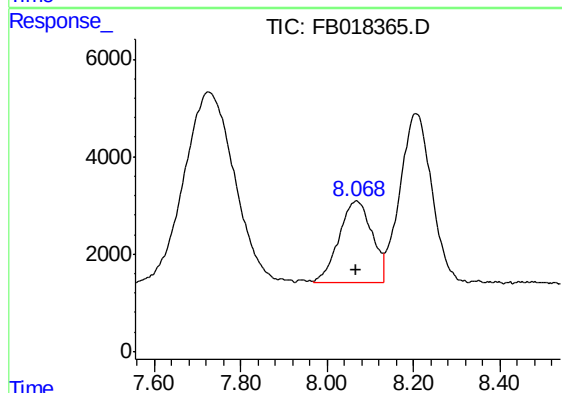


#3 n-Heptane

R.T.: 8.070 min
Delta R.T.: 0.002 min
Response: 89646
Conc: 6.33 ng/ml

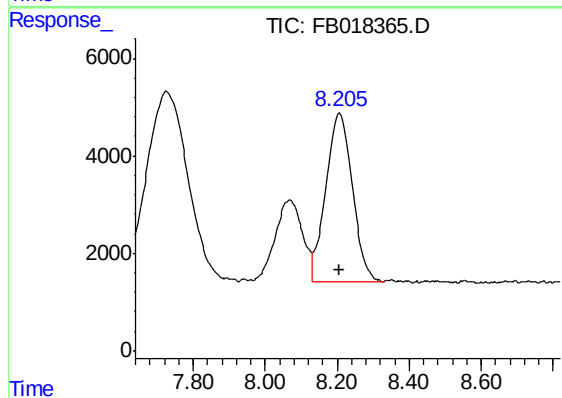


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 177992
Conc: 9.55 ng/ml

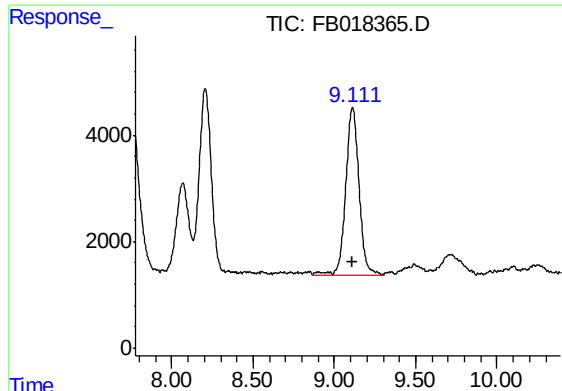


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 180410
Conc: 20.95 ng/ml

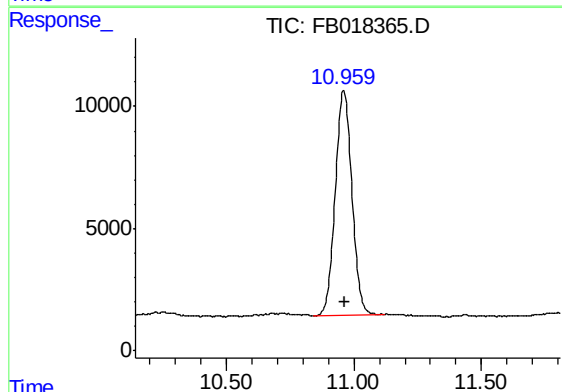


#6 Toluene

R.T.: 10.961 min
Delta R.T.: -0.001 min
Response: 419505
Conc: 27.53 ng/ml

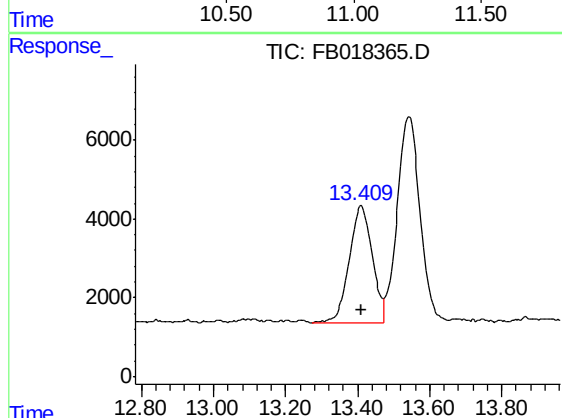


#7 Ethylbenzene

R.T.: 13.411 min
Delta R.T.: -0.002 min
Response: 131861
Conc: 8.31 ng/ml

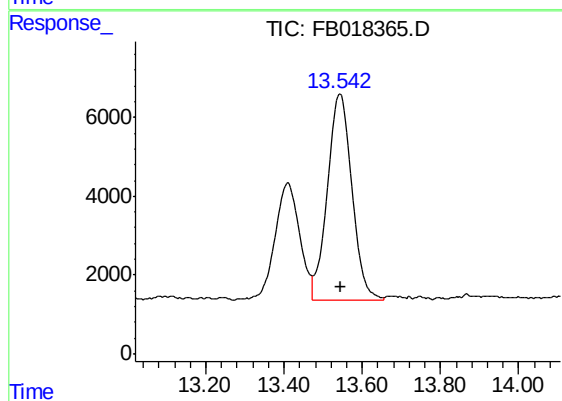


#8 m-Xylene

R.T.: 13.543 min
Delta R.T.: -0.001 min
Response: 230710
Conc: 13.87 ng/ml

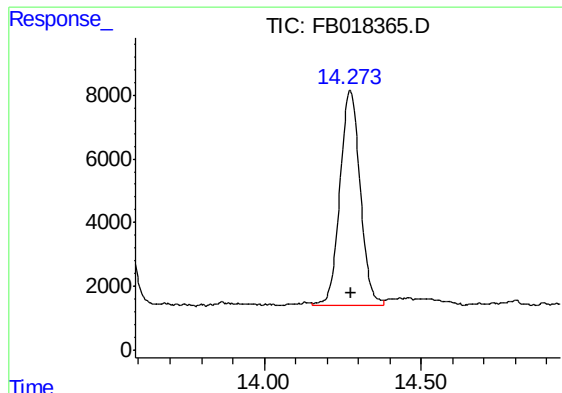

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: -0.002 min
Response: 303372
Conc: 17.01 ng/ml

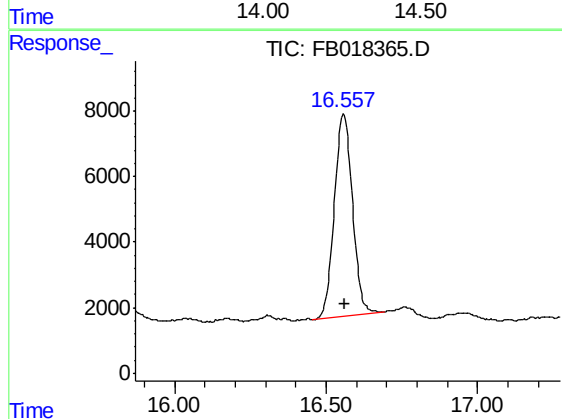

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: -0.002 min
Response: 257289
Conc: 12.65 ng/ml