

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102720\
 Data File : FB025147.D
 Signal(s) : FID2B.CH
 Acq On : 27 Oct 2020 13:03
 Operator : DD/AJ
 Sample : L4219-18MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 27 14:48:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	530819	24.865 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	1007010	33.109 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1001588	32.152 ng/ml
3) t n-Heptane	7.757	323031	10.507 ng/ml
4) t Benzene	7.893	432190	11.500 ng/ml
6) t Toluene	10.631	1194466	33.516 ng/ml
7) t Ethylbenzene	13.070	363986	11.182 ng/ml
8) t m-Xylene	13.204	723815	22.569 ng/ml
9) t O-Xylene	13.931	704213	22.844 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	574228	21.994 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102720\
Data File : FB025147.D
Signal(s) : FID2B.CH
Acq On : 27 Oct 2020 13:03
Operator : DD/AJ
Sample : L4219-18MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 27 14:48:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

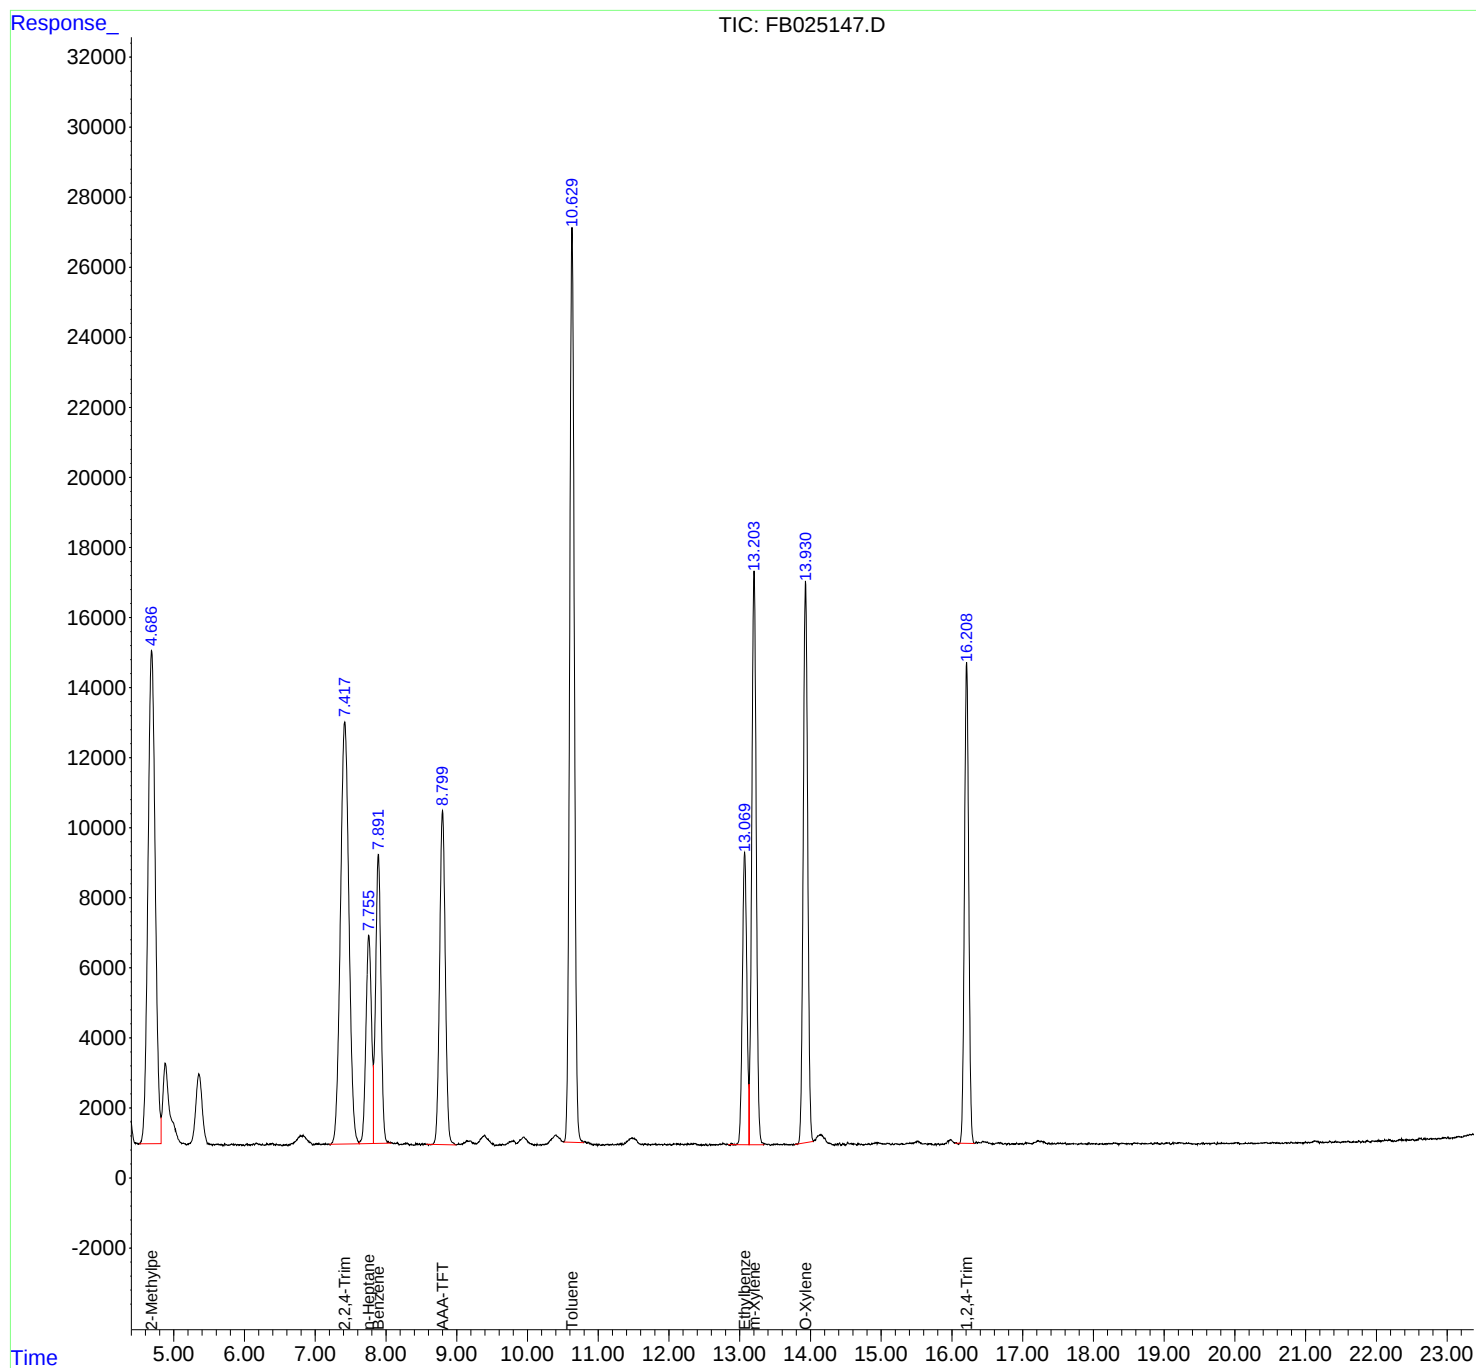

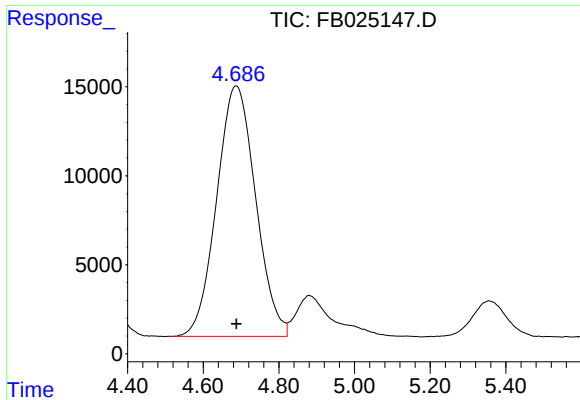


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 1007010
Conc: 33.11 ng/ml

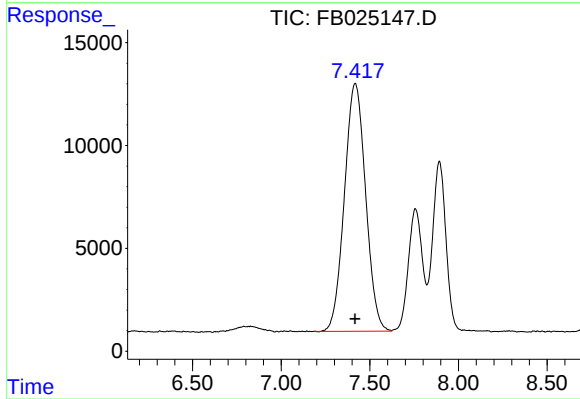


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1001588
Conc: 32.15 ng/ml

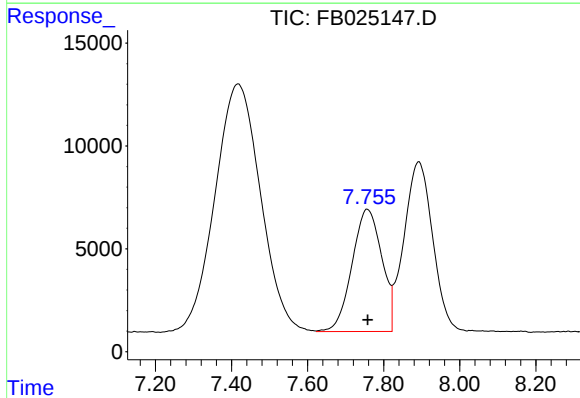


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.001 min
Response: 323031
Conc: 10.51 ng/ml

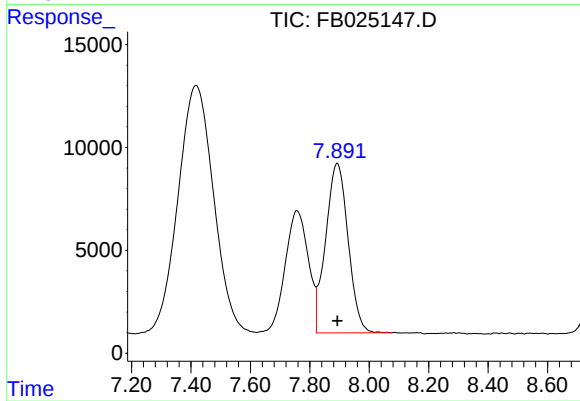


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 432190
Conc: 11.50 ng/ml

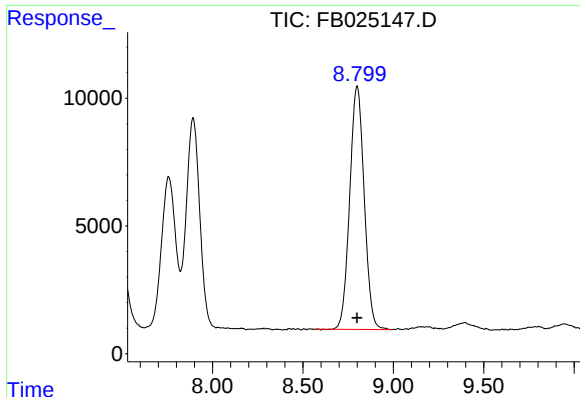


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 530819
Conc: 24.87 ng/ml

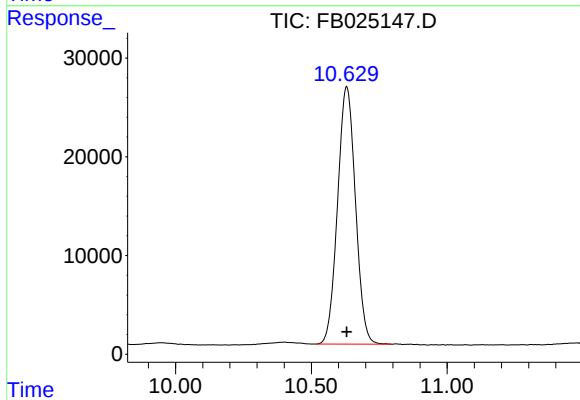


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1194466
Conc: 33.52 ng/ml

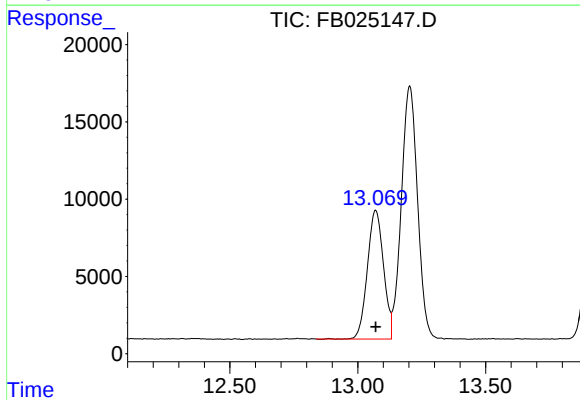


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 363986
Conc: 11.18 ng/ml

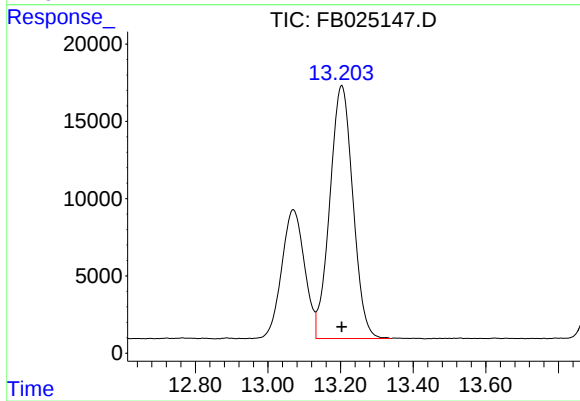


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 723815
Conc: 22.57 ng/ml

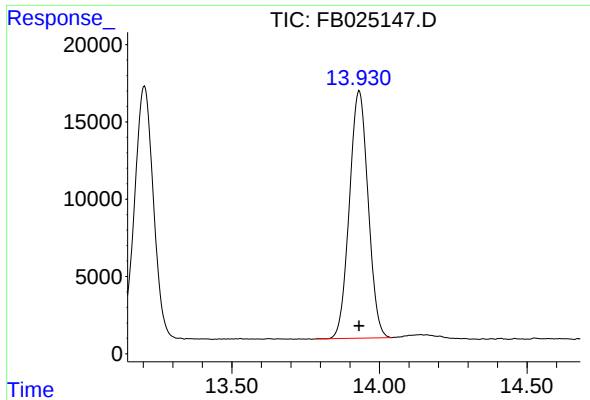

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 704213
Conc: 22.84 ng/ml

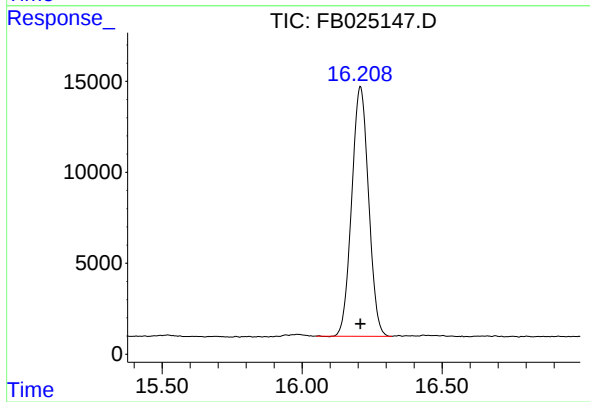

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 574228
Conc: 21.99 ng/ml