

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102720\
 Data File : FB025144.D
 Signal(s) : FID2B.CH
 Acq On : 27 Oct 2020 11:26
 Operator : DD/AJ
 Sample : BSF1027S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 27 14:47:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	435030	20.378 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	888307	29.206 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	948372	30.443 ng/ml
3) t n-Heptane	7.757	310588	10.102 ng/ml
4) t Benzene	7.892	376878	10.028 ng/ml
6) t Toluene	10.630	1073150	30.112 ng/ml
7) t Ethylbenzene	13.070	333284	10.239 ng/ml
8) t m-Xylene	13.203	663045	20.674 ng/ml
9) t O-Xylene	13.930	640952	20.792 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	543661	20.823 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102720\
Data File : FB025144.D
Signal(s) : FID2B.CH
Acq On : 27 Oct 2020 11:26
Operator : DD/AJ
Sample : BSF1027S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 27 14:47:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

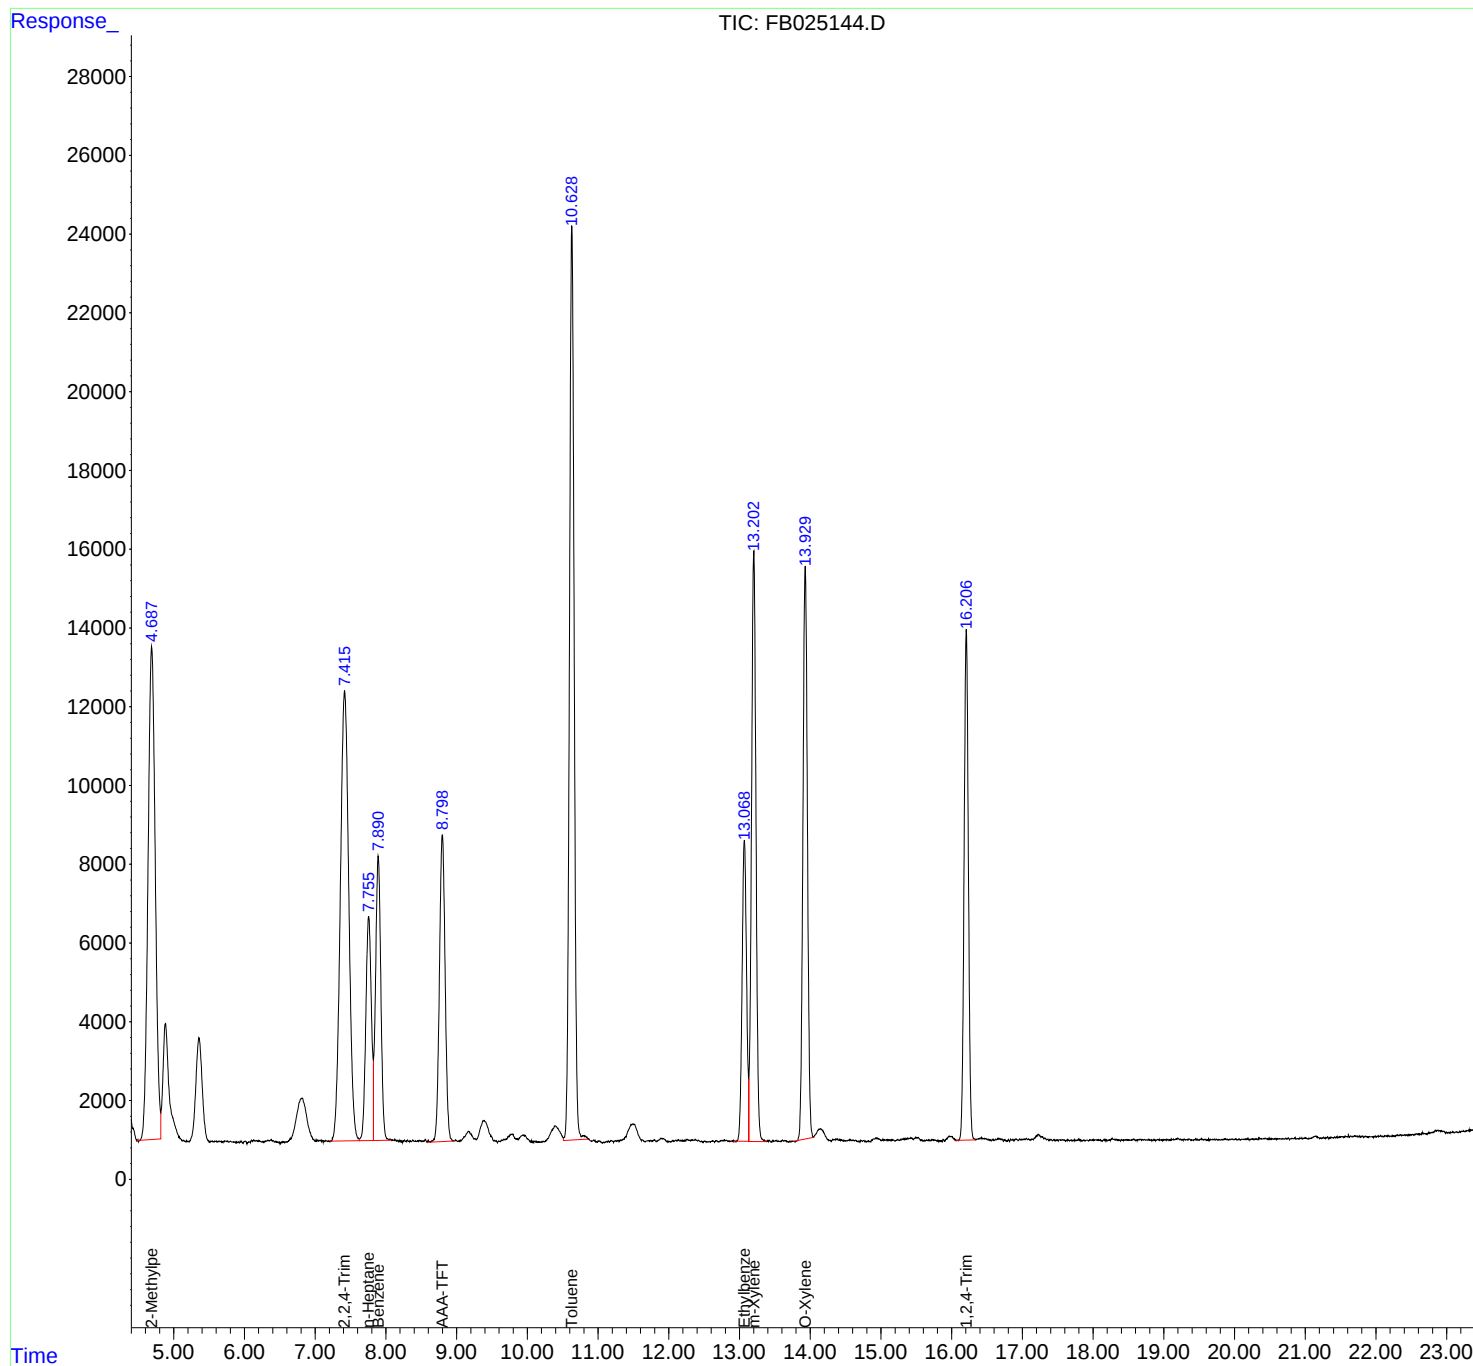

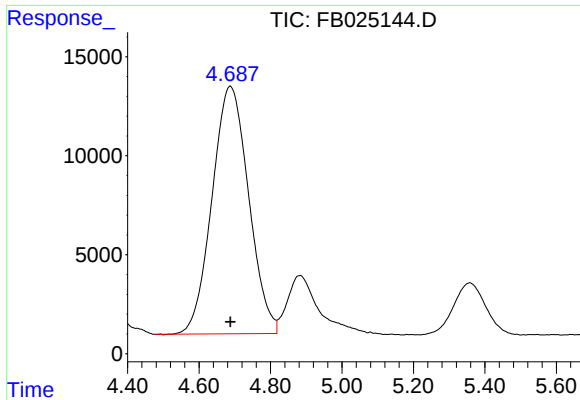


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 888307
Conc: 29.21 ng/ml

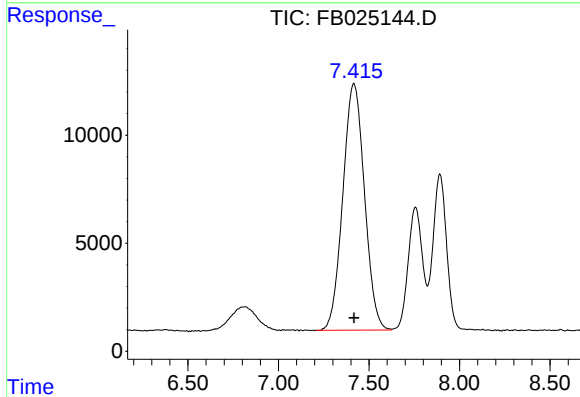


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 948372
Conc: 30.44 ng/ml

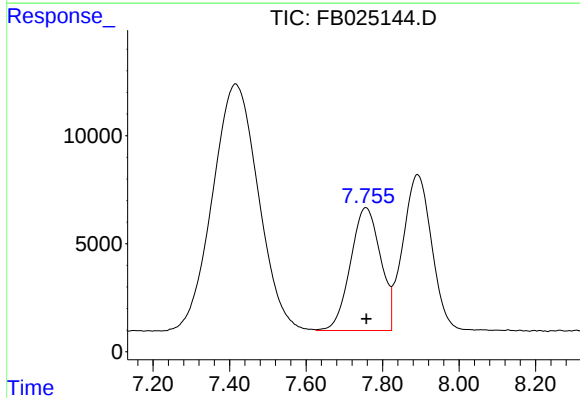


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 310588
Conc: 10.10 ng/ml

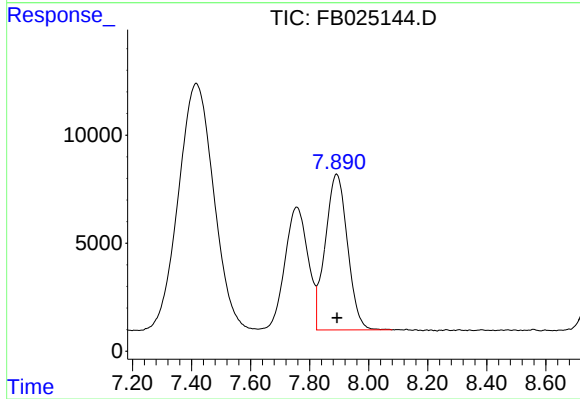


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.001 min
Response: 376878
Conc: 10.03 ng/ml

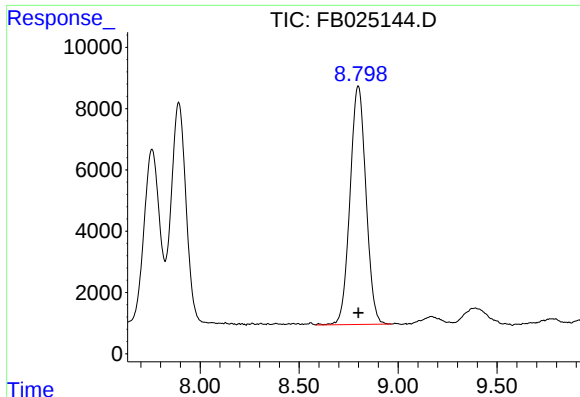


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 435030
Conc: 20.38 ng/ml

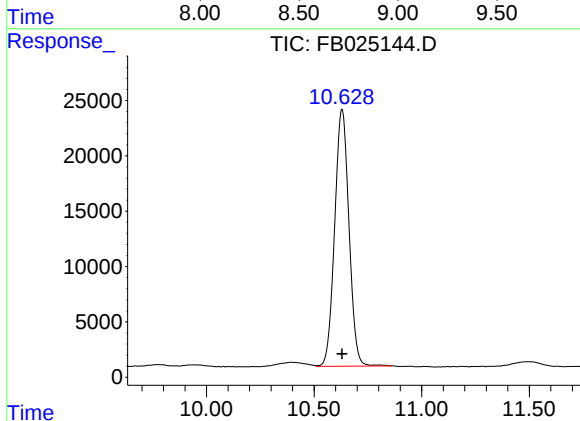


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1073150
Conc: 30.11 ng/ml

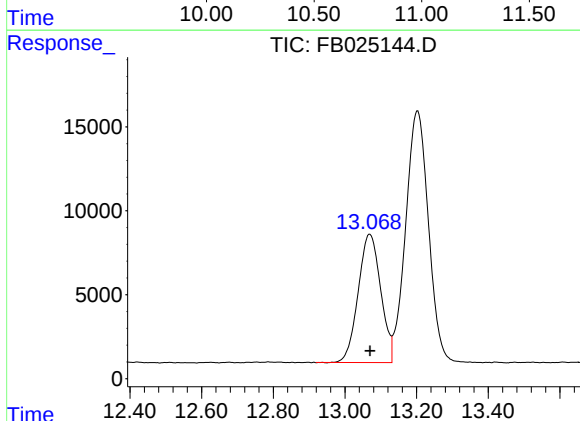


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 333284
Conc: 10.24 ng/ml

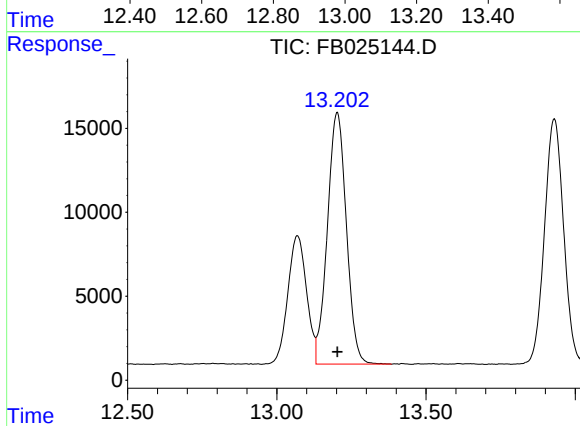


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 663045
Conc: 20.67 ng/ml

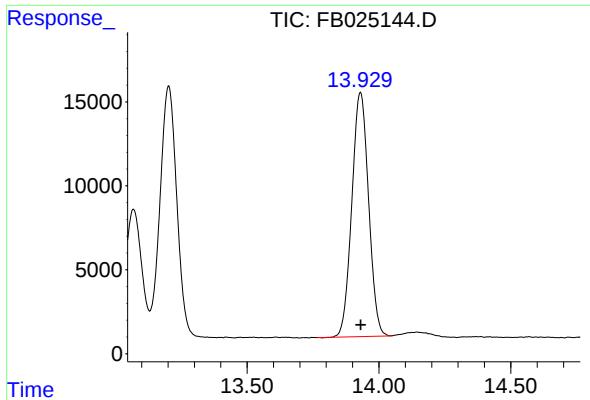

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 640952
Conc: 20.79 ng/ml

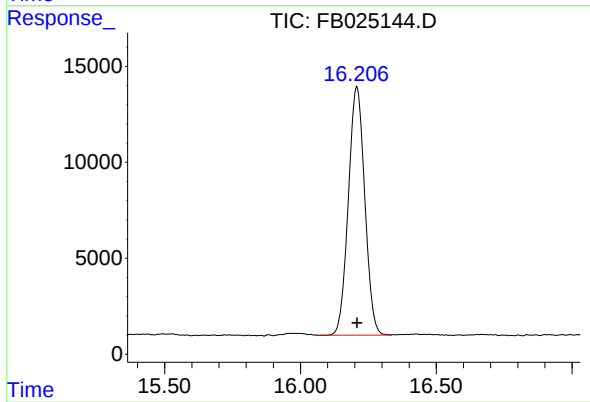

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.000 min
Response: 543661
Conc: 20.82 ng/ml