

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102720\
 Data File : FB025148.D
 Signal(s) : FID2B.CH
 Acq On : 27 Oct 2020 13:34
 Operator : DD/AJ
 Sample : L4219-18MSD
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 27 14:48:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
 Quant Title :
 QLast Update : Mon Oct 19 13:01:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	527927	24.730 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	951917	31.298 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	923210	29.636 ng/ml
3) t n-Heptane	7.758	289118	9.404 ng/ml
4) t Benzene	7.892	423883	11.279 ng/ml
6) t Toluene	10.632	1165052	32.691 ng/ml
7) t Ethylbenzene	13.071	350641	10.772 ng/ml
8) t m-Xylene	13.204	695476	21.686 ng/ml
9) t O-Xylene	13.932	678146	21.999 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	543325	20.810 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102720\
Data File : FB025148.D
Signal(s) : FID2B.CH
Acq On : 27 Oct 2020 13:34
Operator : DD/AJ
Sample : L4219-18MSD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 27 14:48:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101920.M
Quant Title :
QLast Update : Mon Oct 19 13:01:11 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

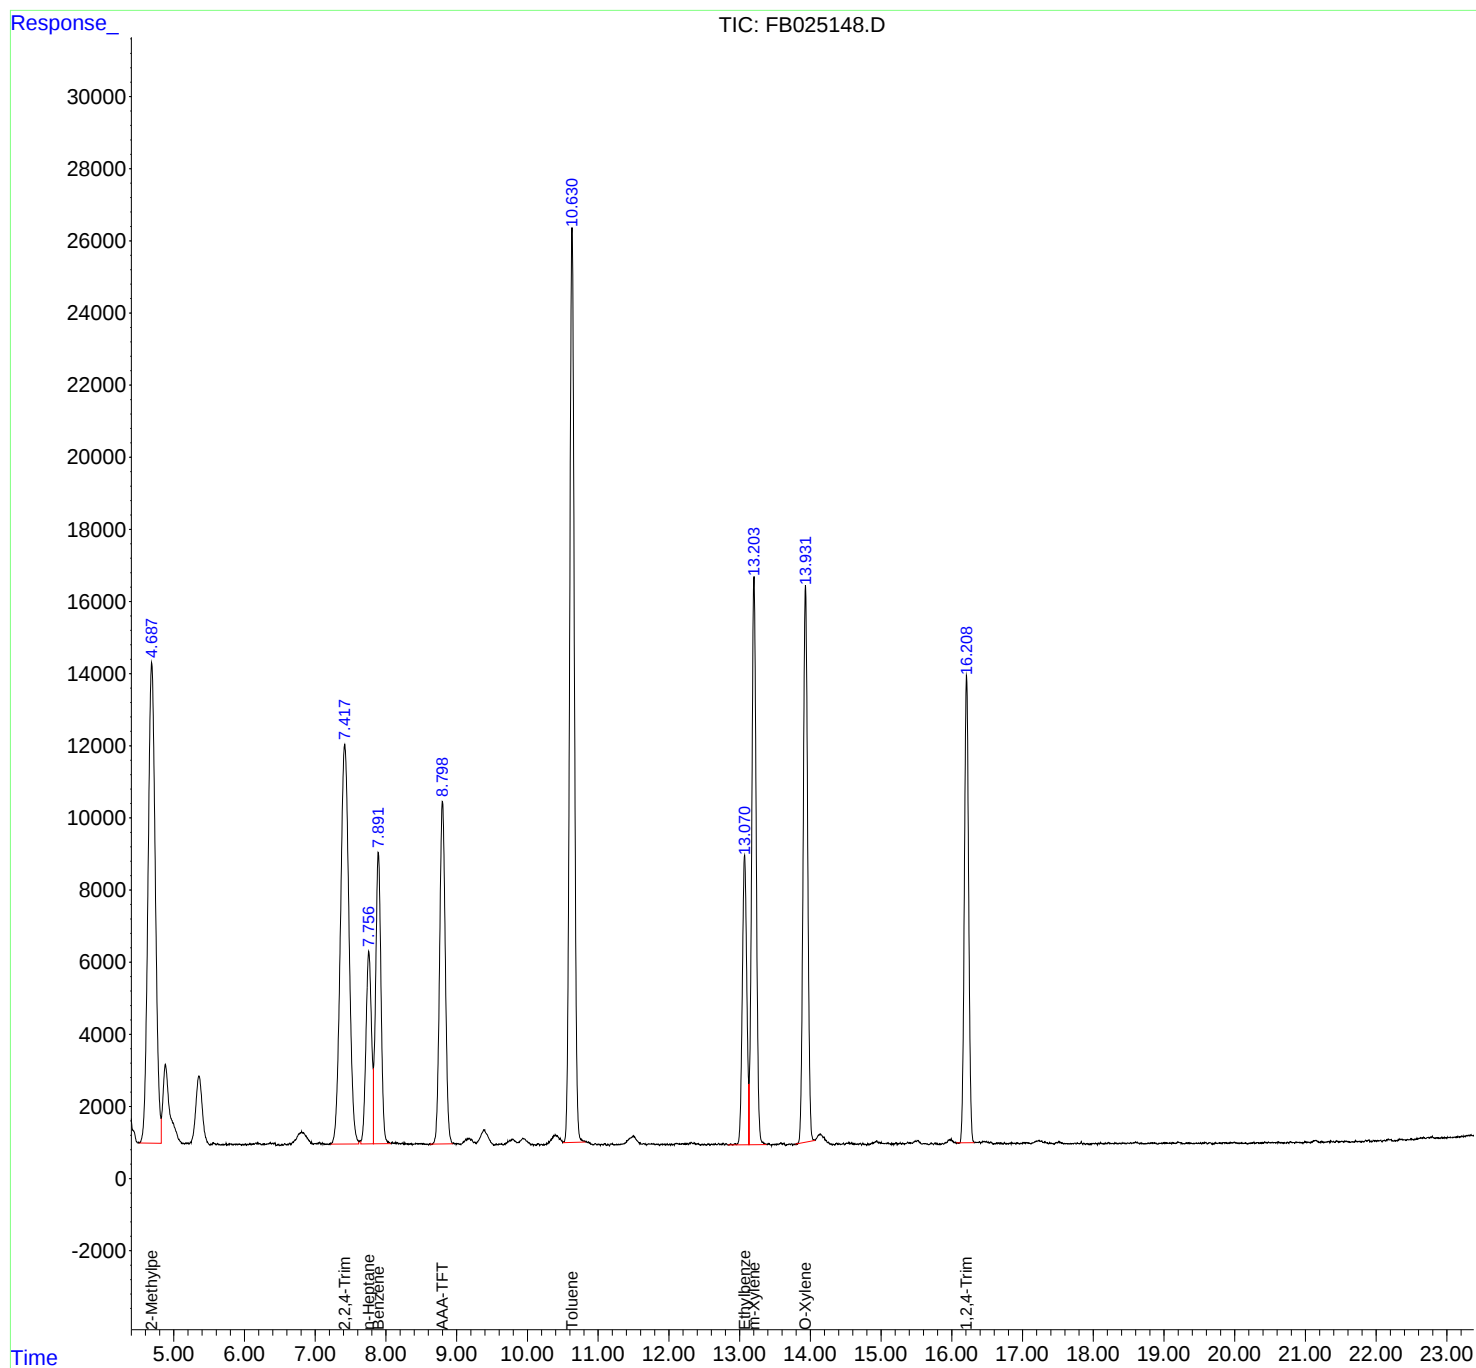

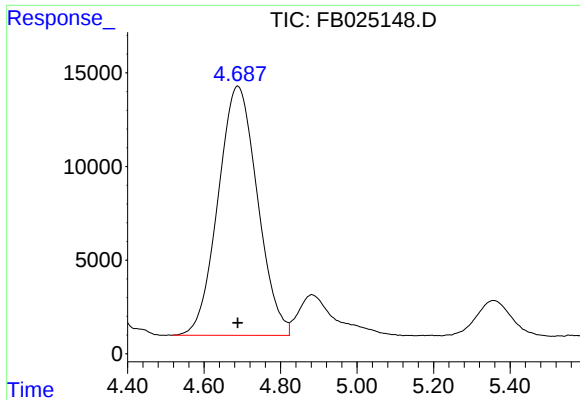


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 951917
Conc: 31.30 ng/ml

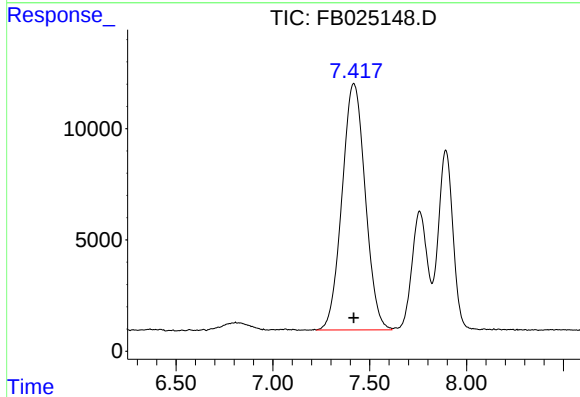


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 923210
Conc: 29.64 ng/ml

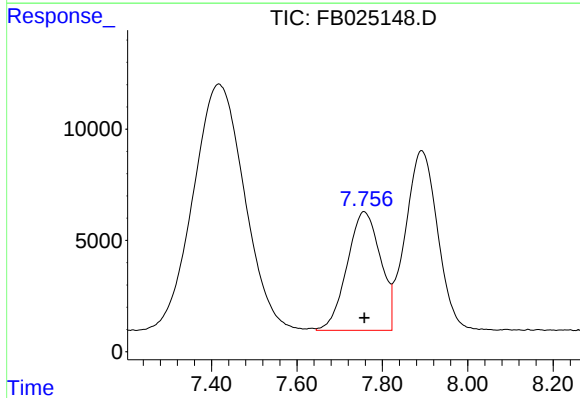


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 289118
Conc: 9.40 ng/ml

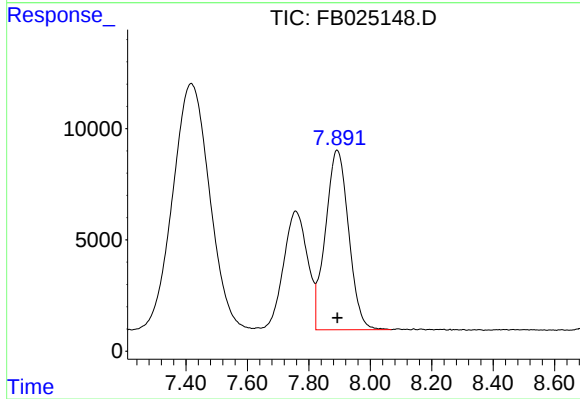


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 423883
Conc: 11.28 ng/ml

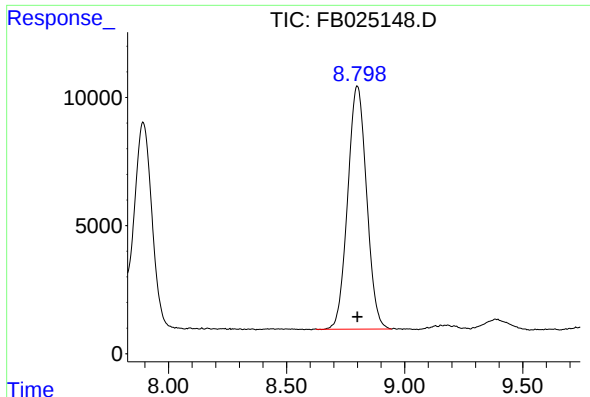


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 527927
Conc: 24.73 ng/ml

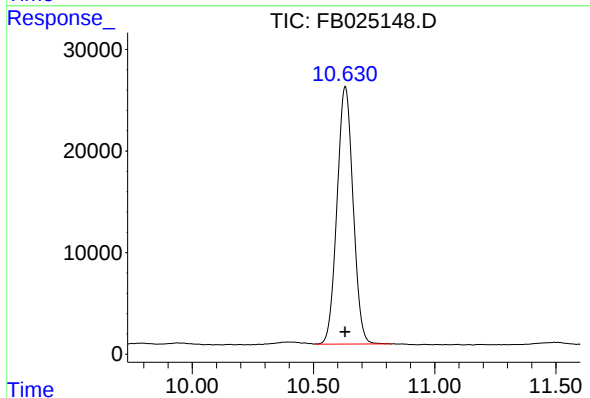


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1165052
Conc: 32.69 ng/ml

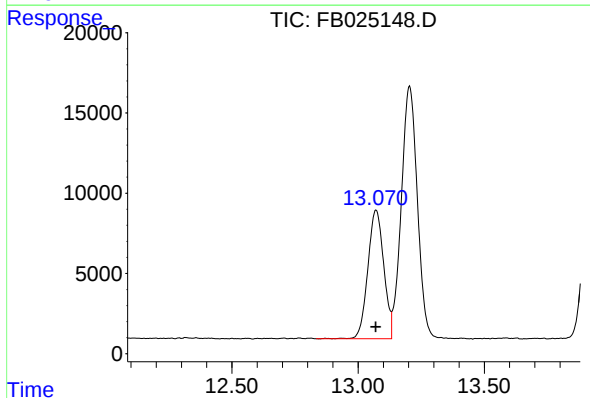


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 350641
Conc: 10.77 ng/ml

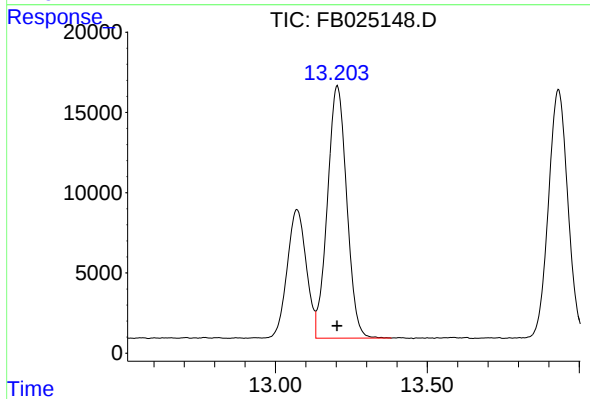


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 695476
Conc: 21.69 ng/ml

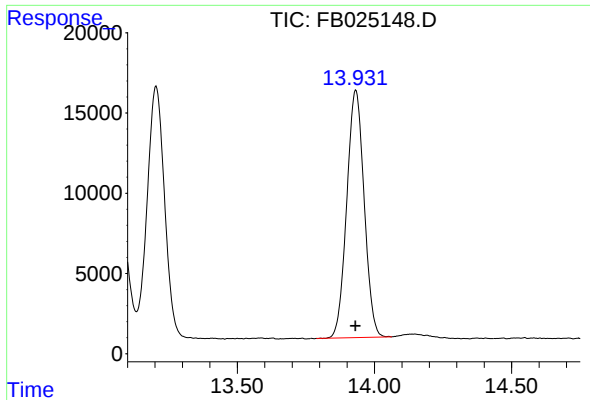

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.001 min
Response: 678146
Conc: 22.00 ng/ml

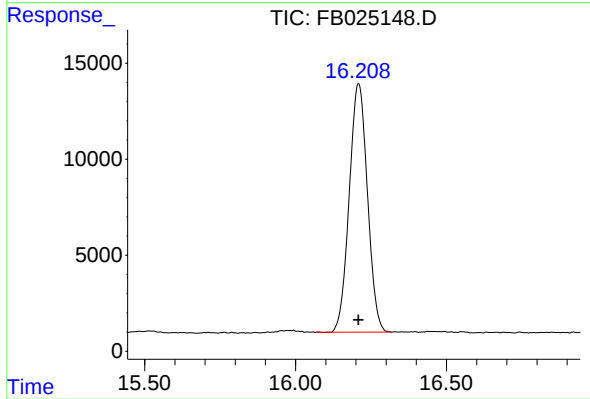

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.001 min
Response: 543325
Conc: 20.81 ng/ml