

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102721\
 Data File : FB026315.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2021 00:23
 Operator : AJ/MA
 Sample : M4068-01
 Misc : 5.01G\5.00 ML DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 28 08:57:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	120118	10.139 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.697	18953	1.138 ng/ml
2) t 2,2,4-Trimethylpentane	7.469	4601	0.236 ng/ml
3) t n-Heptane	7.761	8602	0.466 ng/ml
4) t Benzene	7.894	1349	0.062 ng/ml
6) t Toluene	10.630	30251	1.459 ng/ml
7) t Ethylbenzene	13.072	9926	0.526 ng/ml
8) t m-Xylene	13.203	19070	1.003 ng/ml
9) t O-Xylene	13.934	19691	1.066 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	22087	1.165 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102721\
Data File : FB026315.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2021 00:23
Operator : AJ/MA
Sample : M4068-01
Misc : 5.01G\5.00 ML DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 28 08:57:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

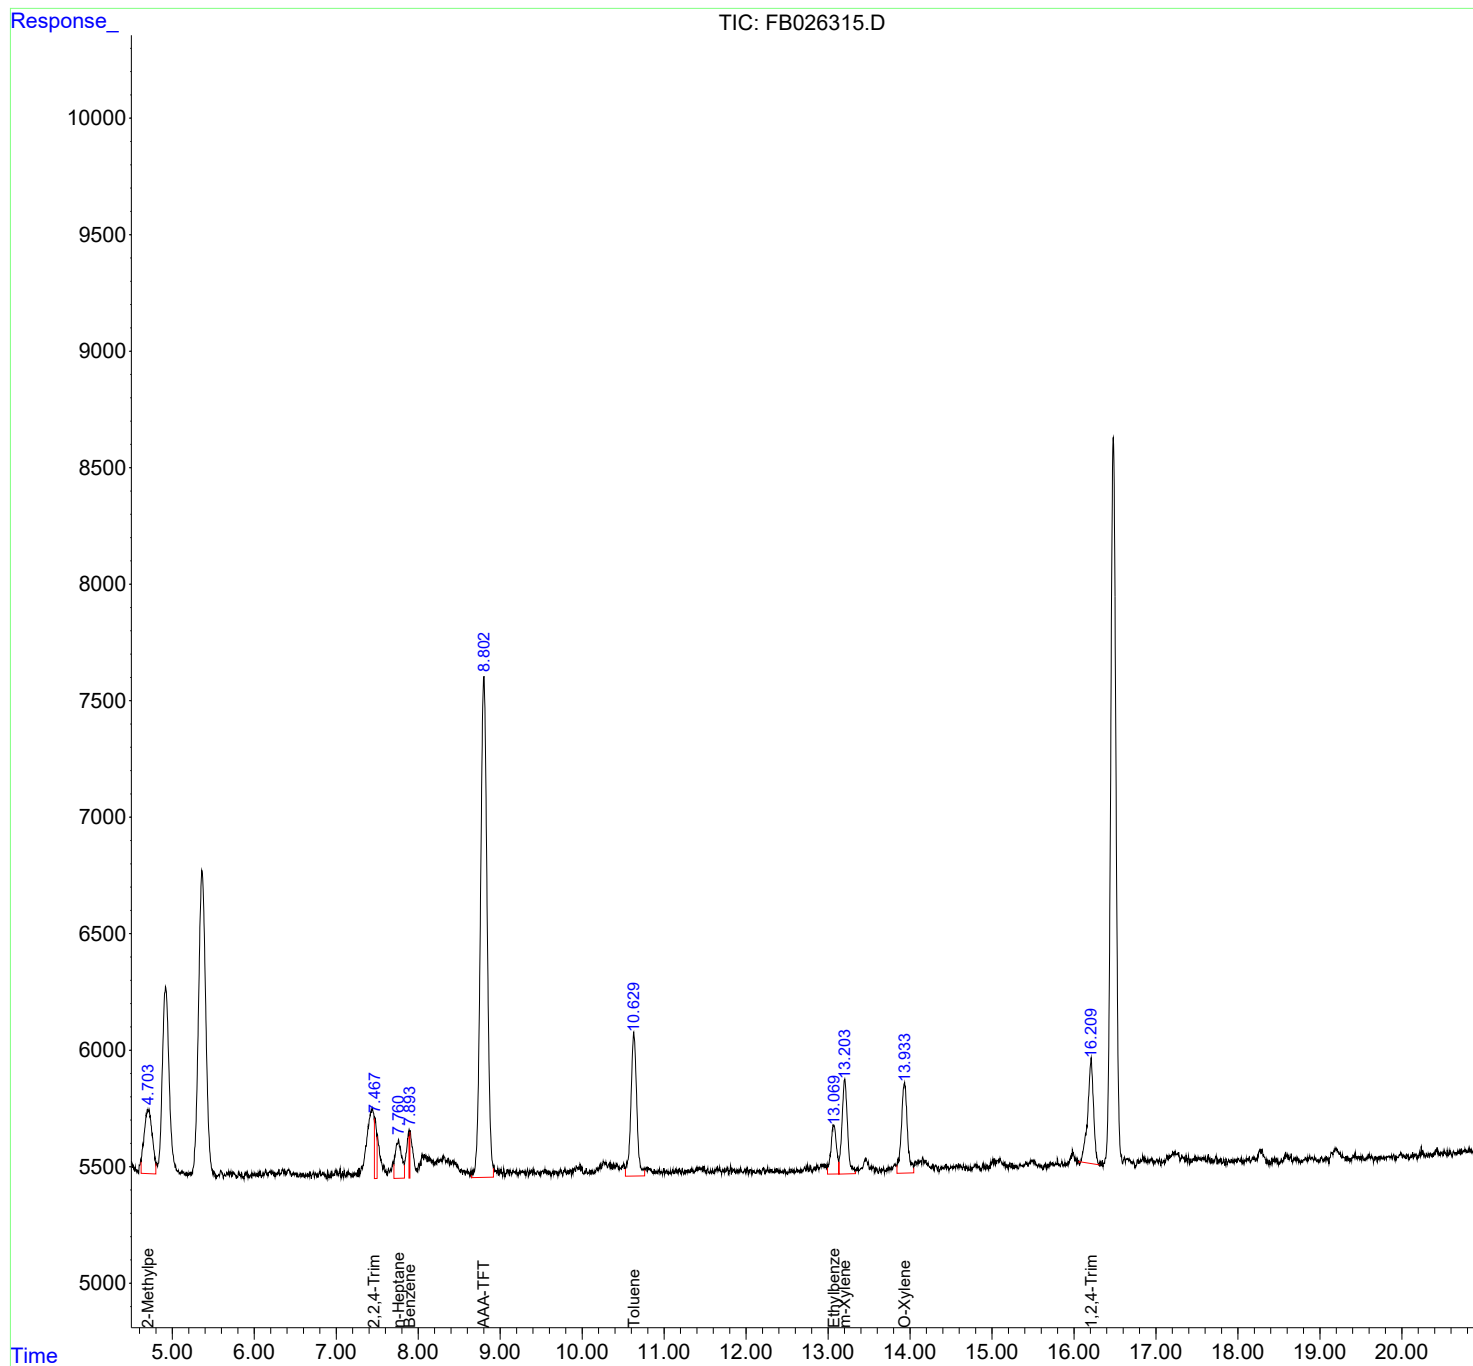


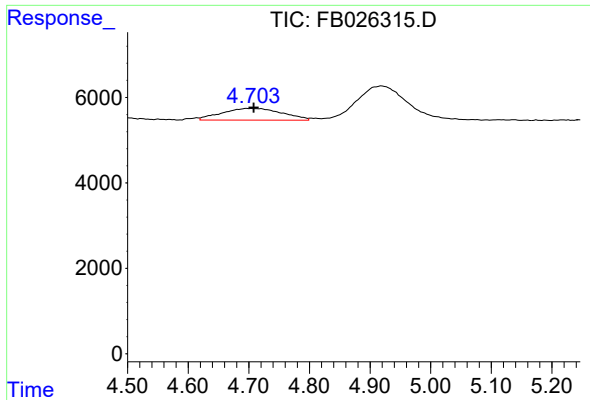

#1 2-Methylpentane


R.T.: 4.697 min
Delta R.T.: -0.011 min
Response: 18953
Conc: 1.14 ng/ml

Instrument :
FID_B
ClientSampleId :

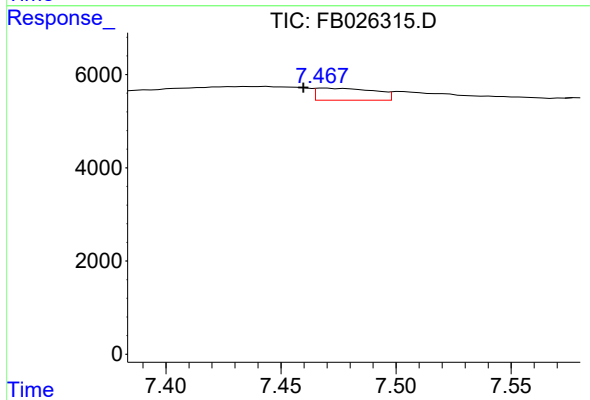


#2 2,2,4-Trimethylpentane

R.T.: 7.469 min
Delta R.T.: 0.010 min
Response: 4601
Conc: 0.24 ng/ml

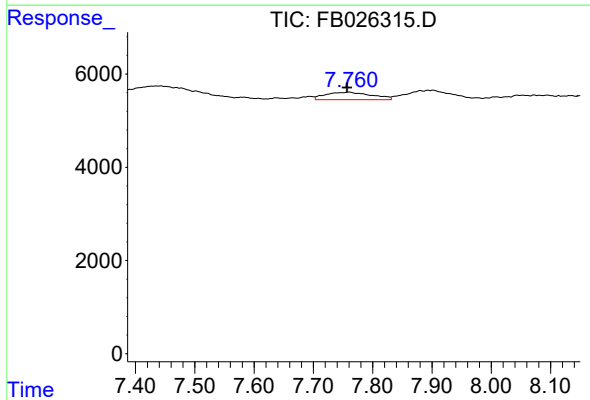


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.004 min
Response: 8602
Conc: 0.47 ng/ml

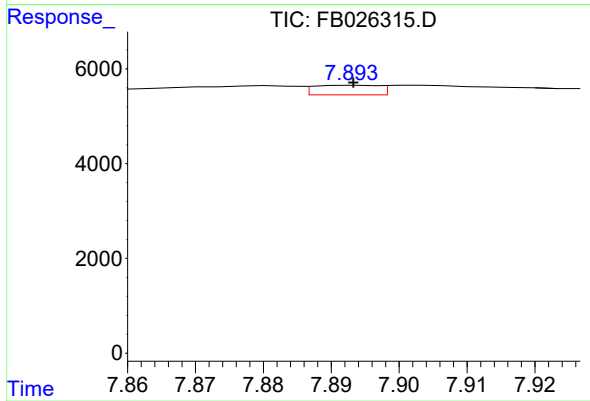

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 1349
Conc: 0.06 ng/ml

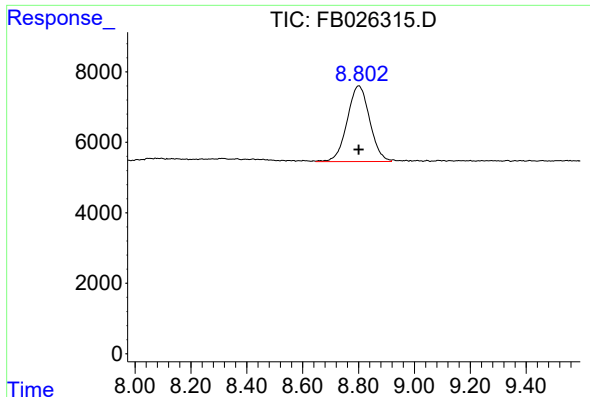

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.002 min
Response: 120118
Conc: 10.14 ng/ml

Instrument :
FID_B
ClientSampleId :

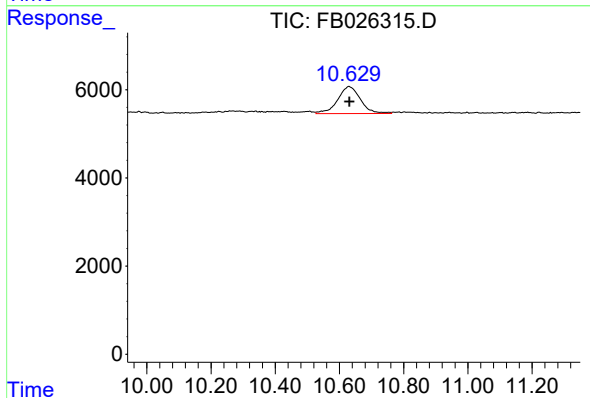


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 30251
Conc: 1.46 ng/ml

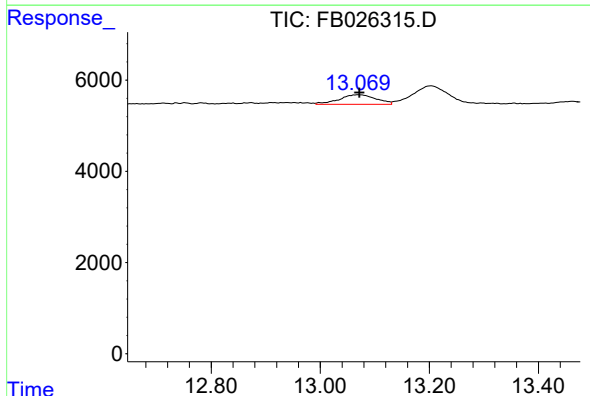


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 9926
Conc: 0.53 ng/ml

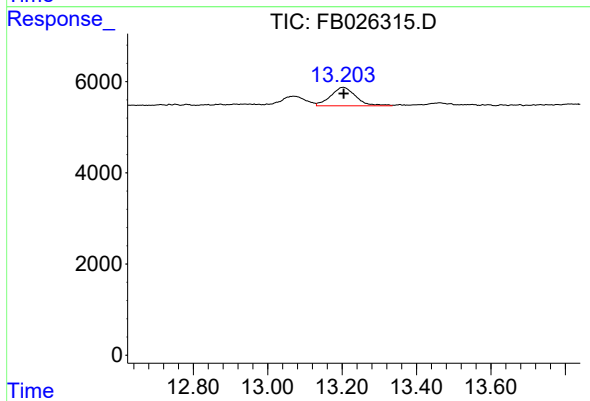

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.001 min
Response: 19070
Conc: 1.00 ng/ml

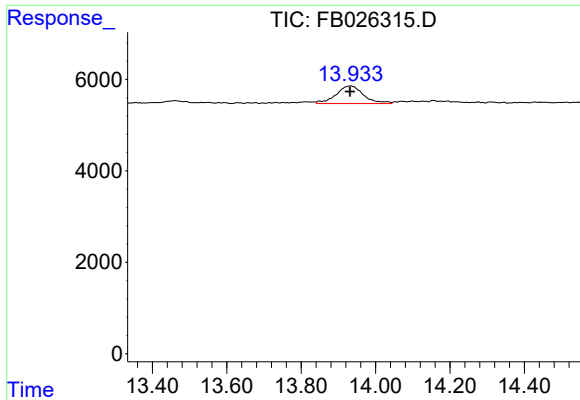

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.002 min
Response: 19691
Conc: 1.07 ng/ml

Instrument :
FID_B
ClientSampleId :

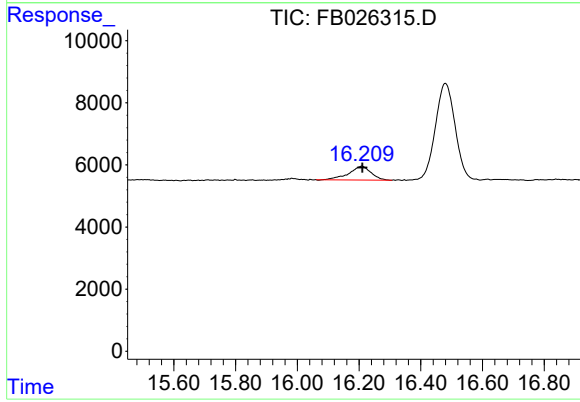

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 22087
Conc: 1.17 ng/ml