

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102721\
 Data File : FB026311.D
 Signal(s) : FID2B.CH
 Acq On : 27 Oct 2021 21:58
 Operator : AJ/MA
 Sample : BSF1027S1
 Misc : 4.99G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1027S1

Integration File: Calibration.e
 Quant Time: Oct 28 05:45:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	232848	19.655 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	526130	31.598 ng/ml
2) t 2,2,4-Trimethylpentane	7.455	620988	31.847 ng/ml
3) t n-Heptane	7.757	194860	10.561 ng/ml
4) t Benzene	7.894	231544	10.621 ng/ml
6) t Toluene	10.631	660357	31.838 ng/ml
7) t Ethylbenzene	13.071	200865	10.637 ng/ml
8) t m-Xylene	13.204	403911	21.236 ng/ml
9) t O-Xylene	13.932	393967	21.330 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	402101	21.210 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102721\
Data File : FB026311.D
Signal(s) : FID2B.CH
Acq On : 27 Oct 2021 21:58
Operator : AJ/MA
Sample : BSF1027S1
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1027S1

Integration File: Calibration.e
Quant Time: Oct 28 05:45:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

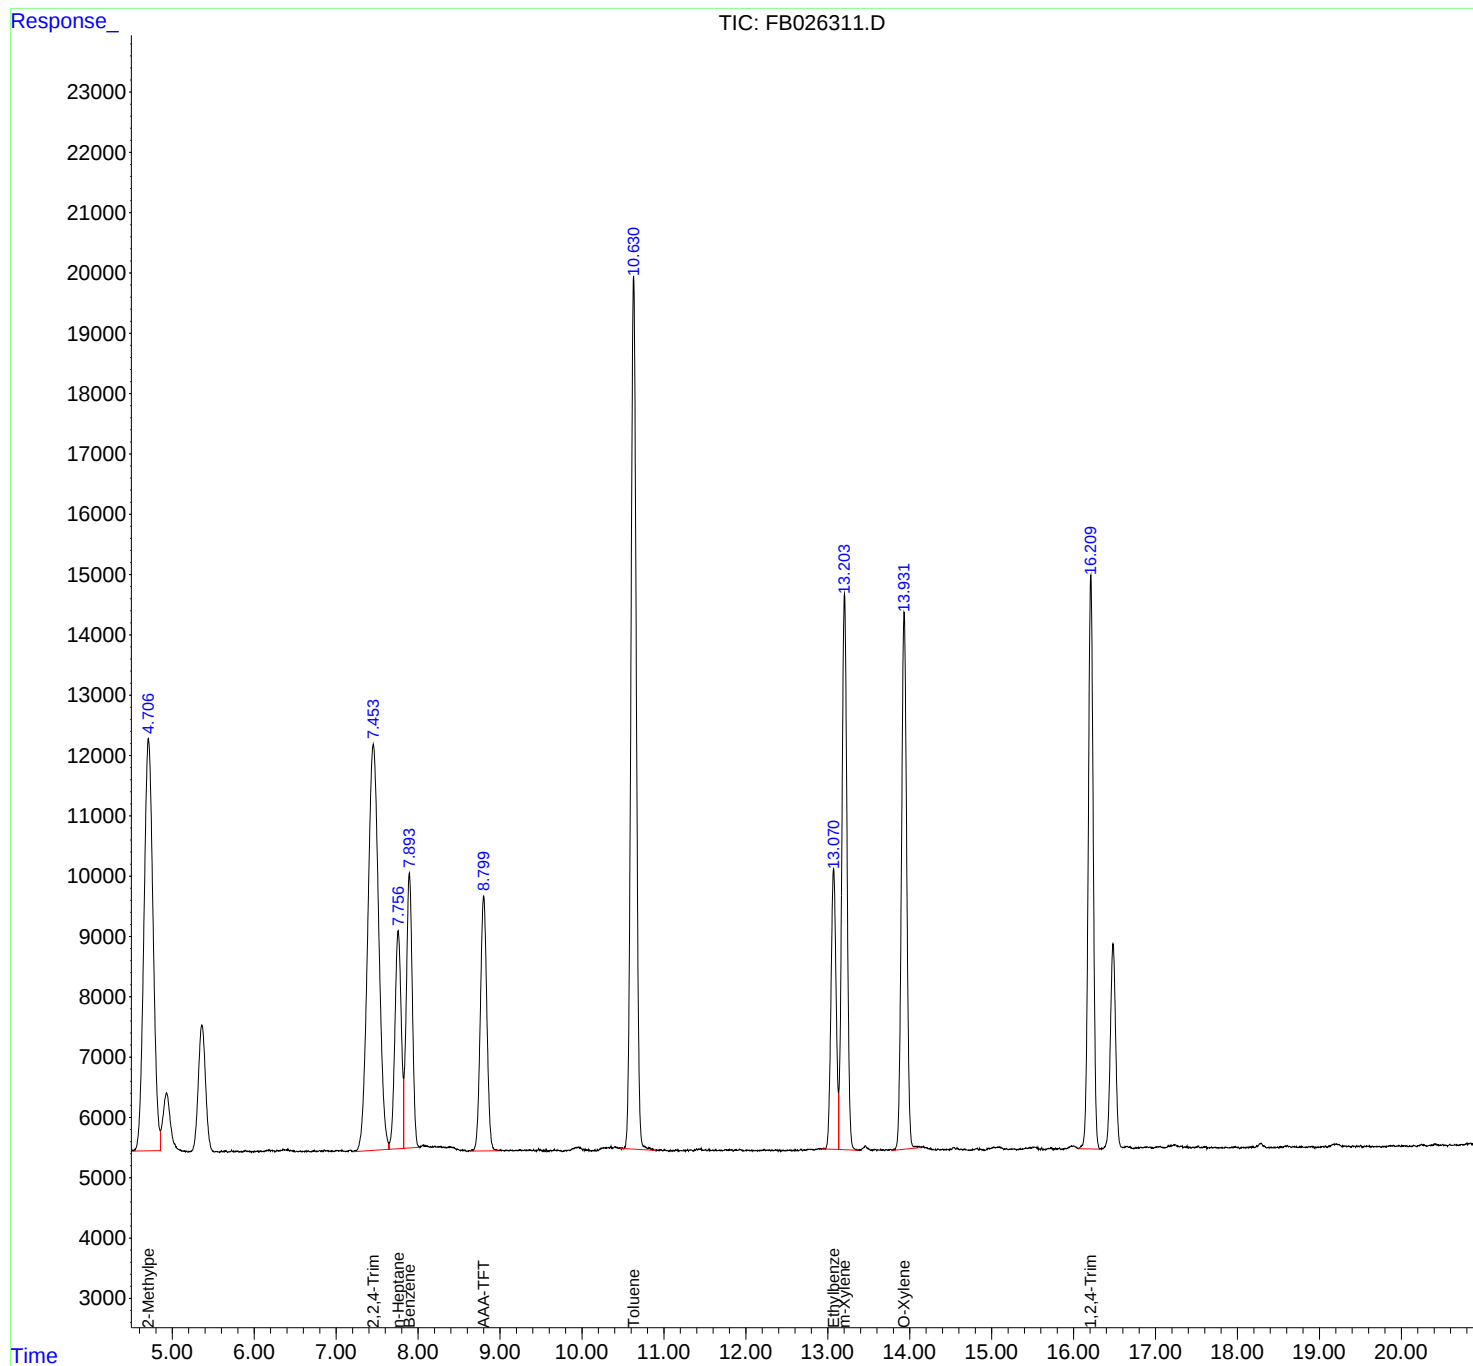


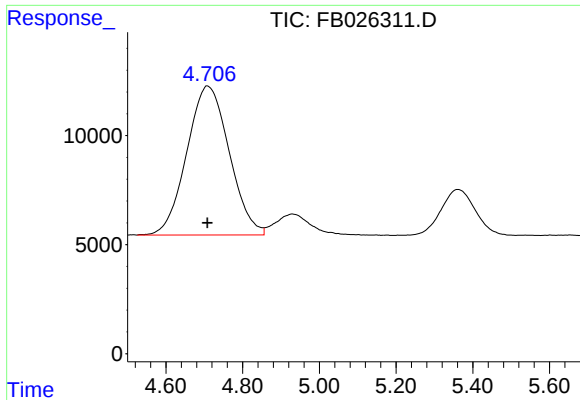

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 526130
Conc: 31.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027S1

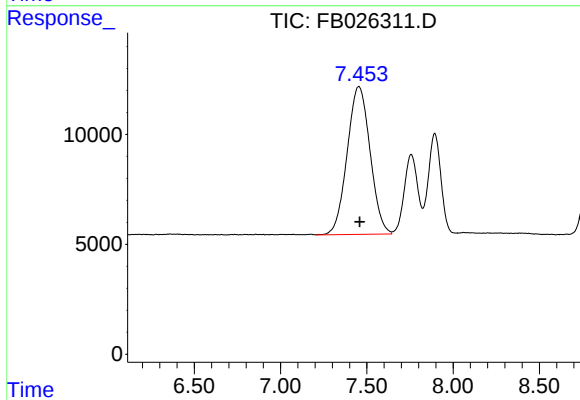


#2 2,2,4-Trimethylpentane

R.T.: 7.455 min
Delta R.T.: -0.005 min
Response: 620988
Conc: 31.85 ng/ml

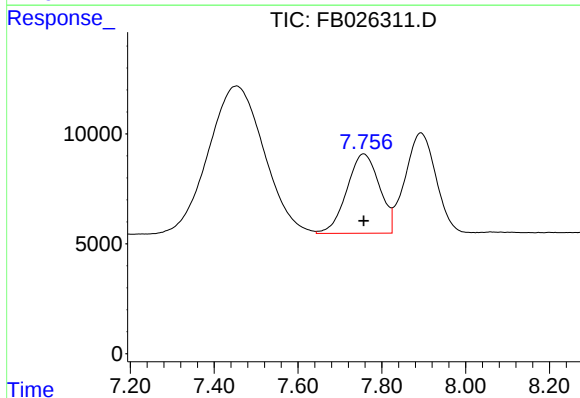


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 194860
Conc: 10.56 ng/ml

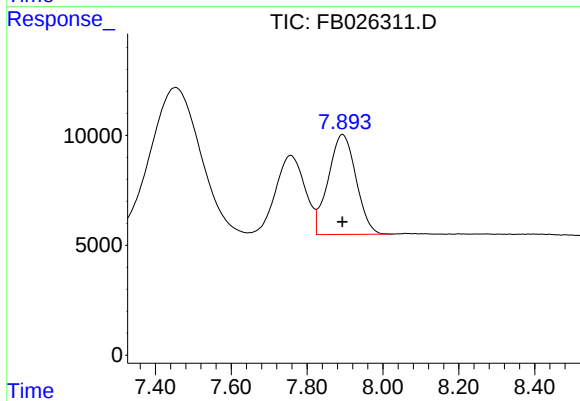

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 231544
Conc: 10.62 ng/ml

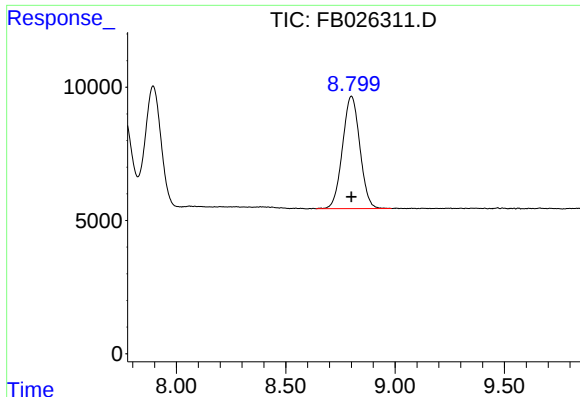

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 232848
Conc: 19.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027S1

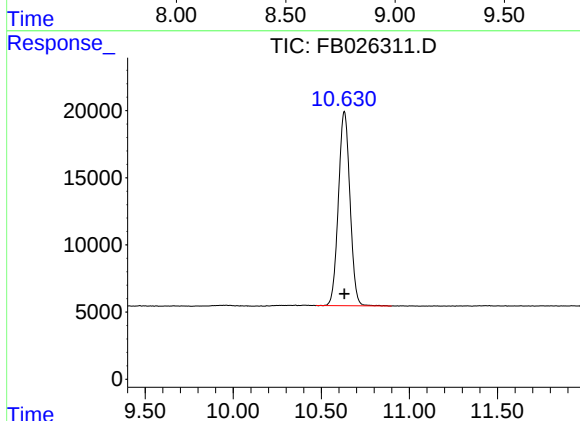


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 660357
Conc: 31.84 ng/ml

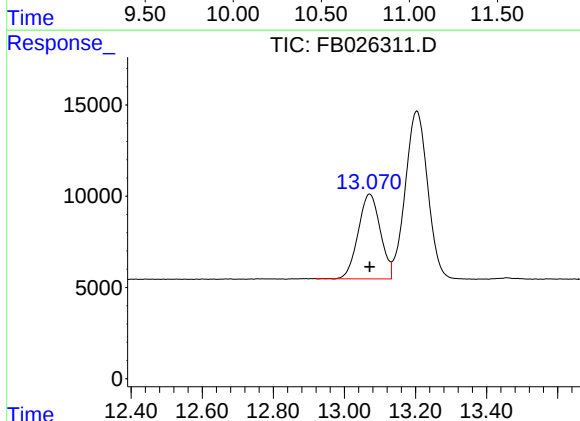


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 200865
Conc: 10.64 ng/ml

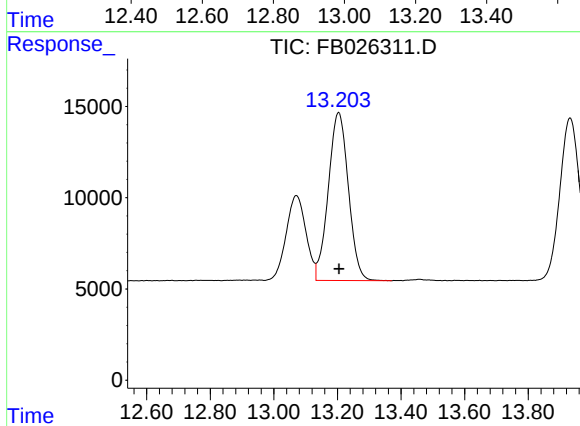

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 403911
Conc: 21.24 ng/ml

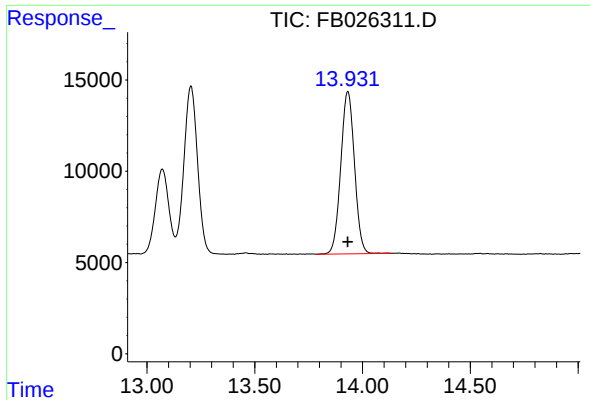

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 393967
Conc: 21.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027S1

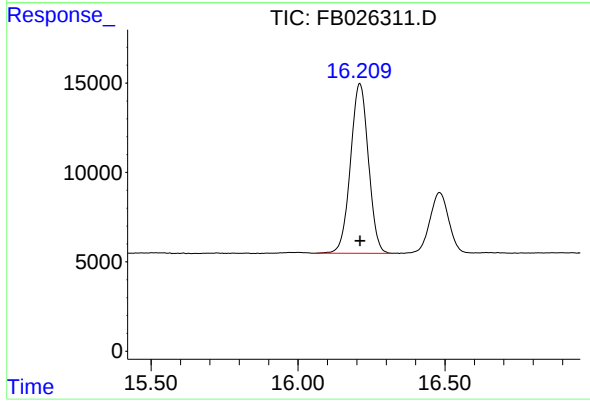

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 402101
Conc: 21.21 ng/ml