

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102721\
 Data File : FB026313.D
 Signal(s) : FID2B.CH
 Acq On : 27 Oct 2021 23:11
 Operator : AJ/MA
 Sample : BSF1027W1
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1027W1

Integration File: Calibration.e
 Quant Time: Oct 28 05:45:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	241929	20.421 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	517589	31.085 ng/ml
2) t 2,2,4-Trimethylpentane	7.450	614302	31.504 ng/ml
3) t n-Heptane	7.756	192622	10.440 ng/ml
4) t Benzene	7.894	229879	10.544 ng/ml
6) t Toluene	10.630	658375	31.743 ng/ml
7) t Ethylbenzene	13.071	201506	10.671 ng/ml
8) t m-Xylene	13.204	405372	21.313 ng/ml
9) t O-Xylene	13.931	393893	21.326 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	399366	21.066 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102721\
Data File : FB026313.D
Signal(s) : FID2B.CH
Acq On : 27 Oct 2021 23:11
Operator : AJ/MA
Sample : BSF1027W1
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1027W1

Integration File: Calibration.e
Quant Time: Oct 28 05:45:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

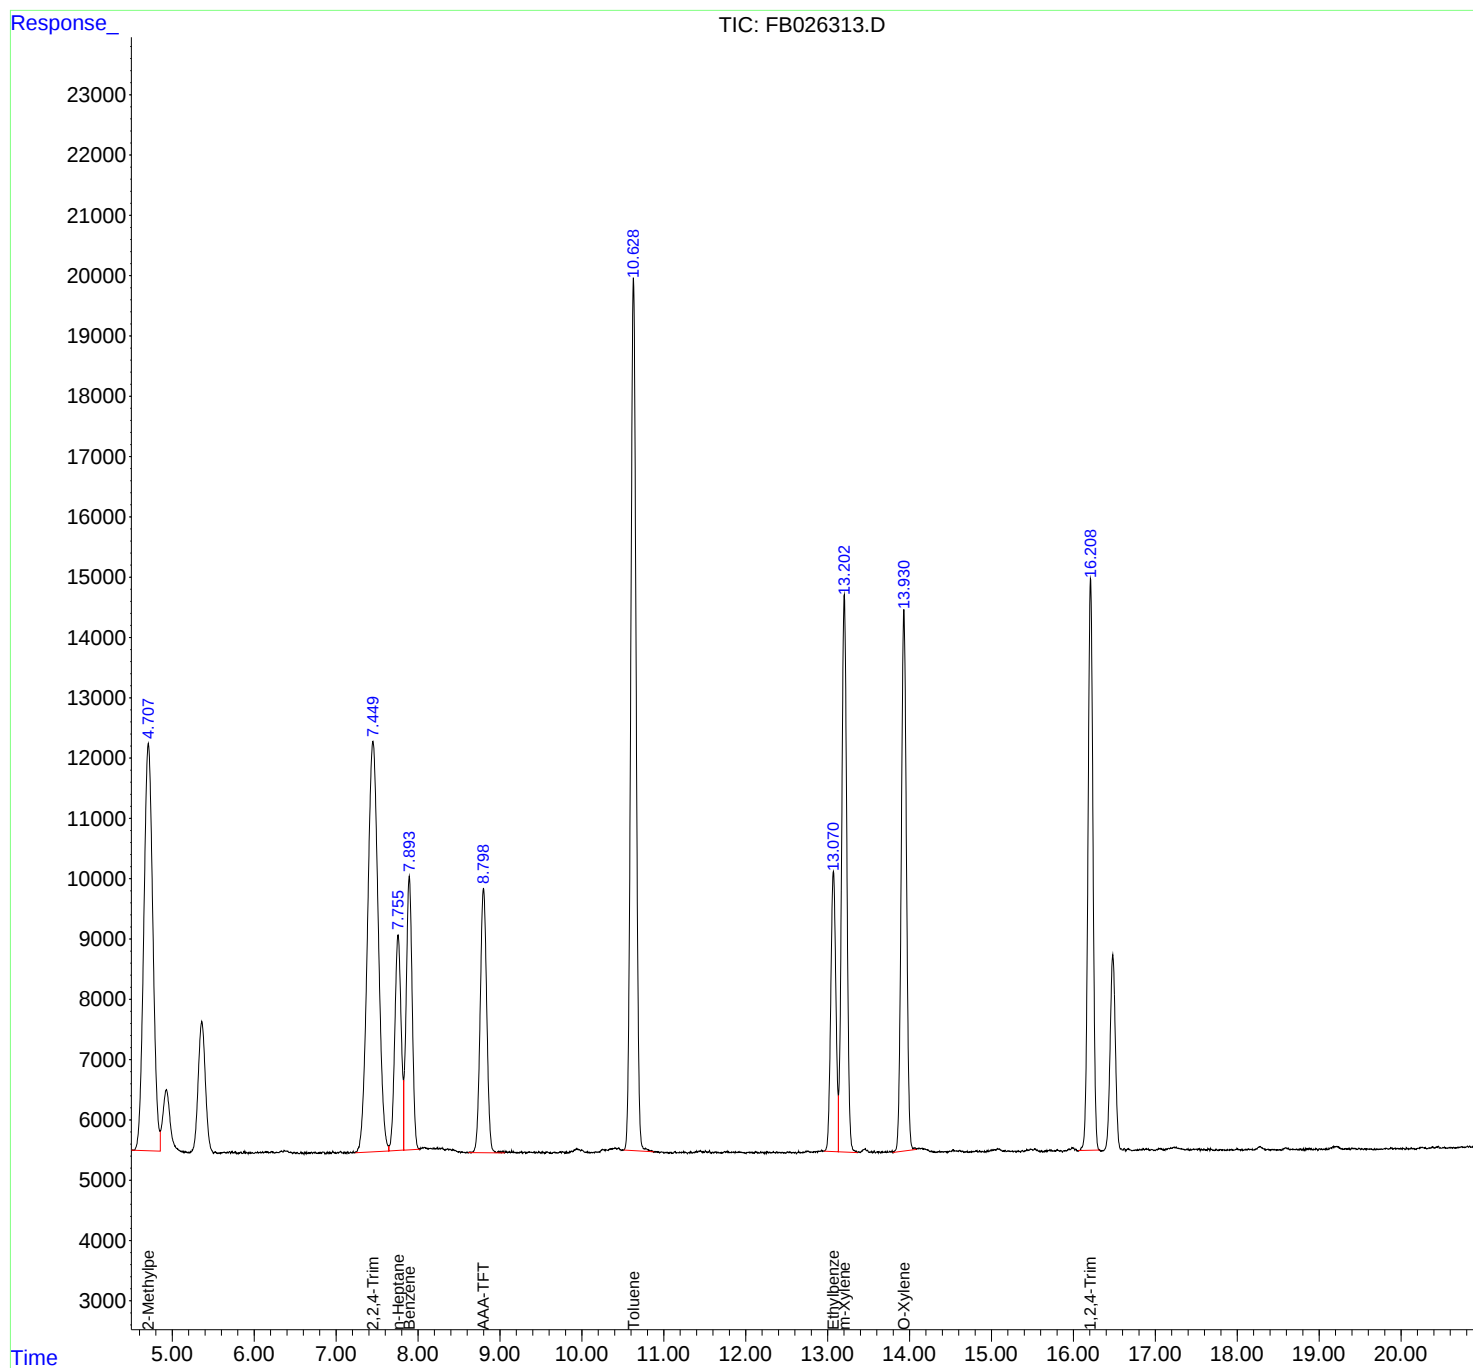


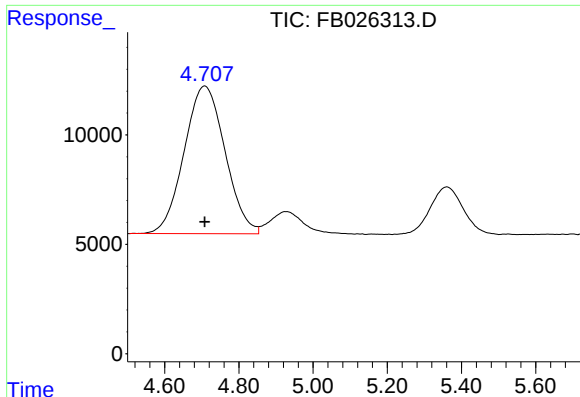

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 517589
Conc: 31.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027W1

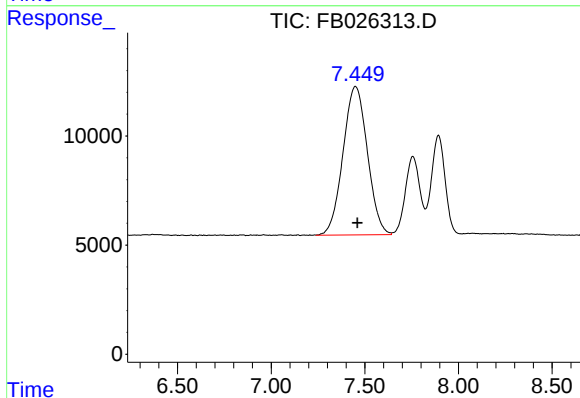


#2 2,2,4-Trimethylpentane

R.T.: 7.450 min
Delta R.T.: -0.010 min
Response: 614302
Conc: 31.50 ng/ml

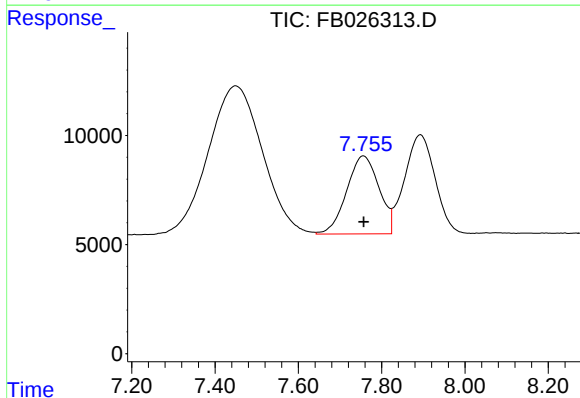


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 192622
Conc: 10.44 ng/ml

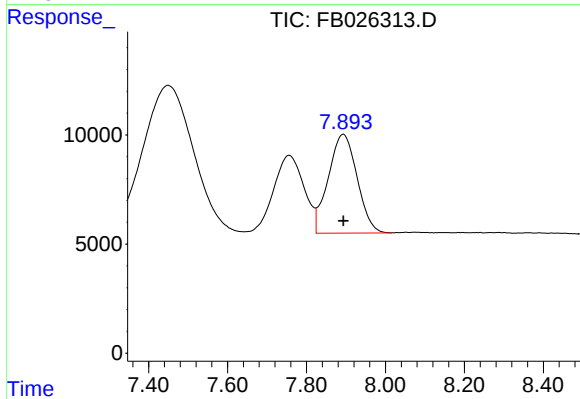

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 229879
Conc: 10.54 ng/ml

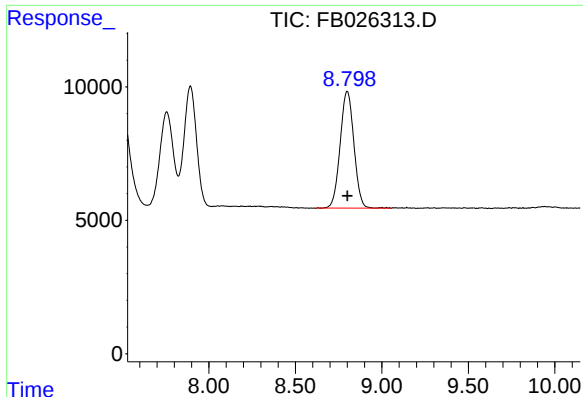

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 241929
Conc: 20.42 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027W1

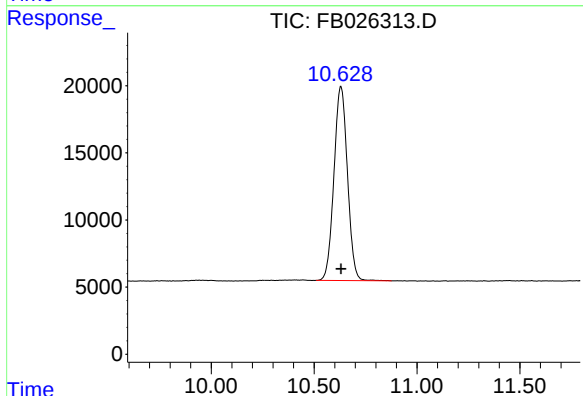


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 658375
Conc: 31.74 ng/ml

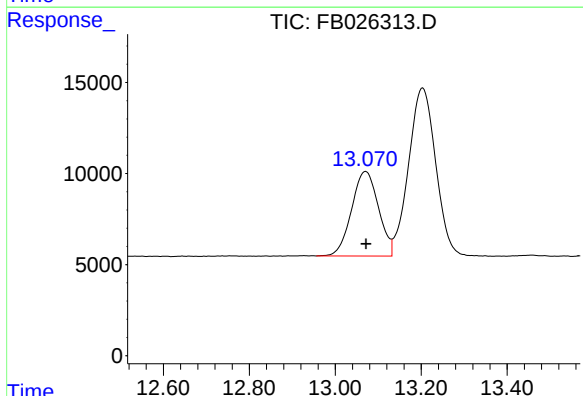


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 201506
Conc: 10.67 ng/ml

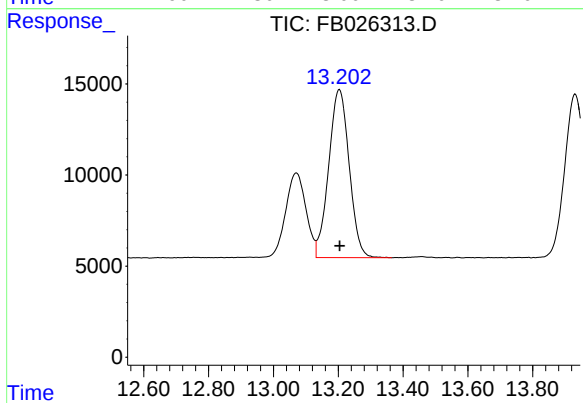

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: -0.001 min
Response: 405372
Conc: 21.31 ng/ml

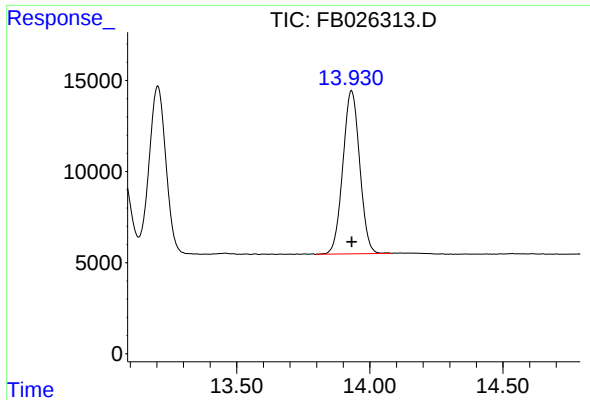

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 393893
Conc: 21.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027W1

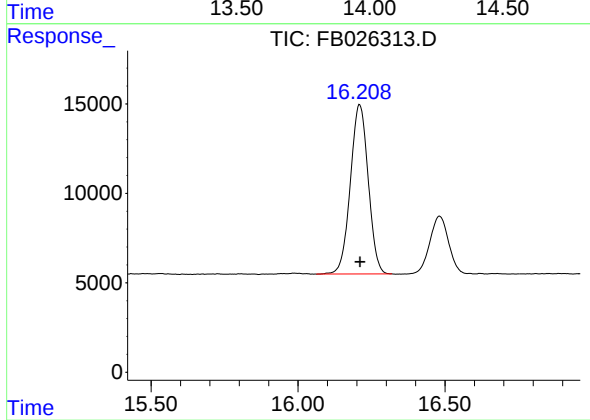

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.001 min
Response: 399366
Conc: 21.07 ng/ml