

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102721\
 Data File : FB026314.D
 Signal(s) : FID2B.CH
 Acq On : 27 Oct 2021 23:47
 Operator : AJ/MA
 Sample : BSF1027W2
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1027W2

Integration File: Calibration.e
 Quant Time: Oct 28 05:45:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	233840	19.738 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	524206	31.482 ng/ml
2) t 2,2,4-Trimethylpentane	7.448	622687	31.934 ng/ml
3) t n-Heptane	7.757	197860	10.724 ng/ml
4) t Benzene	7.895	234830	10.772 ng/ml
6) t Toluene	10.631	672840	32.440 ng/ml
7) t Ethylbenzene	13.071	206745	10.948 ng/ml
8) t m-Xylene	13.203	413033	21.716 ng/ml
9) t O-Xylene	13.931	395421	21.409 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	408066	21.525 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102721\
Data File : FB026314.D
Signal(s) : FID2B.CH
Acq On : 27 Oct 2021 23:47
Operator : AJ/MA
Sample : BSF1027W2
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1027W2

Integration File: Calibration.e
Quant Time: Oct 28 05:45:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

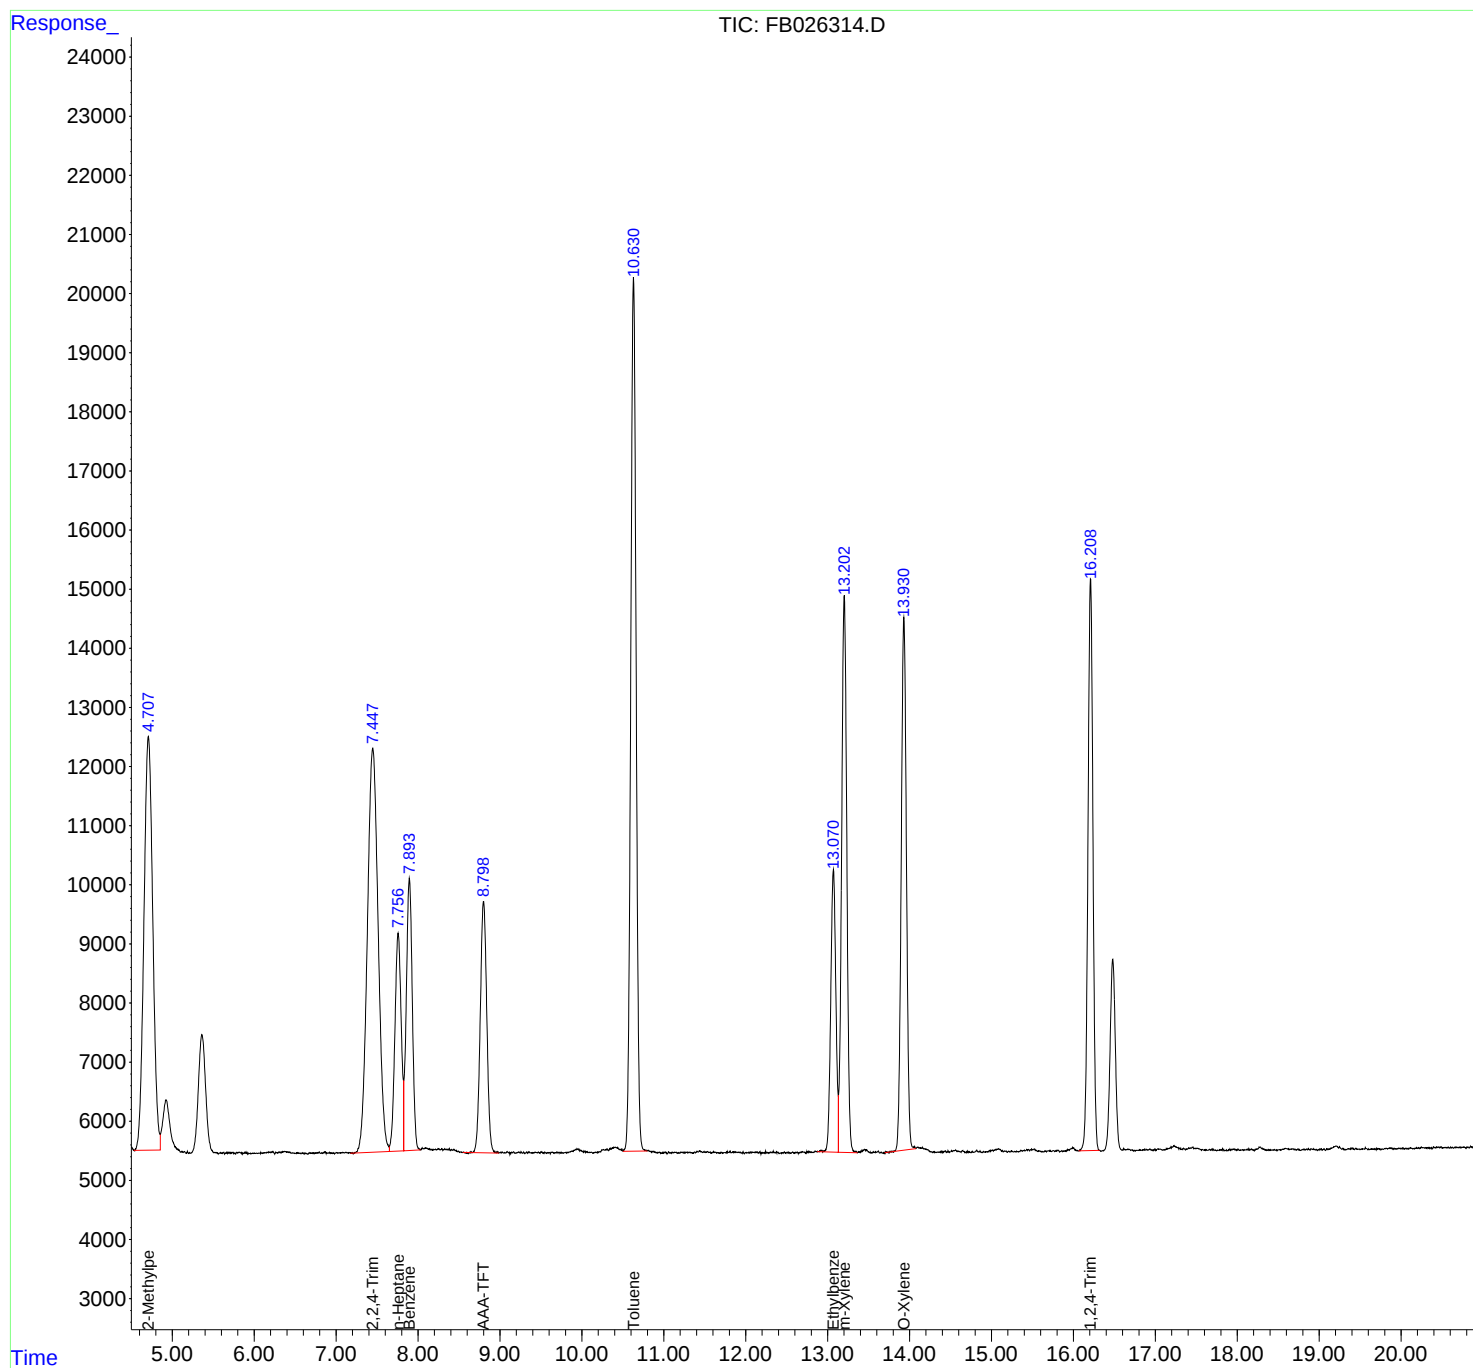


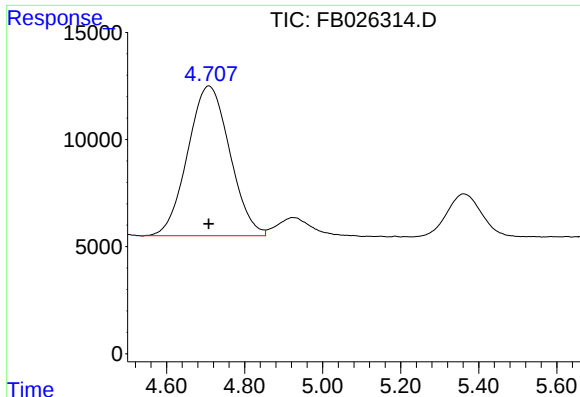

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 524206
Conc: 31.48 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027W2

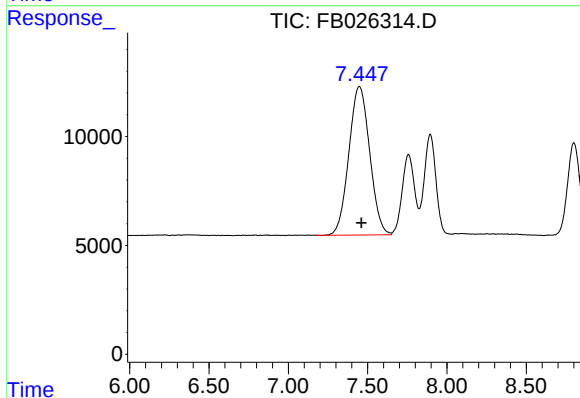


#2 2,2,4-Trimethylpentane

R.T.: 7.448 min
Delta R.T.: -0.012 min
Response: 622687
Conc: 31.93 ng/ml

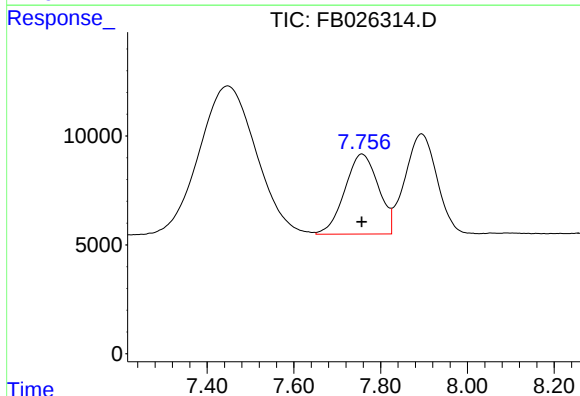


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 197860
Conc: 10.72 ng/ml

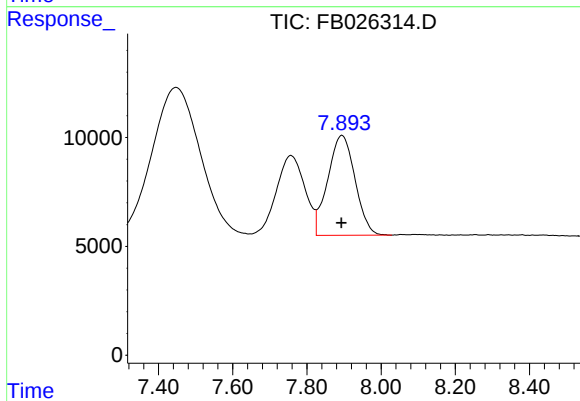

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.002 min
Response: 234830
Conc: 10.77 ng/ml

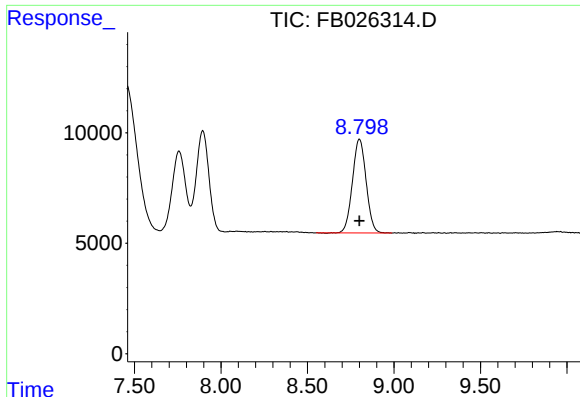

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 233840
Conc: 19.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027W2

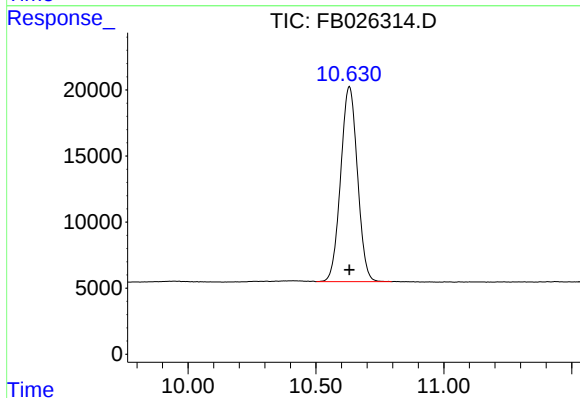


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 672840
Conc: 32.44 ng/ml

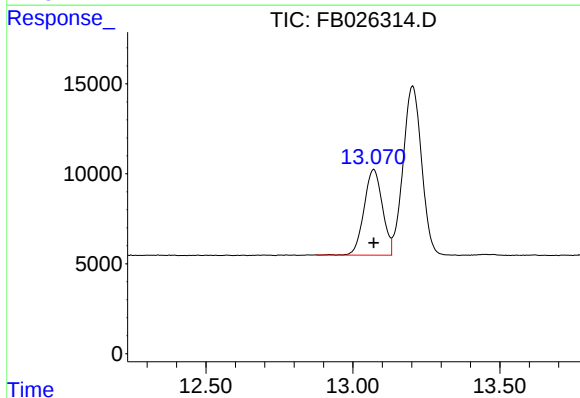


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 206745
Conc: 10.95 ng/ml

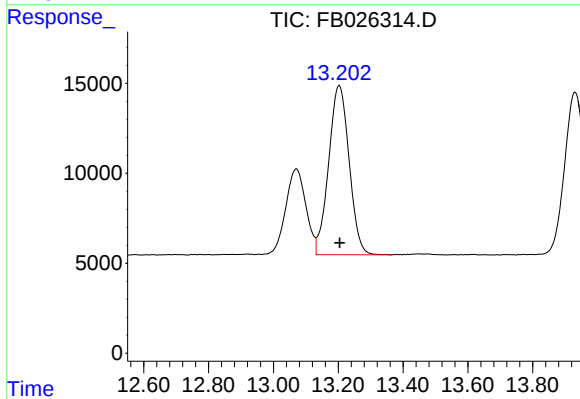

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.001 min
Response: 413033
Conc: 21.72 ng/ml

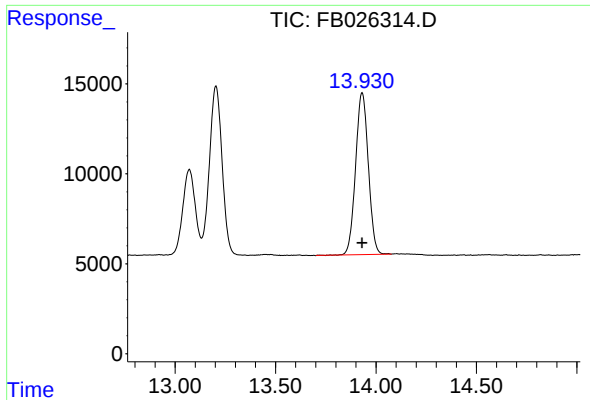

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 395421
Conc: 21.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1027W2

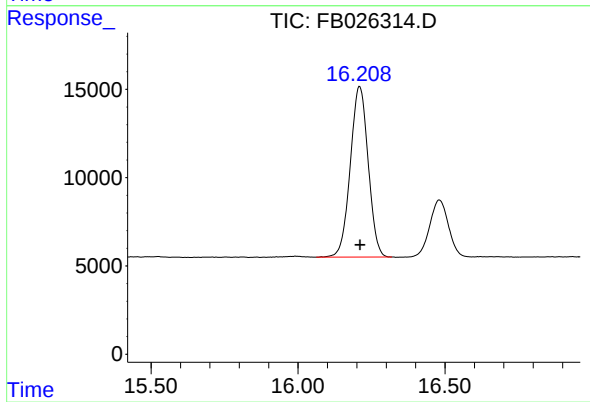

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.001 min
Response: 408066
Conc: 21.52 ng/ml