

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
 Data File : FB022838.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2019 12:24
 Operator : DD/AJ
 Sample : K5140-06MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 08:38:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	555084	21.937 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	834596	24.558 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	878897	24.154 ng/ml
3) t n-Heptane	7.755	266995	7.318 ng/ml
4) t Benzene	7.890	379107	8.586 ng/ml
6) t Toluene	10.629	1105192	25.642 ng/ml
7) t Ethylbenzene	13.060	1235902	30.429 ng/ml
8) t m-Xylene	13.201	1244023	32.333 ng/ml
9) t O-Xylene	13.930	1238741	34.011 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	1693167	59.419 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
Data File : FB022838.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2019 12:24
Operator : DD/AJ
Sample : K5140-06MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 08:38:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

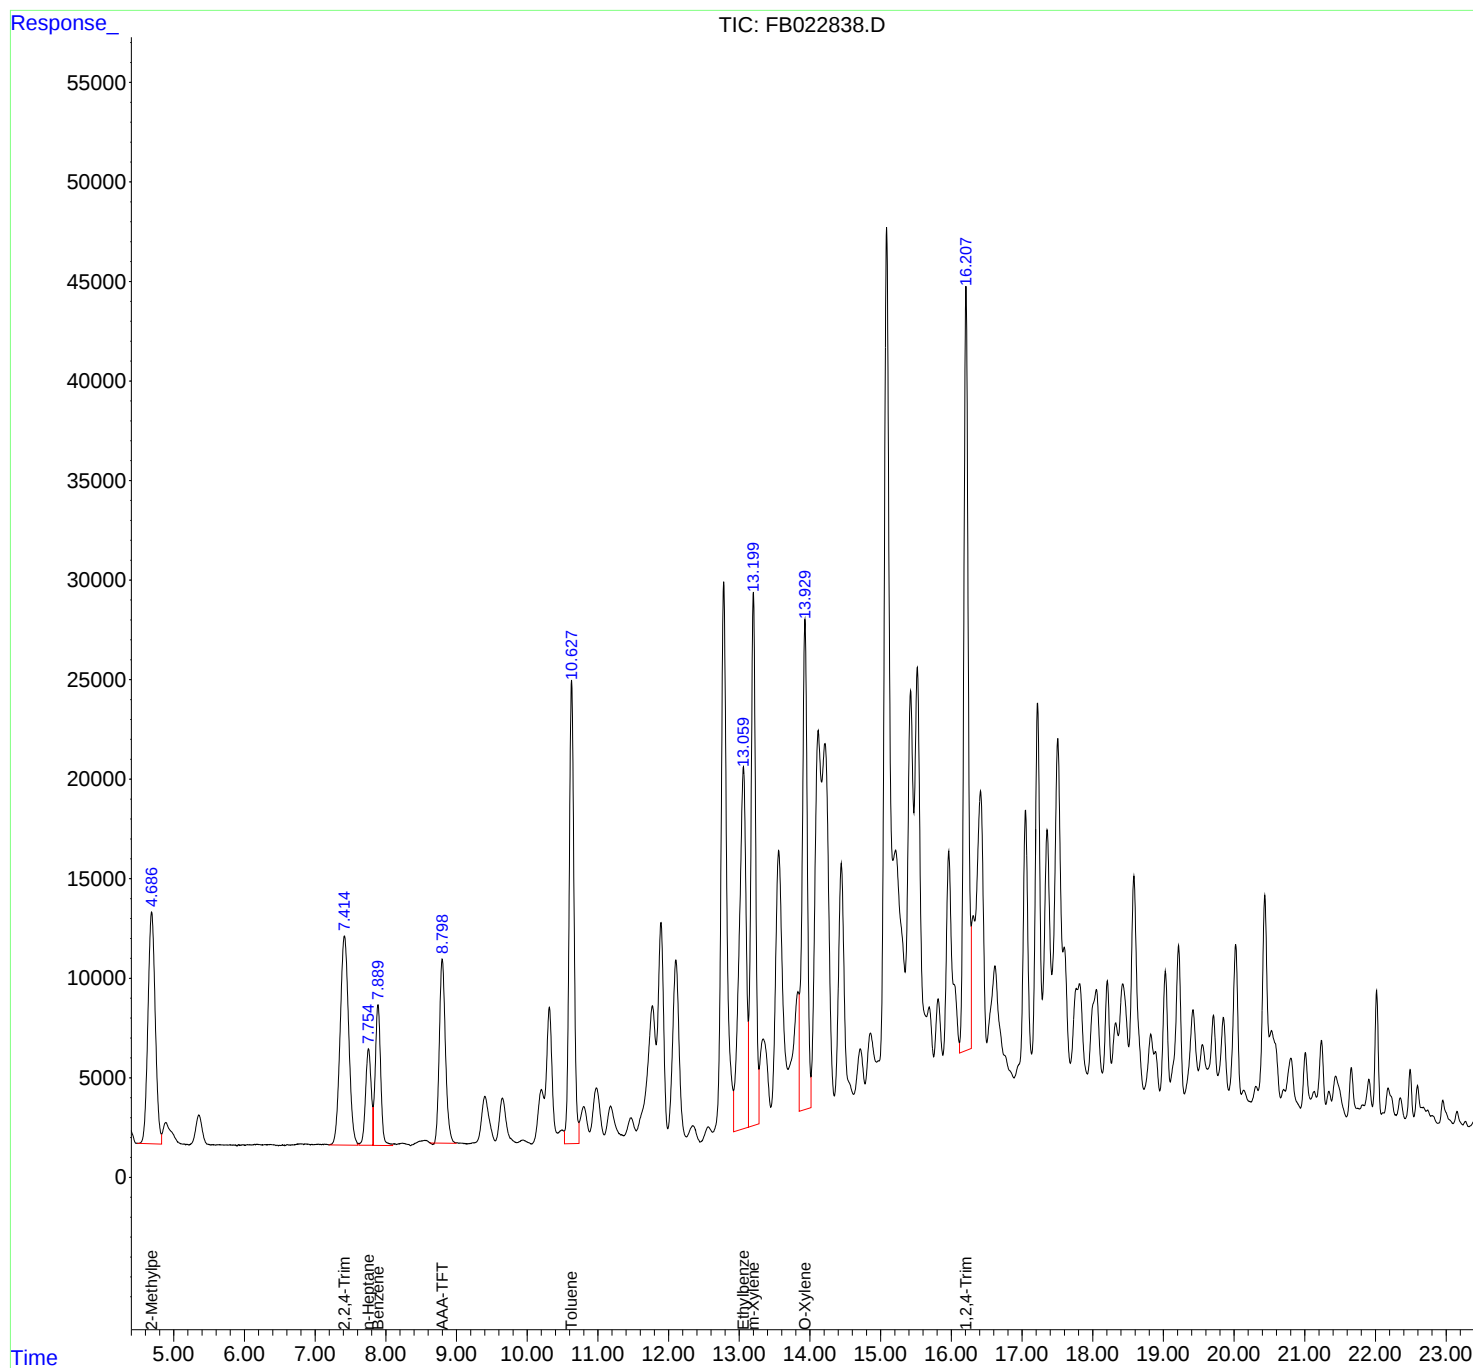

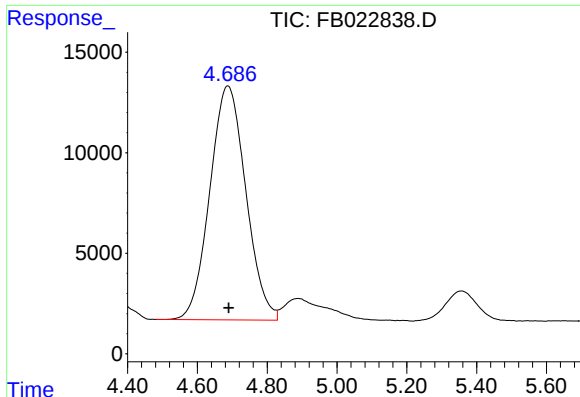


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 834596
Conc: 24.56 ng/ml

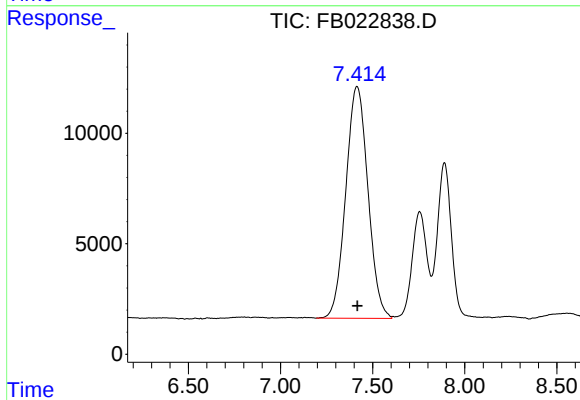


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 878897
Conc: 24.15 ng/ml

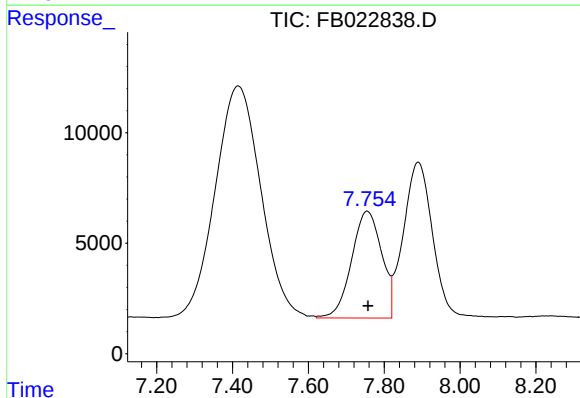


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.002 min
Response: 266995
Conc: 7.32 ng/ml

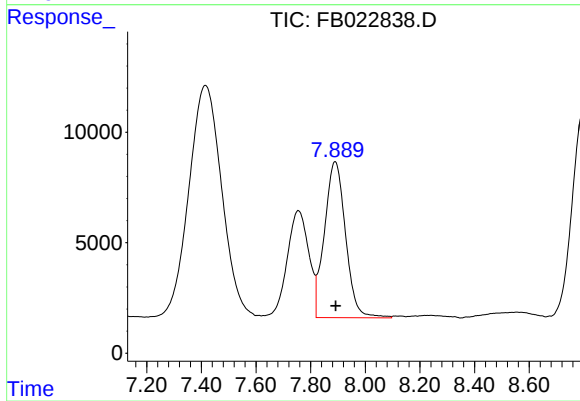


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 379107
Conc: 8.59 ng/ml

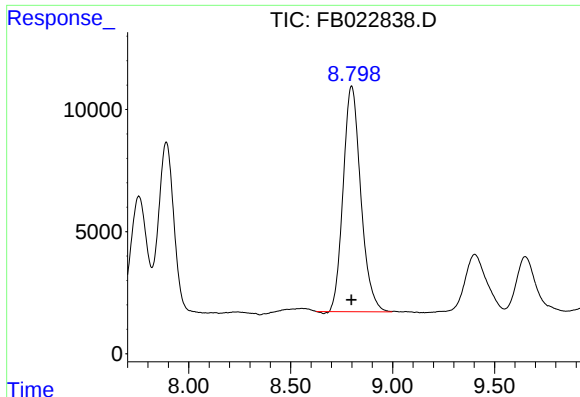


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 555084
Conc: 21.94 ng/ml

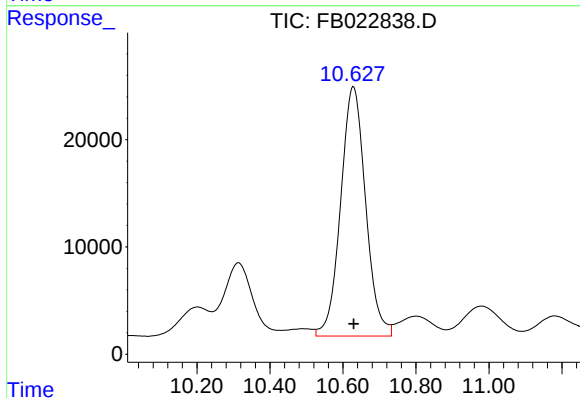


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 1105192
Conc: 25.64 ng/ml

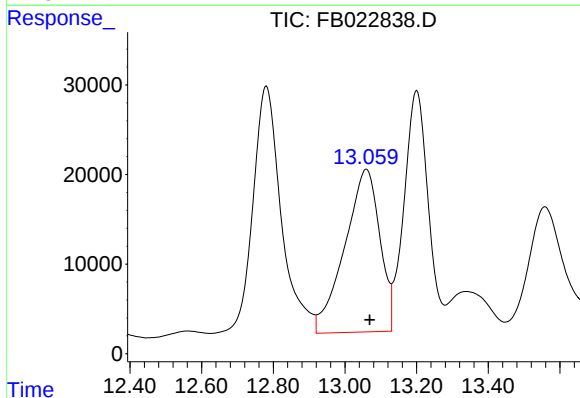


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.010 min
Response: 1235902
Conc: 30.43 ng/ml

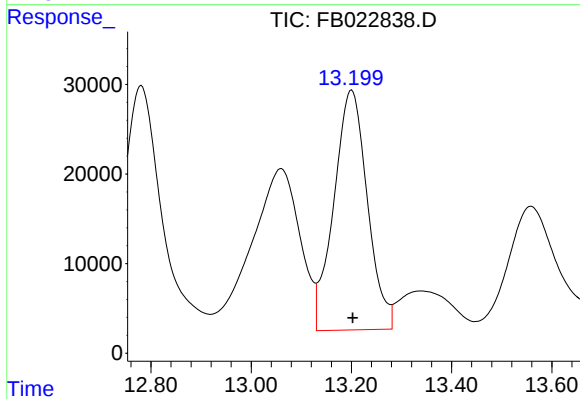


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 1244023
Conc: 32.33 ng/ml

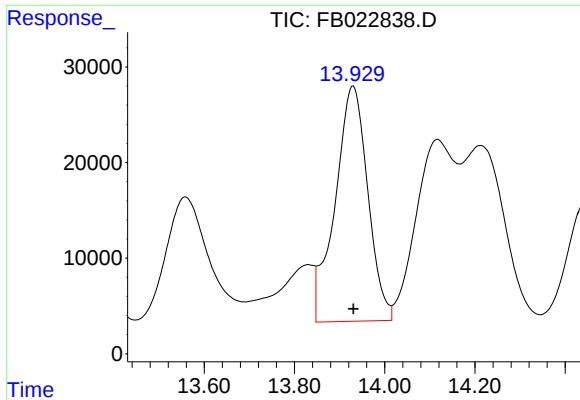

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 1238741
Conc: 34.01 ng/ml

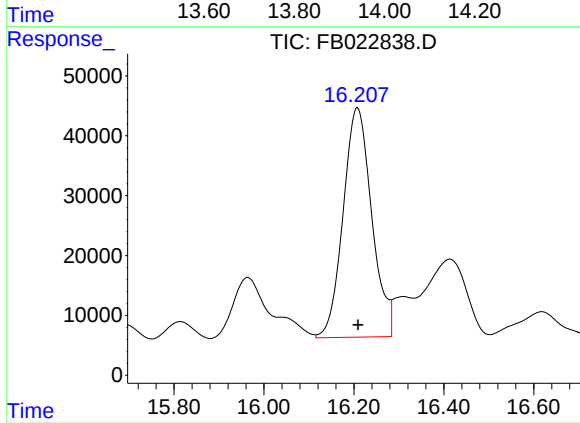

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 1693167
Conc: 59.42 ng/ml