

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
Data File : FB022840.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2019 13:39
Operator : DD/AJ
Sample : VBF1028S2
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 08:38:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	507560	20.058 ng/ml
Target Compounds			
6) t Toluene	10.623	4399	0.102 ng/ml
8) t m-Xylene	13.203	1590	0.041 ng/ml
9) t O-Xylene	13.925	2875	0.079 ng/ml
10) t 1,2,4-Trimethylbenzene	16.216	7402	0.260 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
Data File : FB022840.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2019 13:39
Operator : DD/AJ
Sample : VBF1028S2
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1


Integration File: Calibration.e
Quant Time: Oct 29 08:38:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

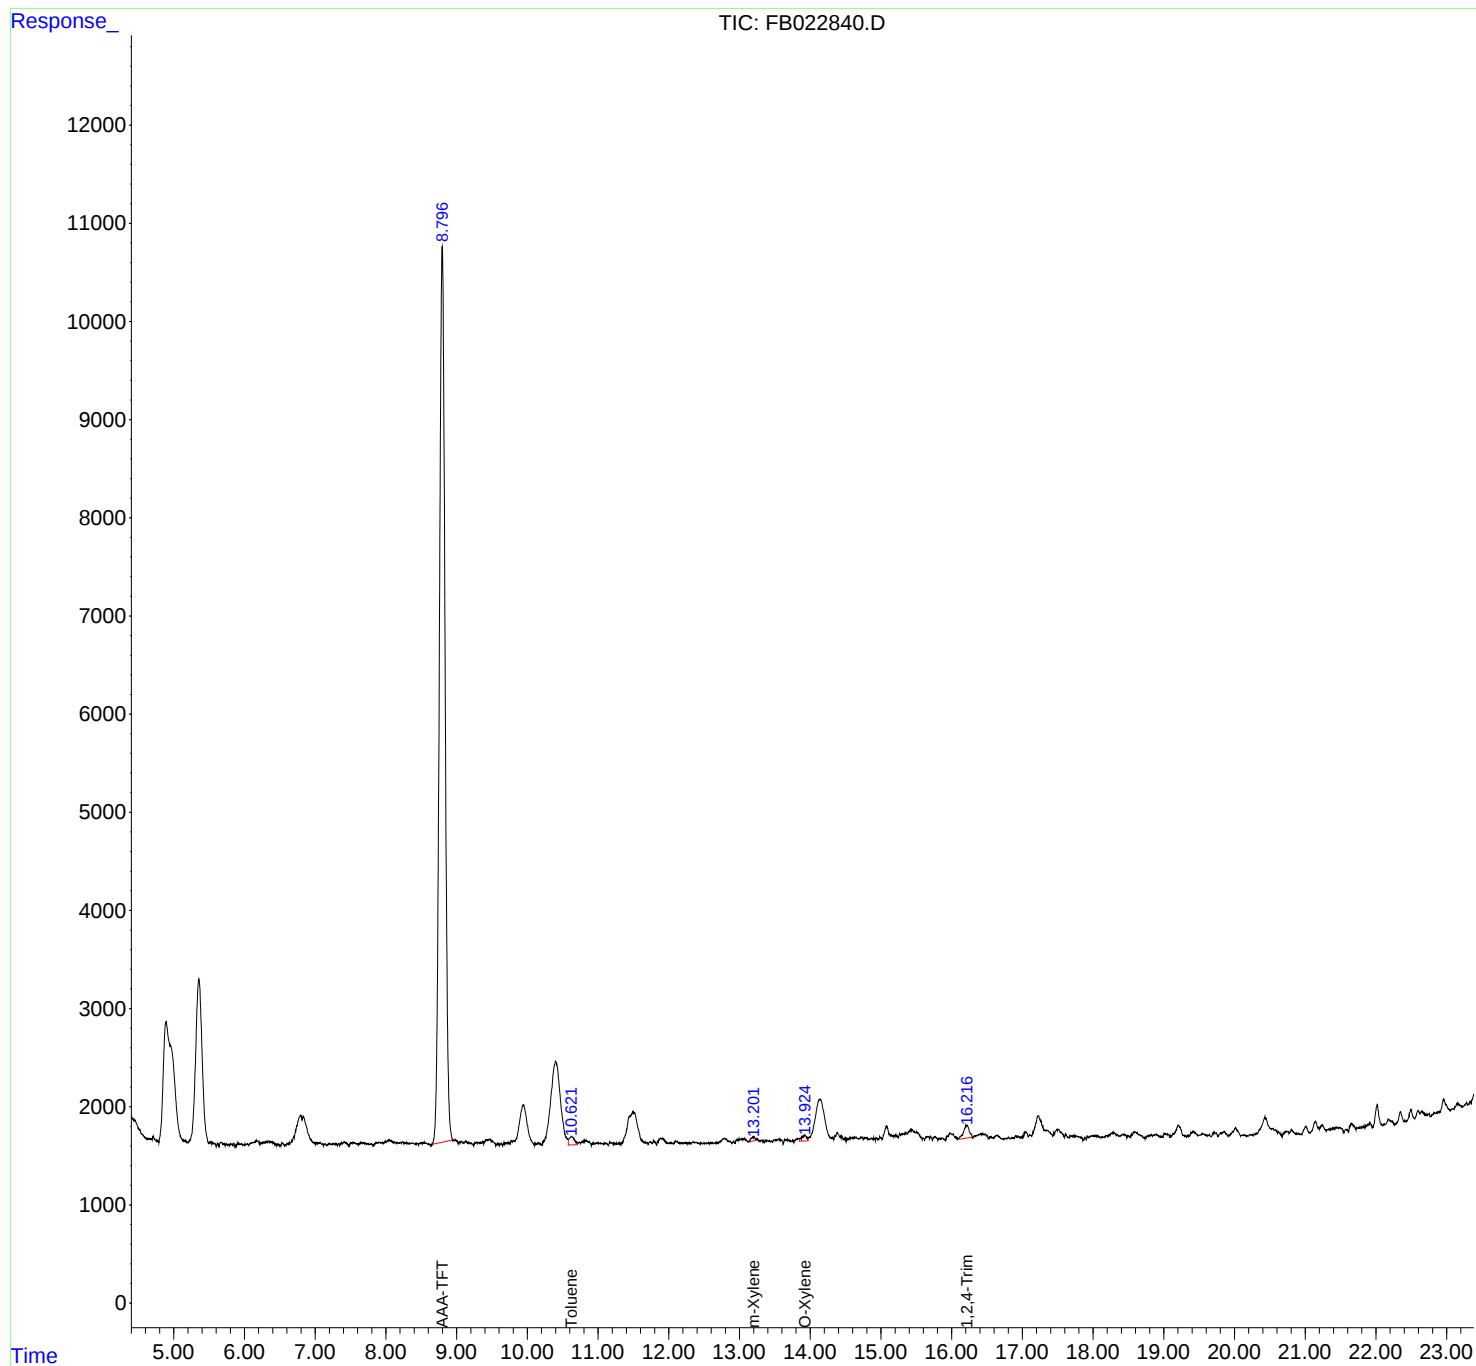


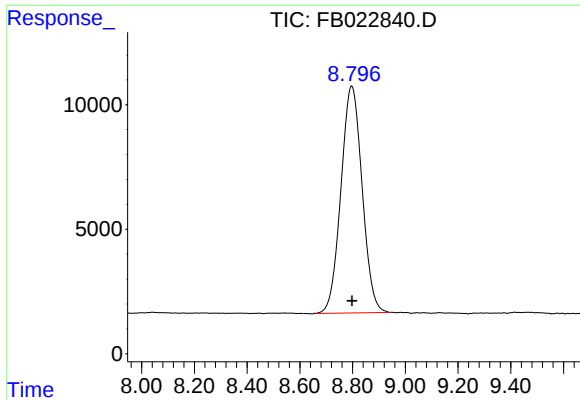


#5 AAA-TFT
 R.T.: 8.797 min
 Delta R.T.: -0.001 min
 Response: 507560
 Conc: 20.06 ng/ml

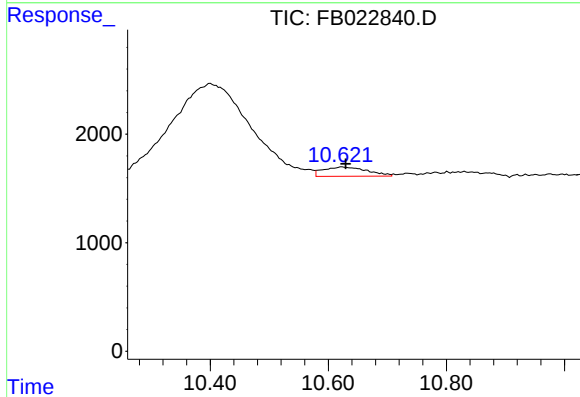


#6 Toluene
 R.T.: 10.623 min
 Delta R.T.: -0.007 min
 Response: 4399
 Conc: 0.10 ng/ml

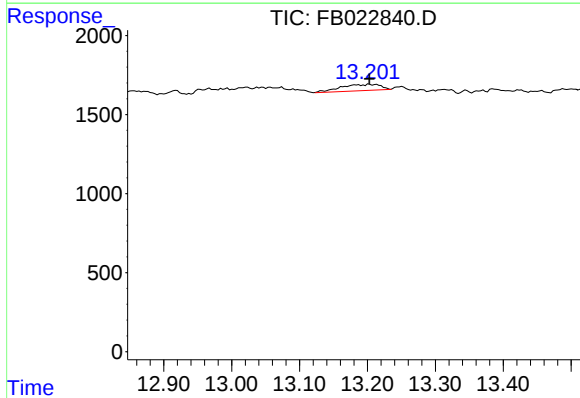

#8 m-Xylene
 R.T.: 13.203 min
 Delta R.T.: 0.000 min
 Response: 1590
 Conc: 0.04 ng/ml

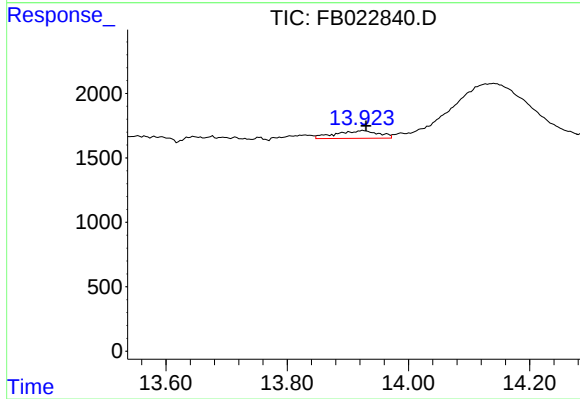

#9 O-Xylene
 R.T.: 13.925 min
 Delta R.T.: -0.005 min
 Response: 2875
 Conc: 0.08 ng/ml

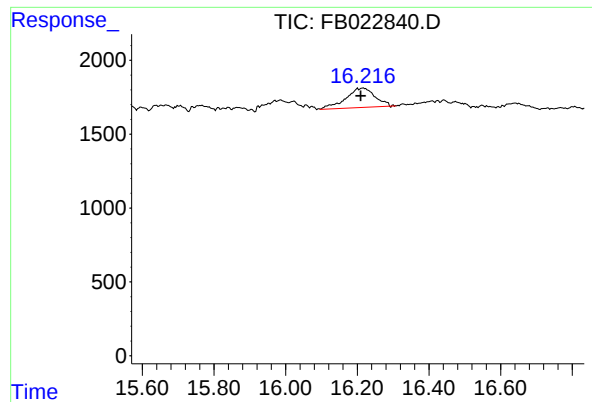

#10 1,2,4-Trimethylbenzene

R.T.: 16.216 min
Delta R.T.: 0.007 min
Response: 7402
Conc: 0.26 ng/ml