

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
 Data File : FB022841.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2019 14:08
 Operator : DD/AJ
 Sample : K5140-06 50X
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 08:38:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	544528	21.519 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.697	10135	0.298 ng/ml
2) t 2,2,4-Trimethylpentane	7.371	308	0.008 ng/ml
3) t n-Heptane	7.747	4876	0.134 ng/ml
4) t Benzene	7.920	704	0.016 ng/ml
6) t Toluene	10.626	1883	0.044 ng/ml
7) t Ethylbenzene	13.036	147936	3.642 ng/ml
8) t m-Xylene	13.196	60366	1.569 ng/ml
9) t O-Xylene	13.930	59396	1.631 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	218189	7.657 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
Data File : FB022841.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2019 14:08
Operator : DD/AJ
Sample : K5140-06 50X
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 08:38:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

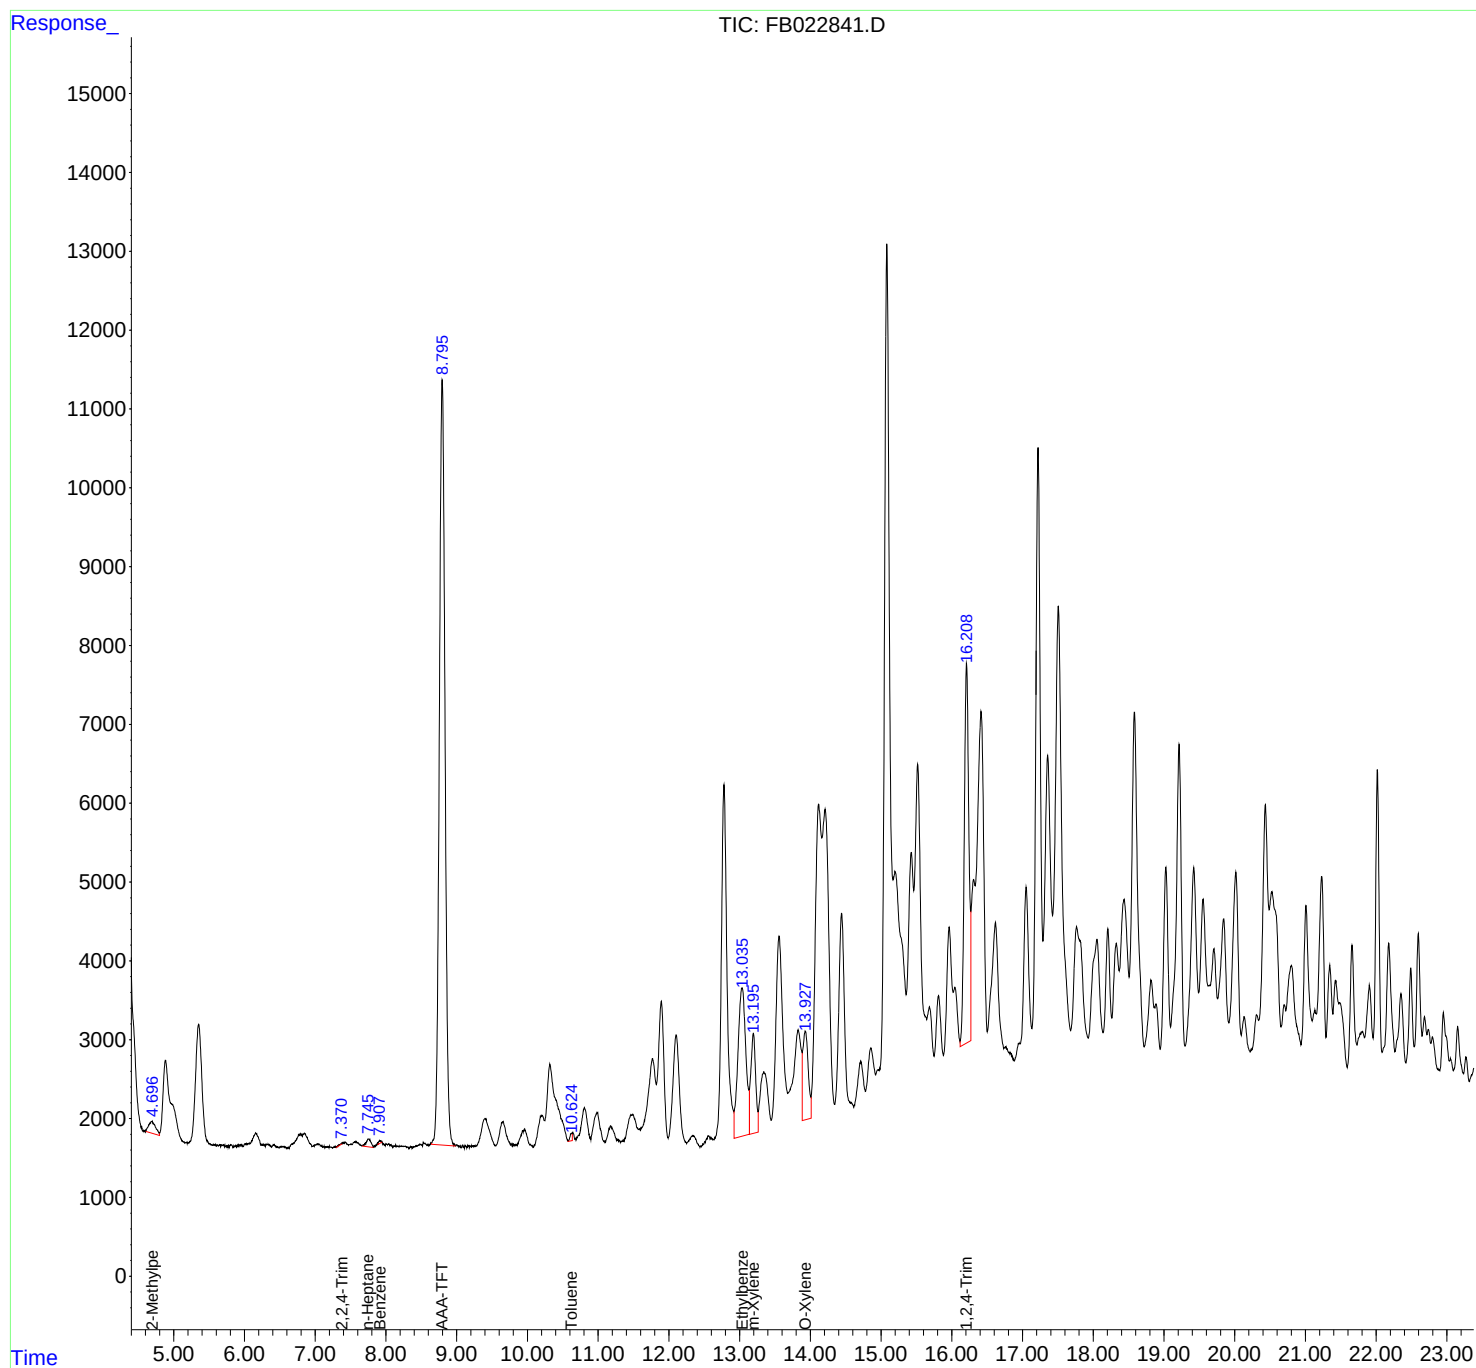

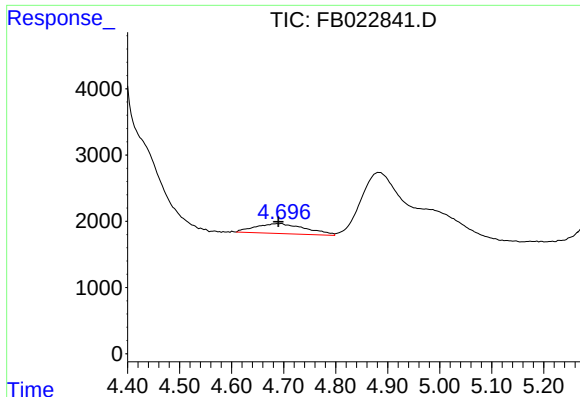


#1 2-Methylpentane

R.T.: 4.697 min
Delta R.T.: 0.007 min
Response: 10135
Conc: 0.30 ng/ml

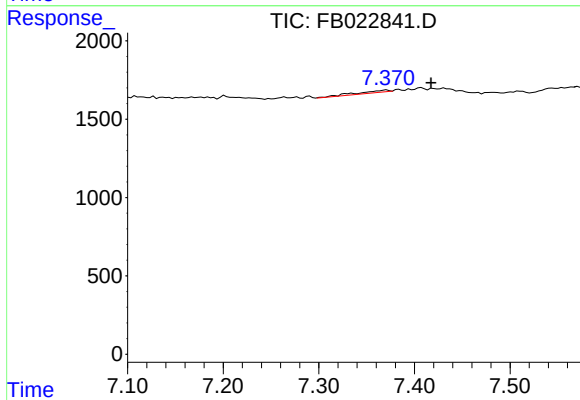


#2 2,2,4-Trimethylpentane

R.T.: 7.371 min
Delta R.T.: -0.046 min
Response: 308
Conc: 0.01 ng/ml

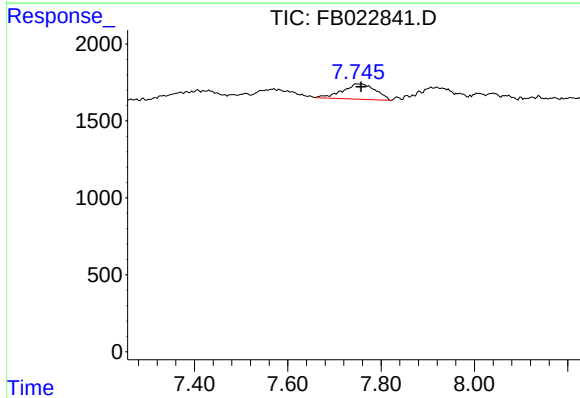


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.010 min
Response: 4876
Conc: 0.13 ng/ml

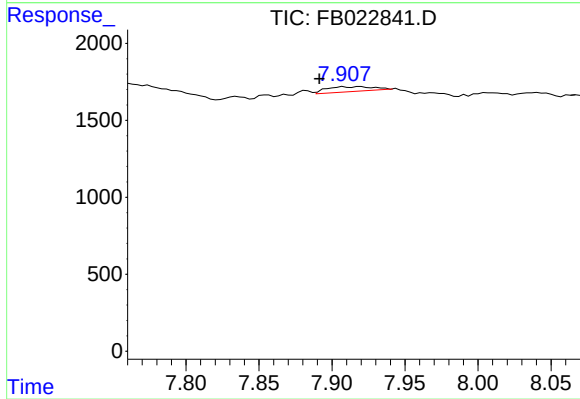


#4 Benzene

R.T.: 7.920 min
Delta R.T.: 0.028 min
Response: 704
Conc: 0.02 ng/ml

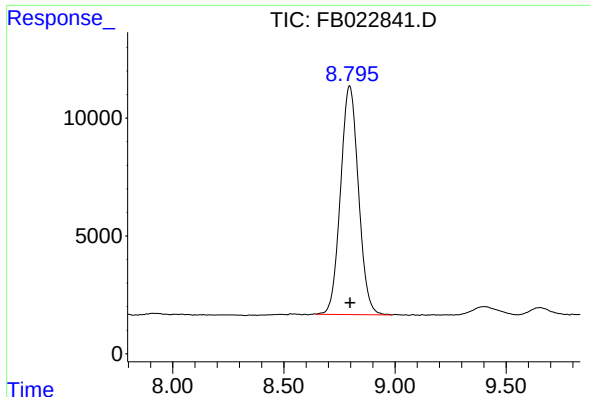


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.002 min
Response: 544528
Conc: 21.52 ng/ml

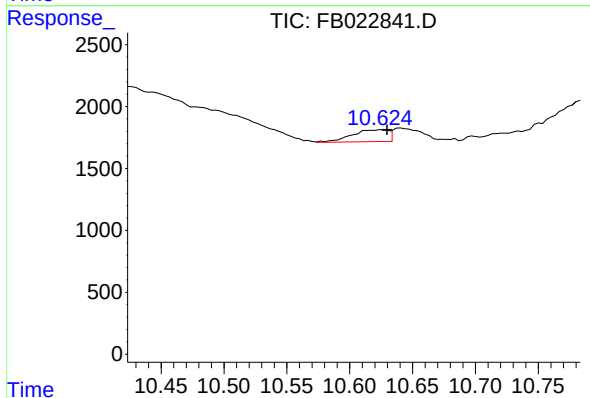


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 1883
Conc: 0.04 ng/ml

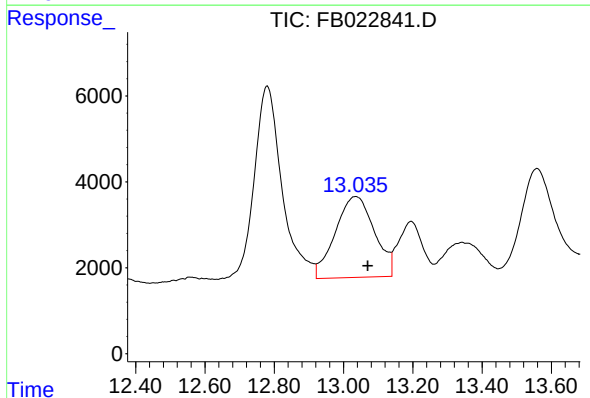


#7 Ethylbenzene

R.T.: 13.036 min
Delta R.T.: -0.034 min
Response: 147936
Conc: 3.64 ng/ml

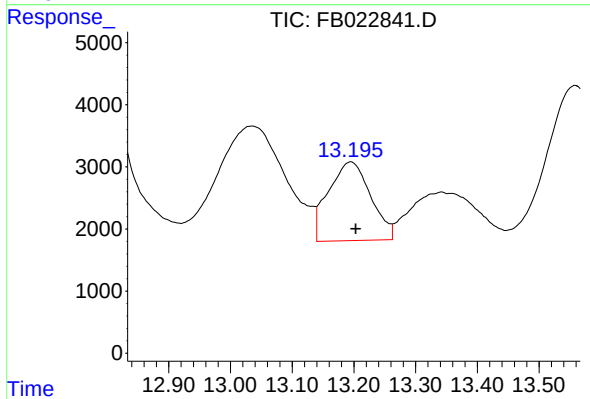


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.007 min
Response: 60366
Conc: 1.57 ng/ml

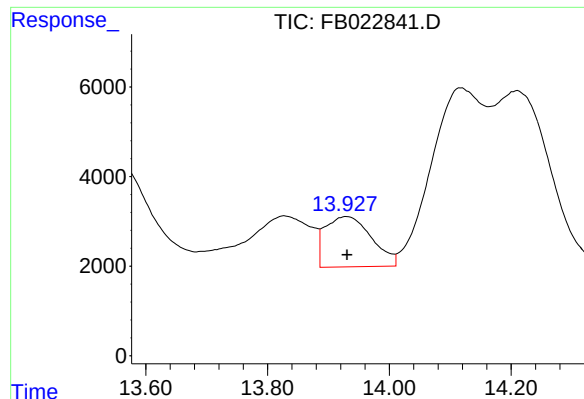

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 59396
Conc: 1.63 ng/ml

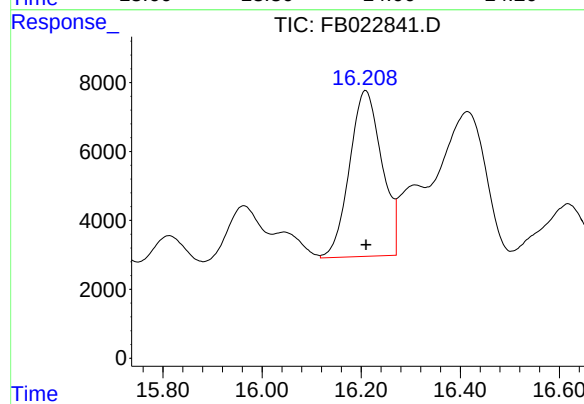

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 218189
Conc: 7.66 ng/ml