

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
 Data File : FB022836.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2019 11:25
 Operator : DD/AJ
 Sample : BSF1028S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 08:38:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	531166	20.991 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	1035851	30.480 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	1163288	31.970 ng/ml
3) t	n-Heptane	7.756	380959	10.441 ng/ml
4) t	Benzene	7.891	453335	10.268 ng/ml
6) t	Toluene	10.629	1317085	30.558 ng/ml
7) t	Ethylbenzene	13.069	413756	10.187 ng/ml
8) t	m-Xylene	13.201	776606	20.184 ng/ml
9) t	O-Xylene	13.929	739222	20.296 ng/ml
10) t	1,2,4-Trimethylbenzene	16.208	586400	20.579 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
Data File : FB022836.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2019 11:25
Operator : DD/AJ
Sample : BSF1028S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 08:38:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

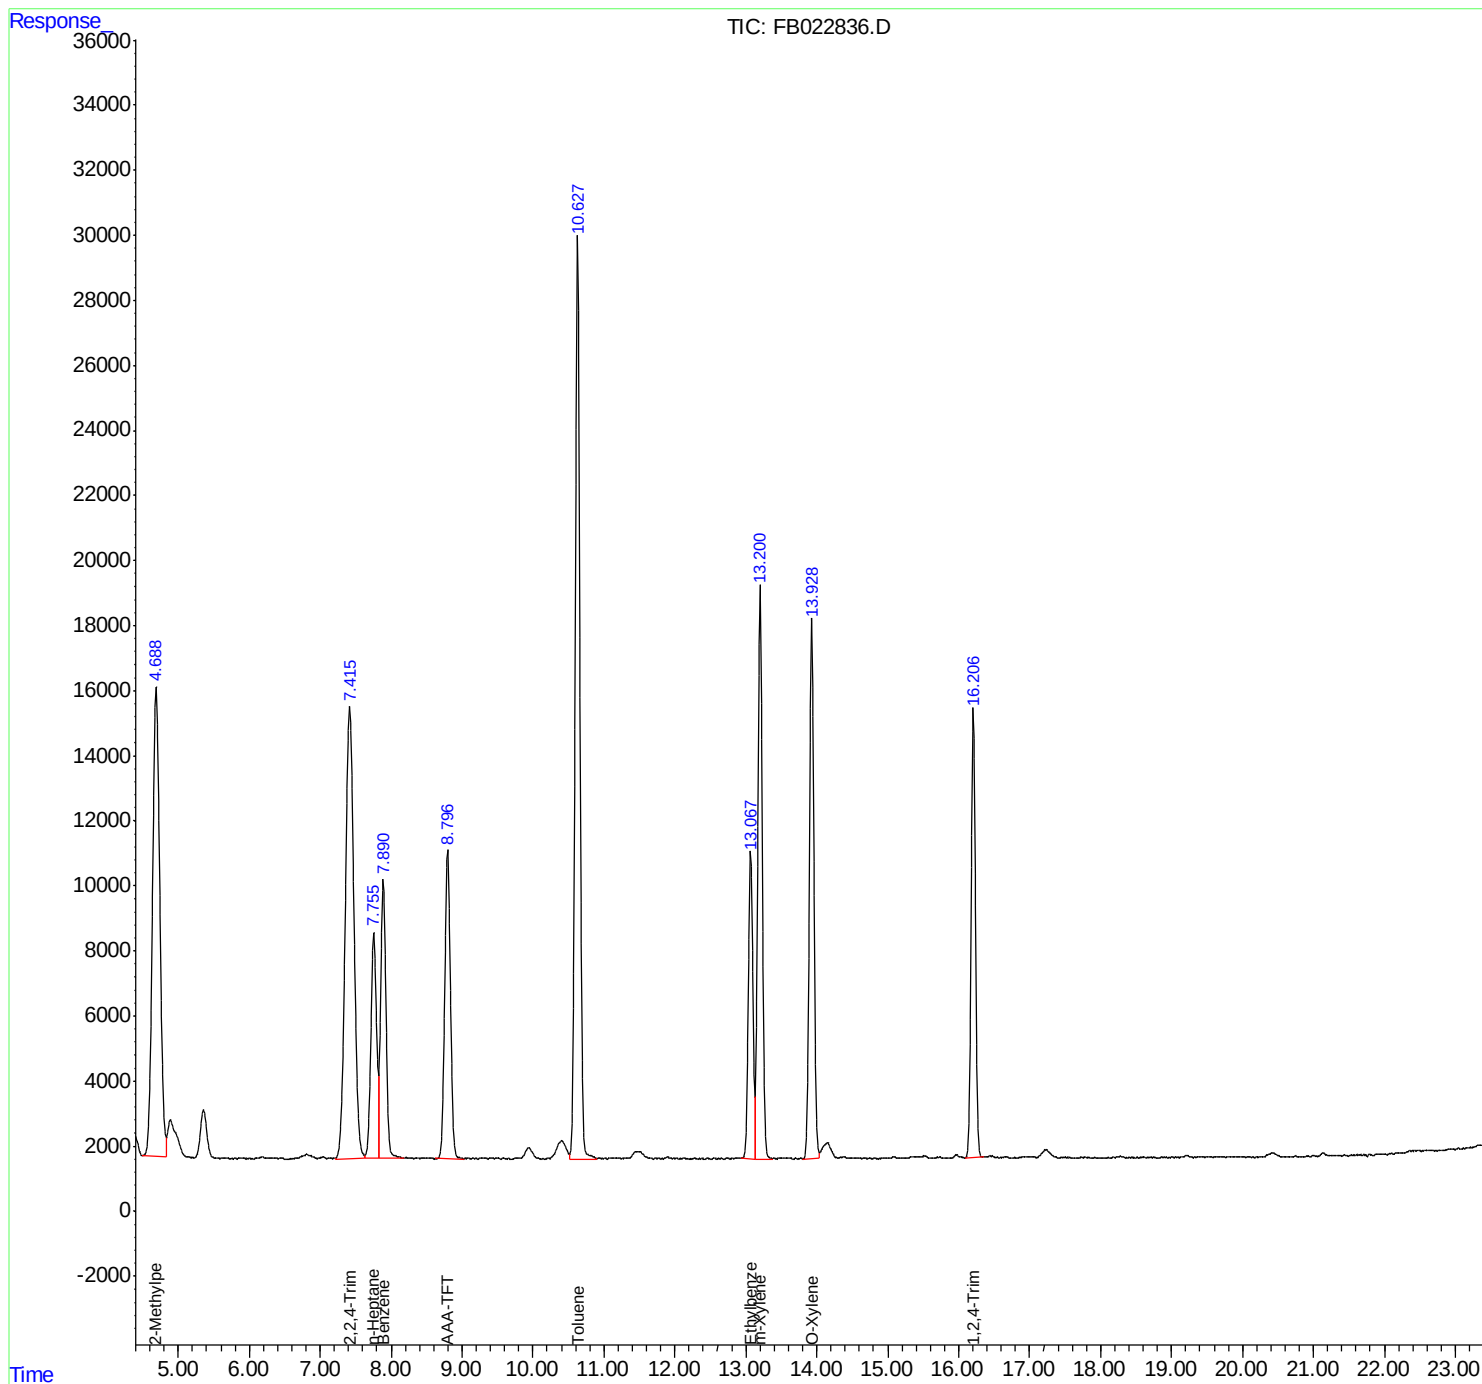

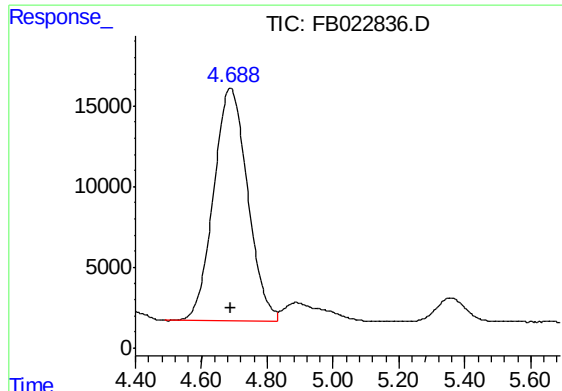


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.001 min
Response: 1035851
Conc: 30.48 ng/ml

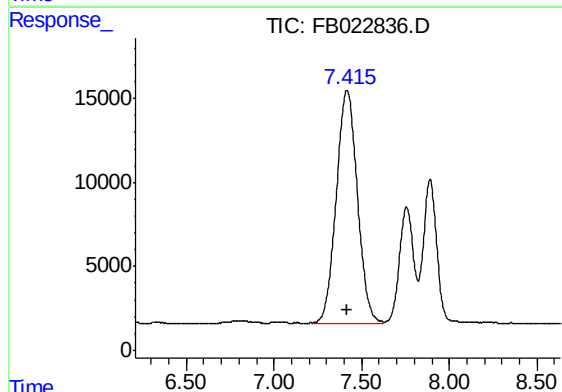


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 1163288
Conc: 31.97 ng/ml

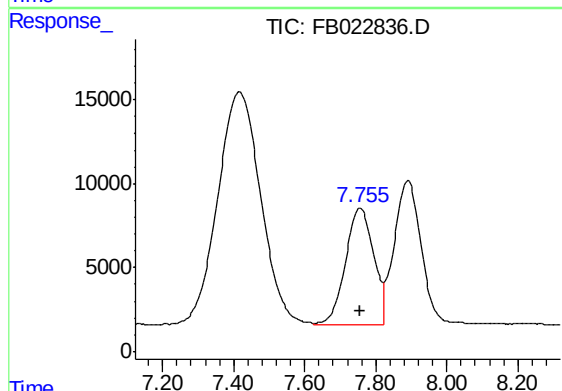


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.001 min
Response: 380959
Conc: 10.44 ng/ml

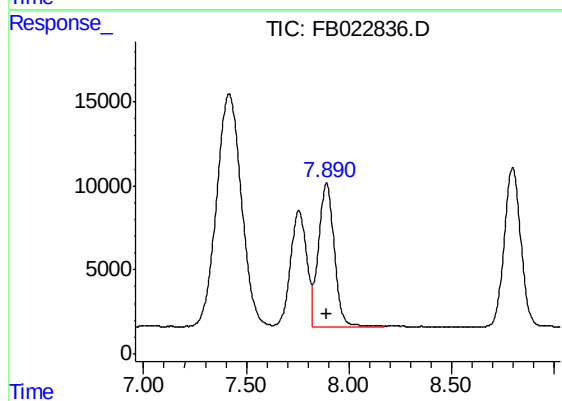


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 453335
Conc: 10.27 ng/ml

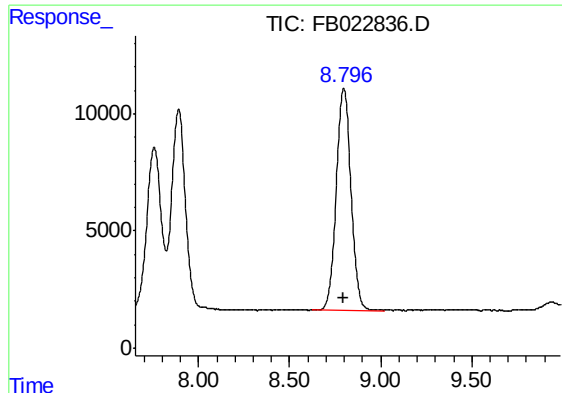


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 531166
Conc: 20.99 ng/ml

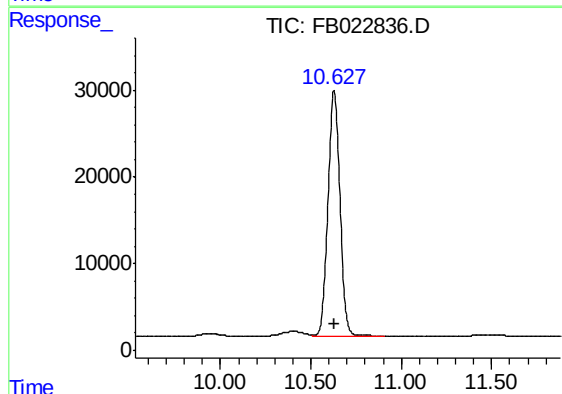


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 1317085
Conc: 30.56 ng/ml

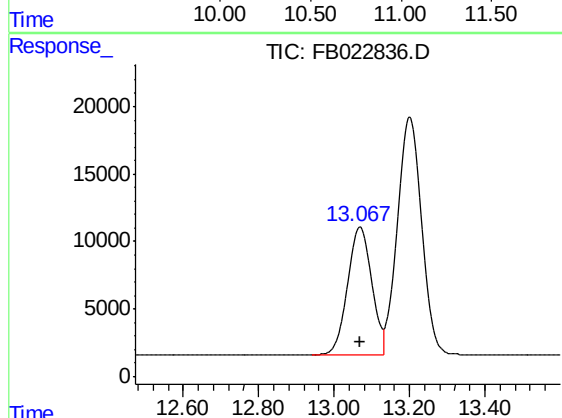


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 413756
Conc: 10.19 ng/ml

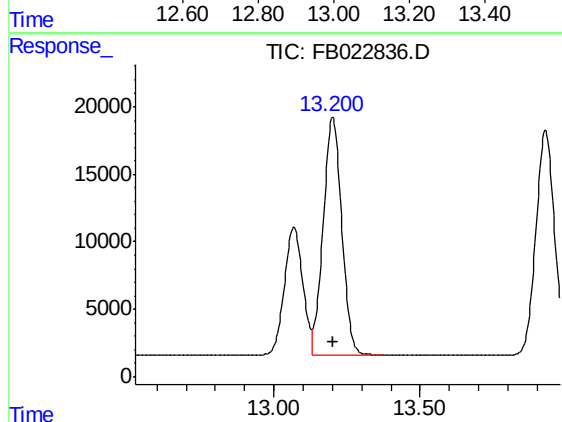


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.001 min
Response: 776606
Conc: 20.18 ng/ml

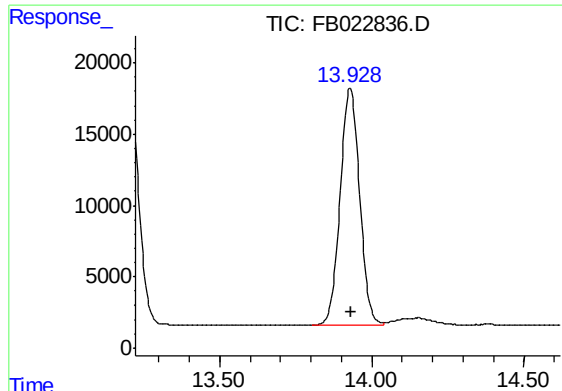

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.001 min
Response: 739222
Conc: 20.30 ng/ml

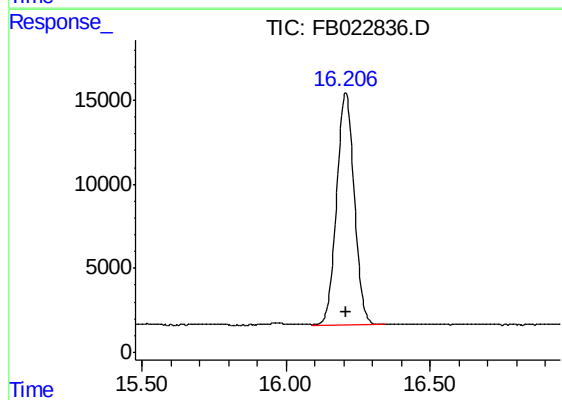

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 586400
Conc: 20.58 ng/ml