

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
 Data File : FB022839.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2019 12:54
 Operator : DD/AJ
 Sample : K5140-06MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Oct 29 08:38:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
 Quant Title :
 QLast Update : Wed Oct 16 15:04:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	572479	22.624 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	803176	23.633 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	818342	22.490 ng/ml
3) t n-Heptane	7.756	226680	6.213 ng/ml
4) t Benzene	7.890	356705	8.079 ng/ml
6) t Toluene	10.629	1067014	24.756 ng/ml
7) t Ethylbenzene	13.056	1558967	38.383 ng/ml
8) t m-Xylene	13.199	1399184	36.365 ng/ml
9) t O-Xylene	13.929	1400891	38.463 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	1963427	68.903 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102819\
Data File : FB022839.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2019 12:54
Operator : DD/AJ
Sample : K5140-06MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Oct 29 08:38:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB101619.M
Quant Title :
QLast Update : Wed Oct 16 15:04:00 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

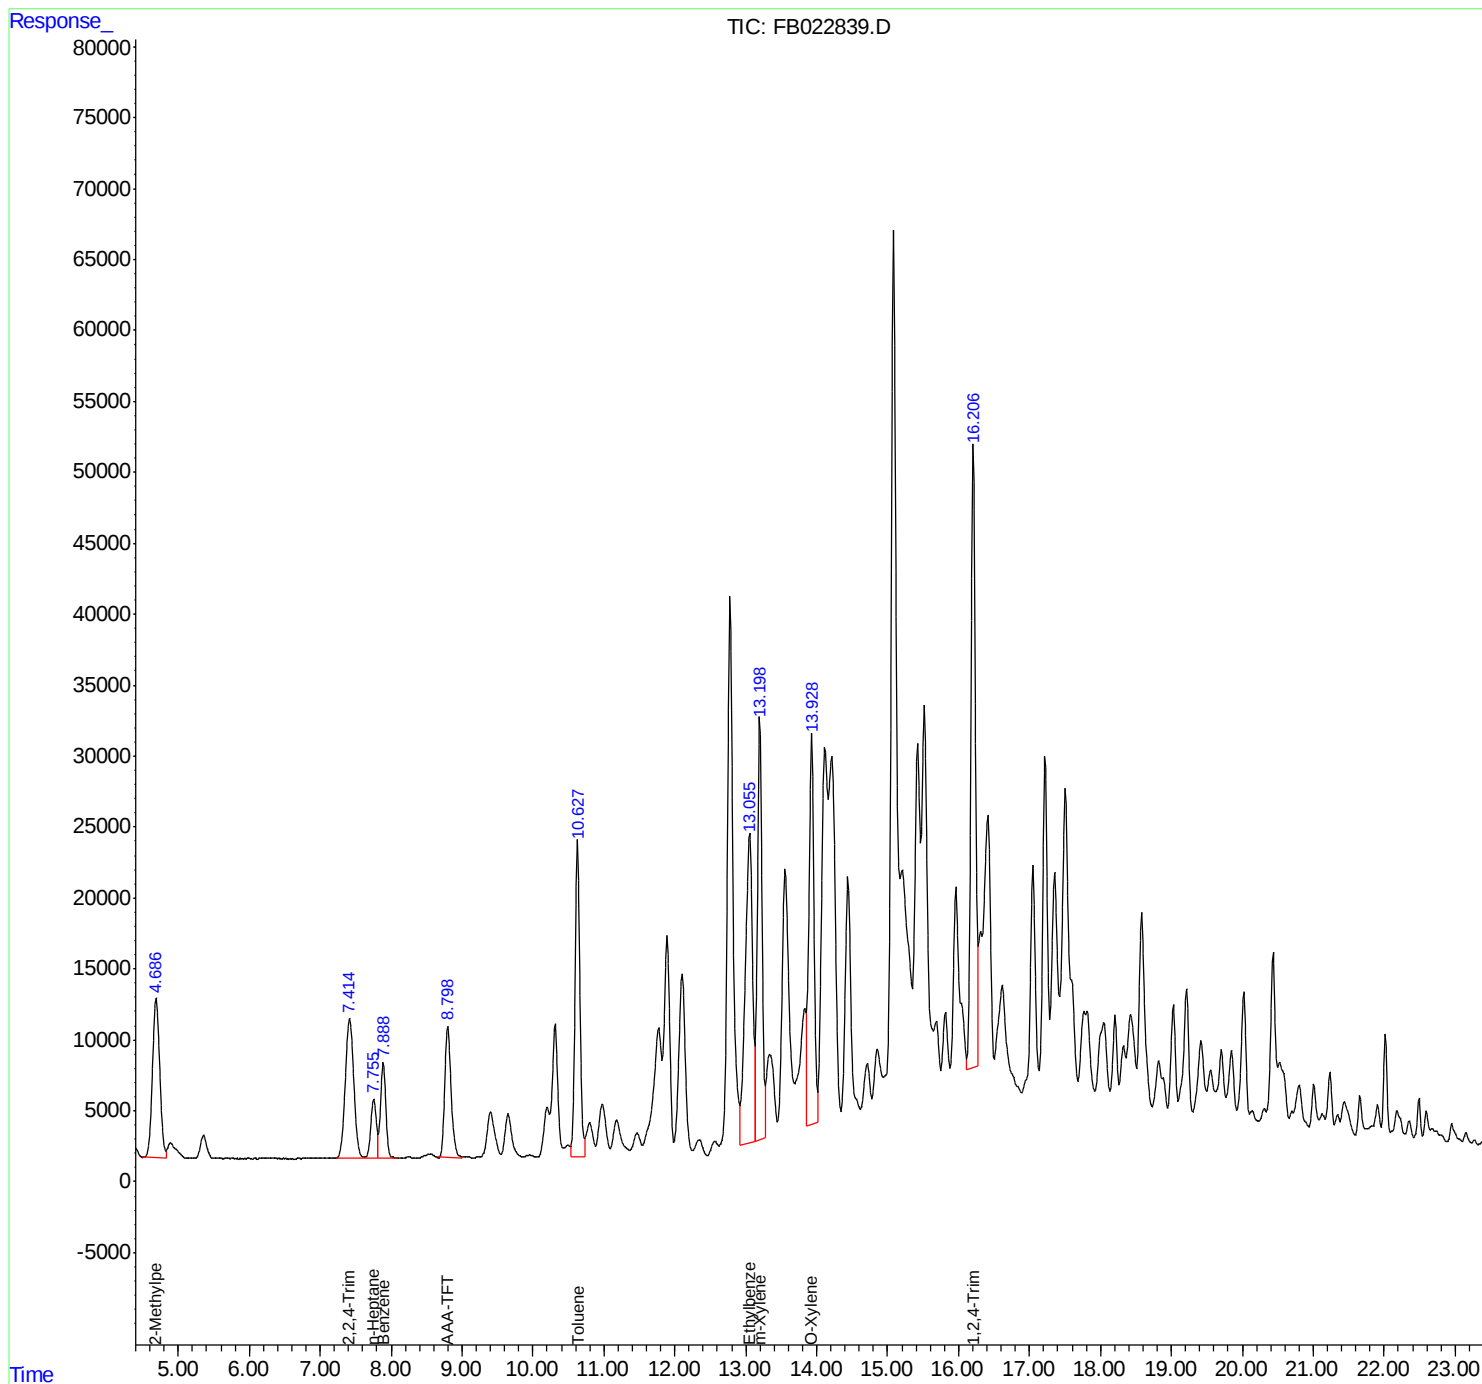

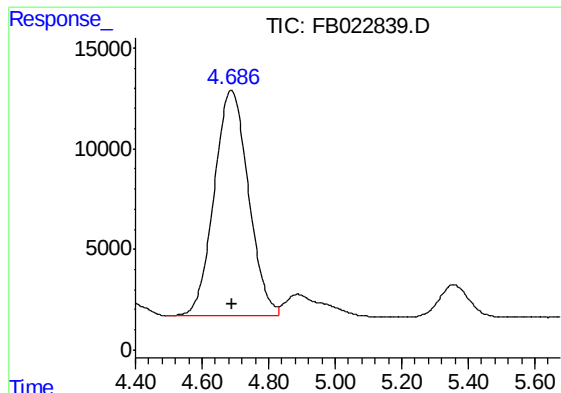


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 803176
Conc: 23.63 ng/ml

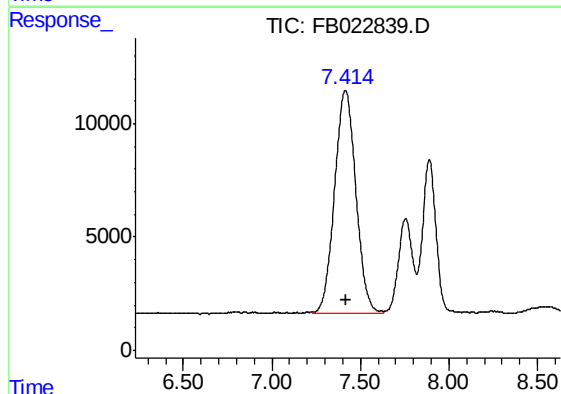


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 818342
Conc: 22.49 ng/ml

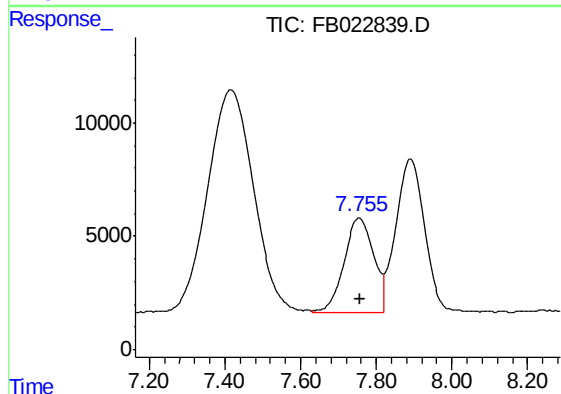


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 226680
Conc: 6.21 ng/ml

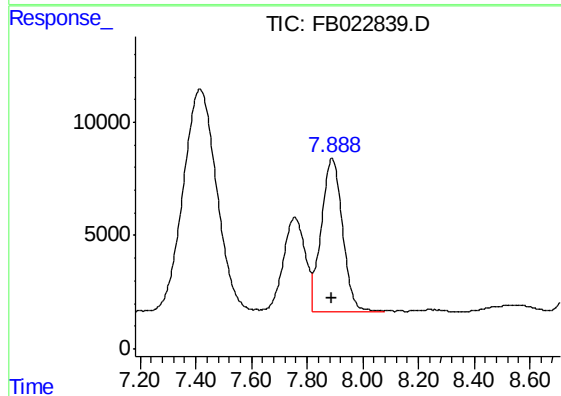


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 356705
Conc: 8.08 ng/ml

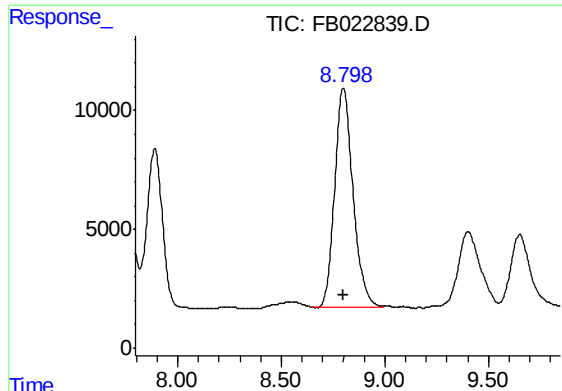


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.001 min
Response: 572479
Conc: 22.62 ng/ml

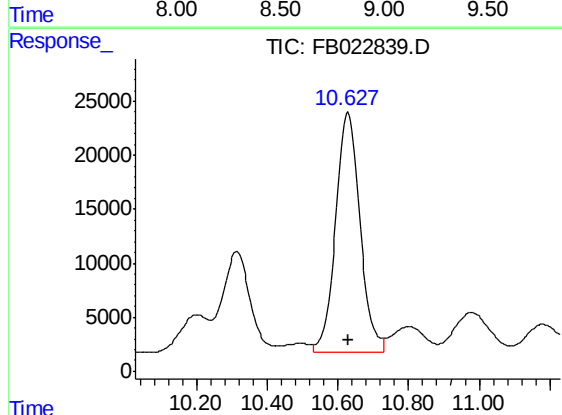


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 1067014
Conc: 24.76 ng/ml

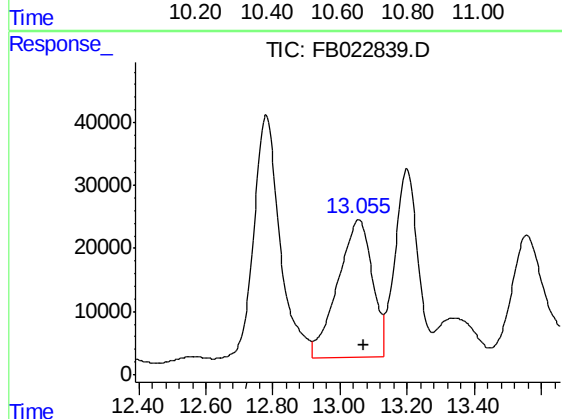


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.014 min
Response: 1558967
Conc: 38.38 ng/ml

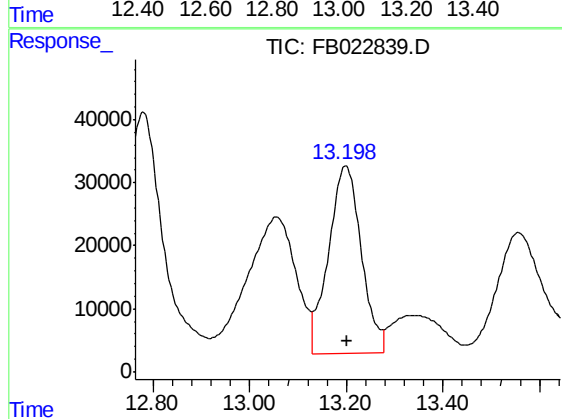


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.004 min
Response: 1399184
Conc: 36.37 ng/ml

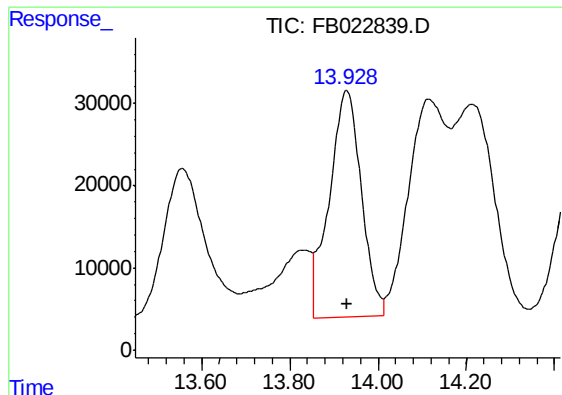

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.001 min
Response: 1400891
Conc: 38.46 ng/ml

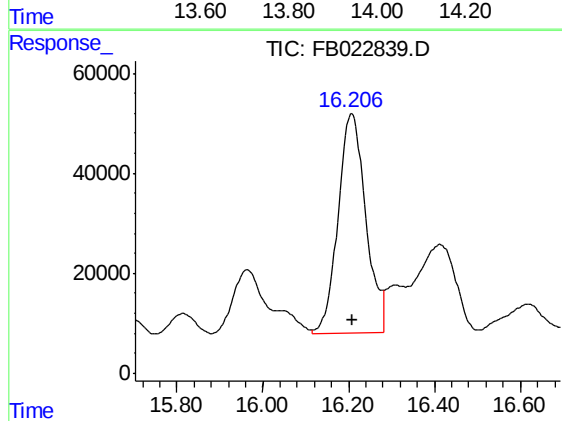

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 1963427
Conc: 68.90 ng/ml