

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102821\
 Data File : FB026324.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2021 10:56
 Operator : AJ/MA
 Sample : BSF1028S1
 Misc : 5.00G\5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 29 07:18:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	227065	19.167 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	532815	31.999 ng/ml
2) t 2,2,4-Trimethylpentane	7.440	630240	32.322 ng/ml
3) t n-Heptane	7.755	195702	10.607 ng/ml
4) t Benzene	7.892	232087	10.646 ng/ml
6) t Toluene	10.628	660370	31.839 ng/ml
7) t Ethylbenzene	13.069	205142	10.863 ng/ml
8) t m-Xylene	13.202	412070	21.665 ng/ml
9) t O-Xylene	13.930	399685	21.640 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	413847	21.830 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102821\
Data File : FB026324.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2021 10:56
Operator : AJ/MA
Sample : BSF1028S1
Misc : 5.00G\5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 29 07:18:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

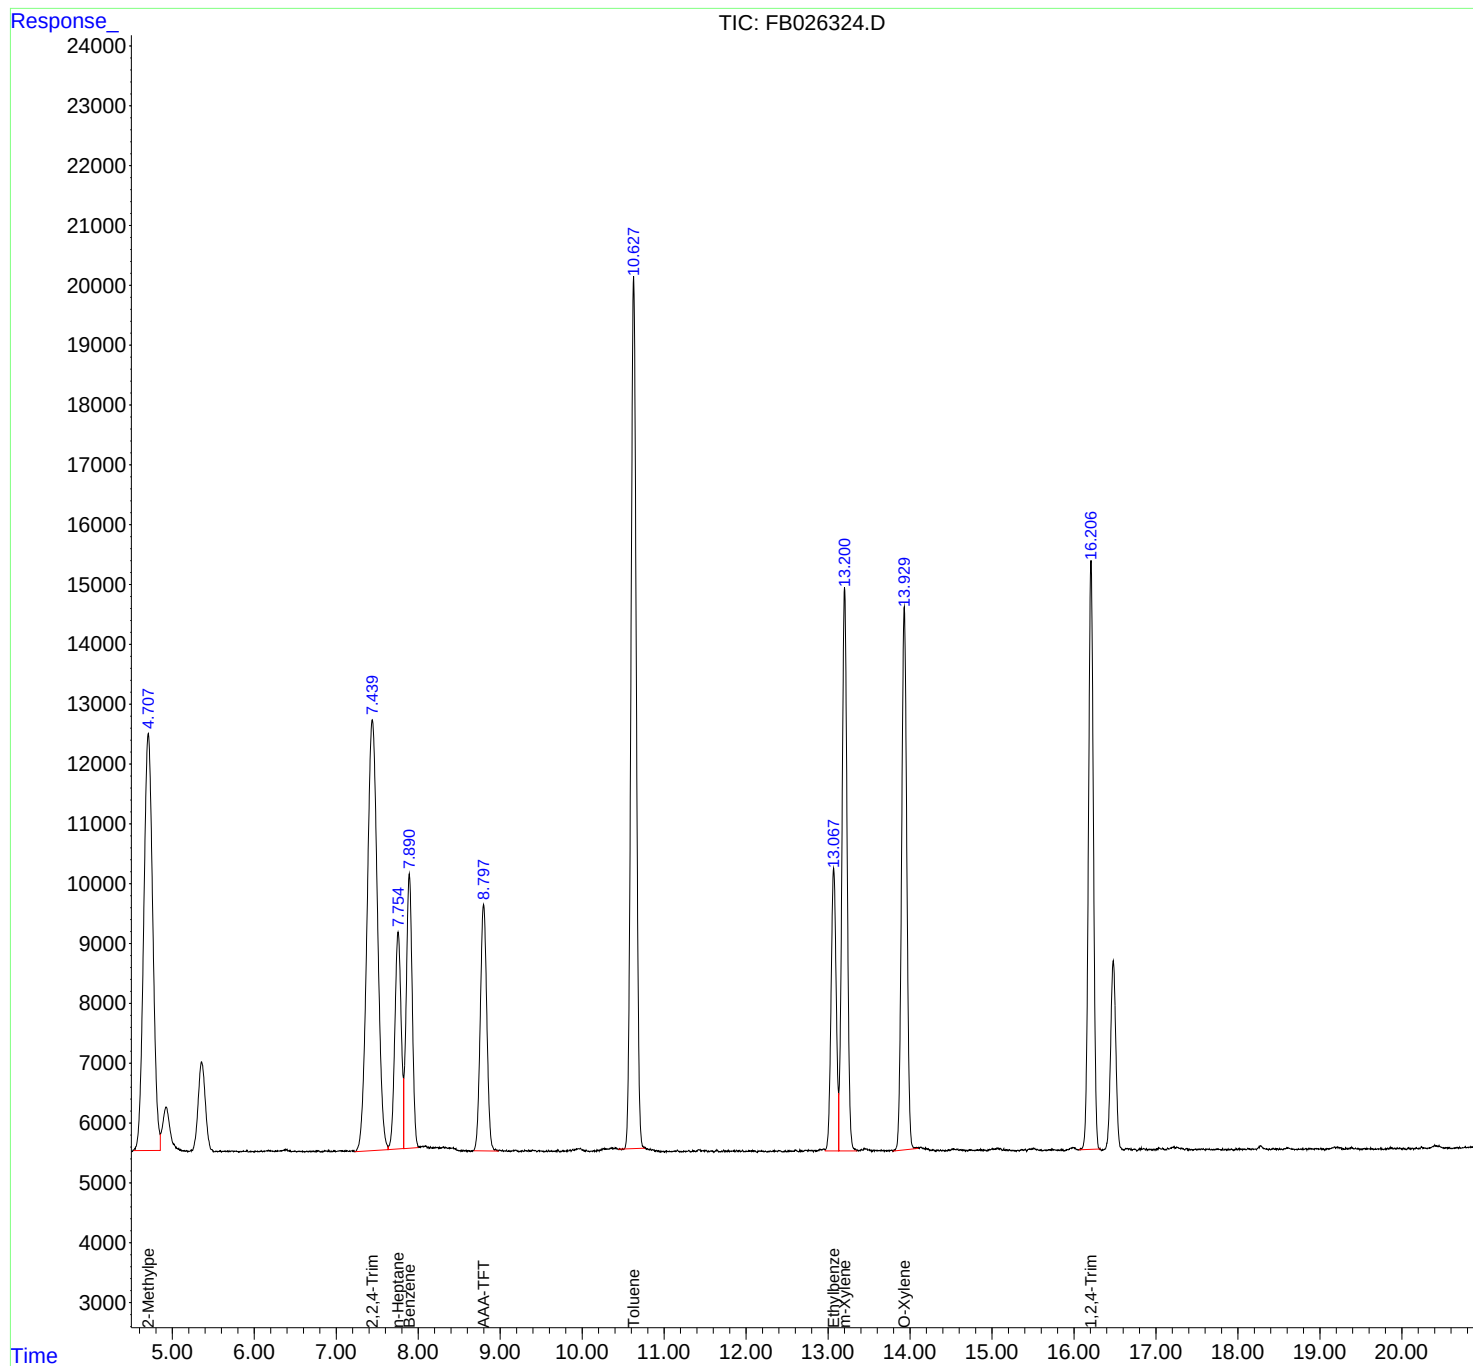


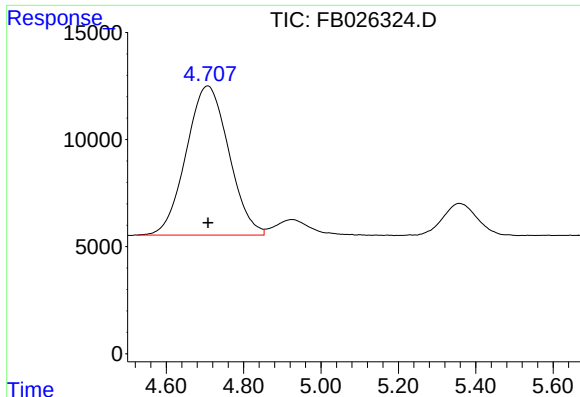

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 532815
Conc: 32.00 ng/ml

Instrument :
FID_B
ClientSampleId :

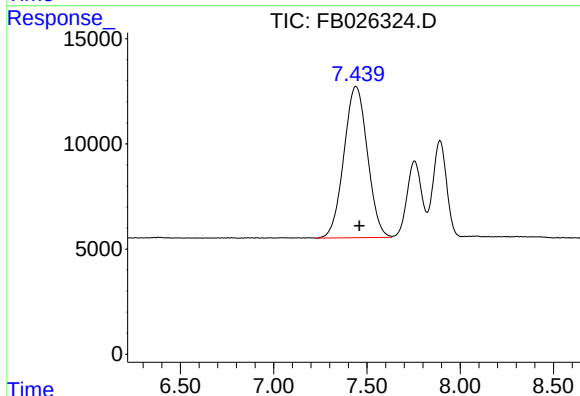


#2 2,2,4-Trimethylpentane

R.T.: 7.440 min
Delta R.T.: -0.019 min
Response: 630240
Conc: 32.32 ng/ml

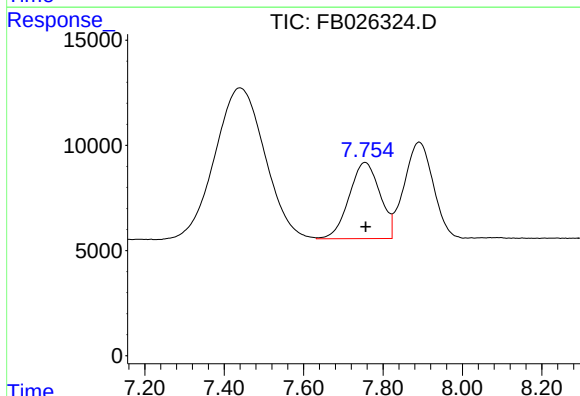


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.001 min
Response: 195702
Conc: 10.61 ng/ml

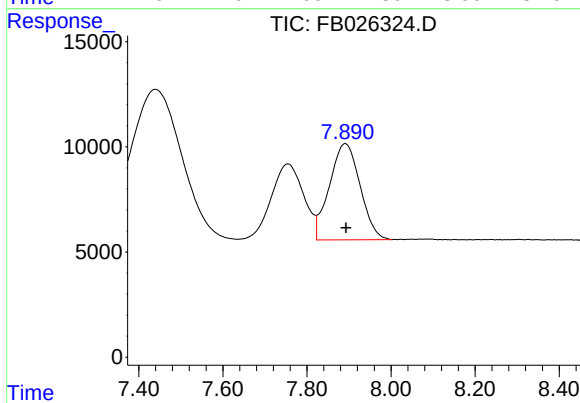

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.002 min
Response: 232087
Conc: 10.65 ng/ml

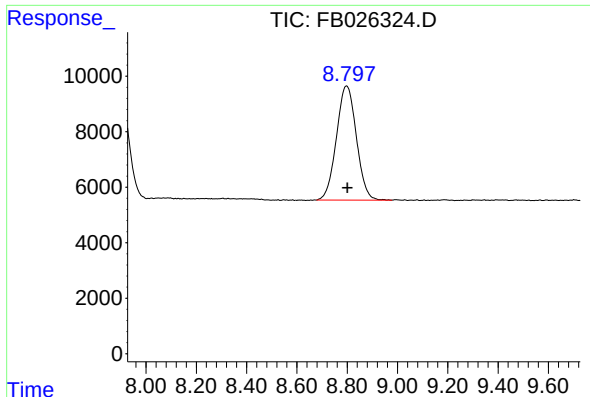

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.003 min
Response: 227065
Conc: 19.17 ng/ml

Instrument :
FID_B
ClientSampleId :

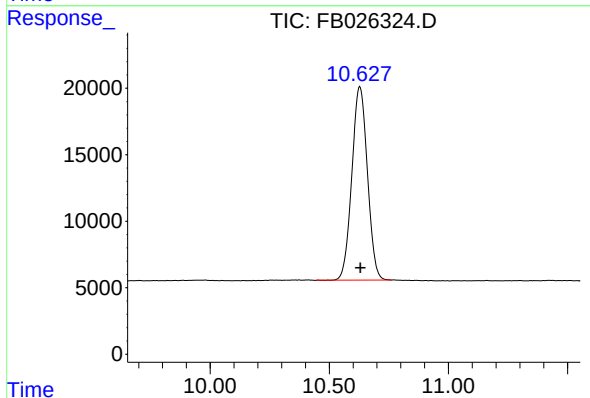


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 660370
Conc: 31.84 ng/ml

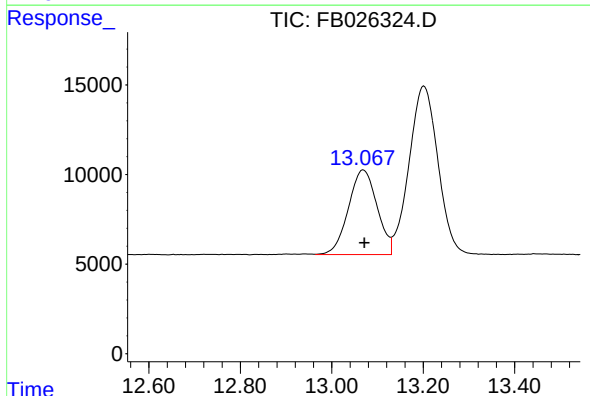


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.003 min
Response: 205142
Conc: 10.86 ng/ml

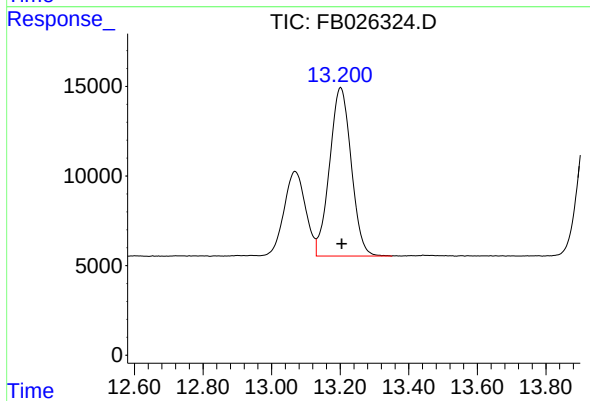

#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.003 min
Response: 412070
Conc: 21.66 ng/ml

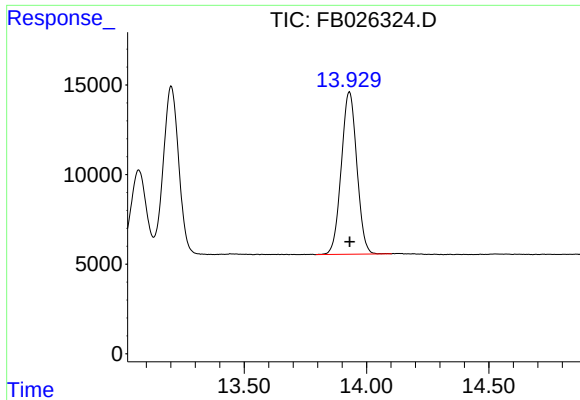

#9 O-Xylene


R.T.: 13.930 min

Delta R.T.: -0.002 min

Response: 399685

Conc: 21.64 ng/ml

Instrument :
FID_B
ClientSampleId :

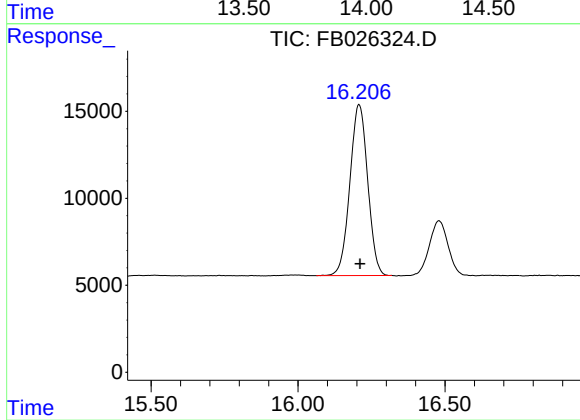

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min

Delta R.T.: -0.003 min

Response: 413847

Conc: 21.83 ng/ml