

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102821\
 Data File : FB026327.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2021 12:46
 Operator : AJ/MA
 Sample : M4380-01MS
 Misc : 5.01\5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 29 07:18:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	226654	19.132 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	394670	23.703 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	367721	18.858 ng/ml
3) t n-Heptane	7.756	116461	6.312 ng/ml
4) t Benzene	7.893	192333	8.822 ng/ml
6) t Toluene	10.630	559831	26.992 ng/ml
7) t Ethylbenzene	13.069	172542	9.137 ng/ml
8) t m-Xylene	13.203	339795	17.865 ng/ml
9) t O-Xylene	13.930	328962	17.811 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	328279	17.316 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102821\
Data File : FB026327.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2021 12:46
Operator : AJ/MA
Sample : M4380-01MS
Misc : 5.01\5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 29 07:18:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

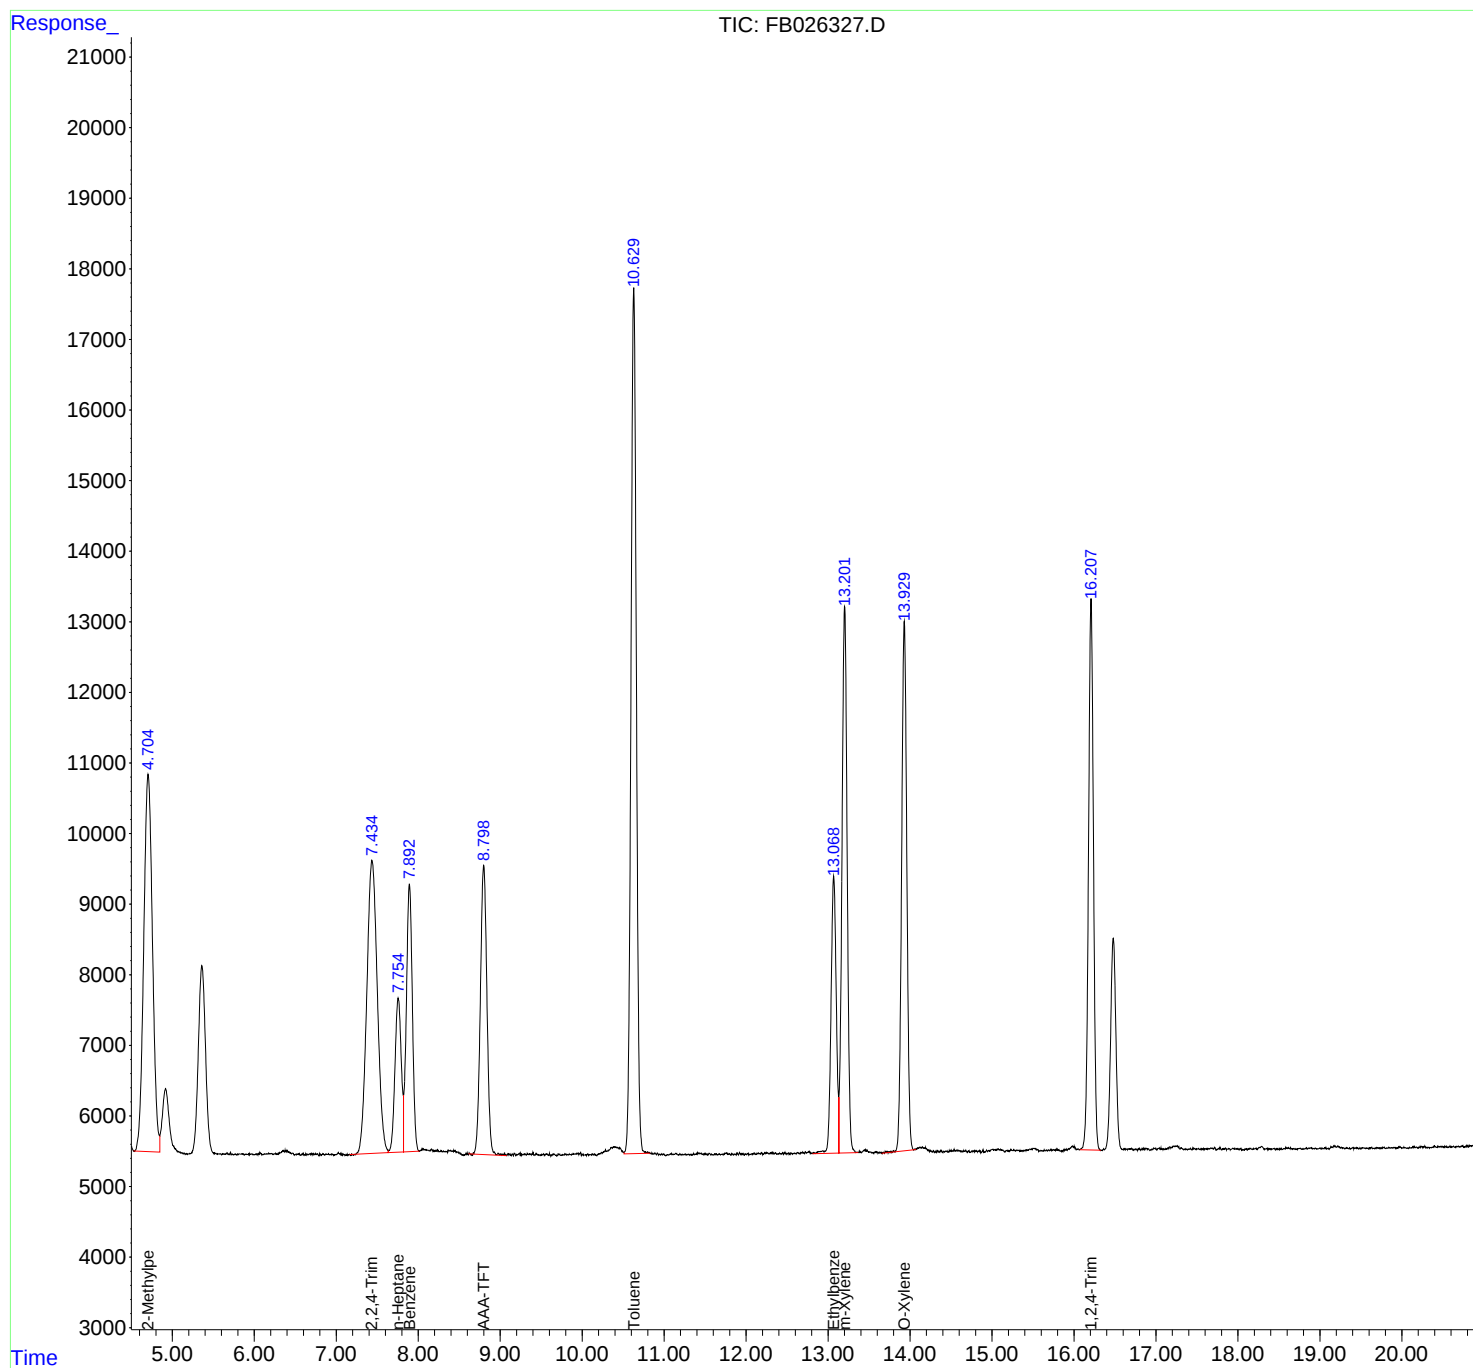


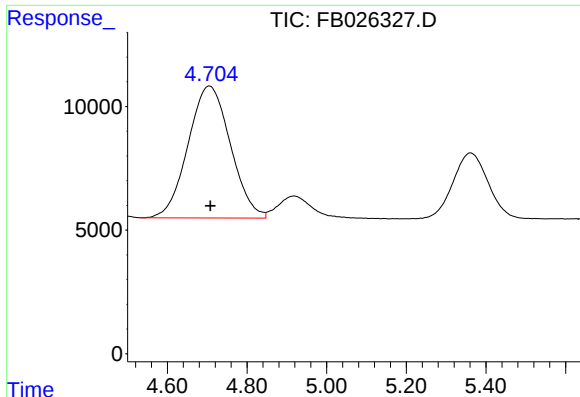

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.003 min
Response: 394670
Conc: 23.70 ng/ml

Instrument :
FID_B
ClientSampleId :

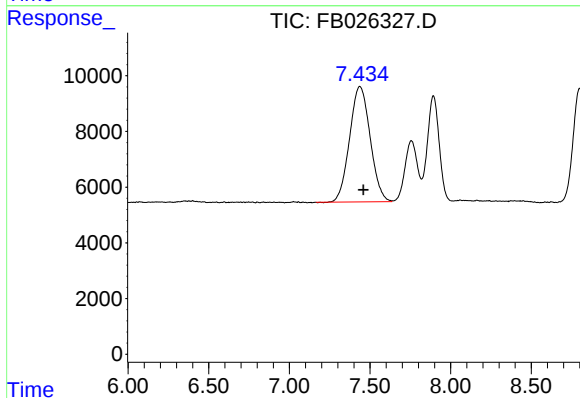


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: -0.024 min
Response: 367721
Conc: 18.86 ng/ml

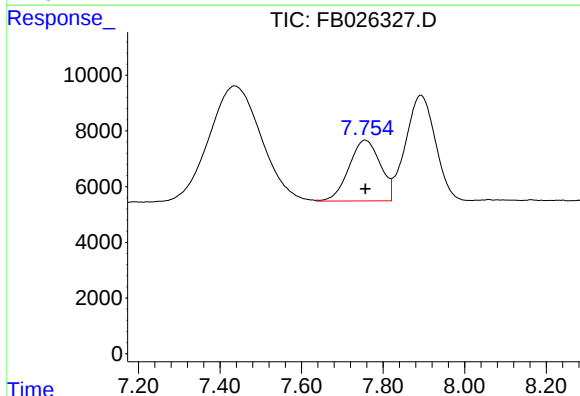


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 116461
Conc: 6.31 ng/ml

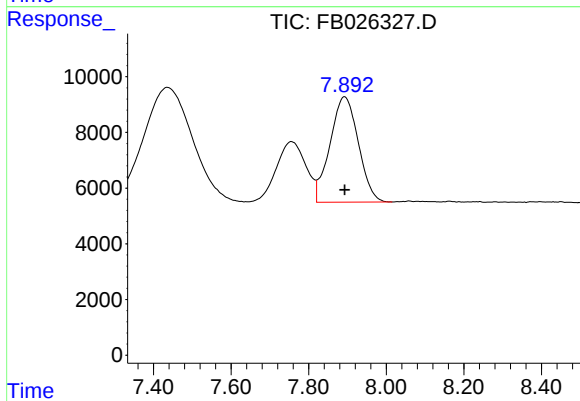

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 192333
Conc: 8.82 ng/ml

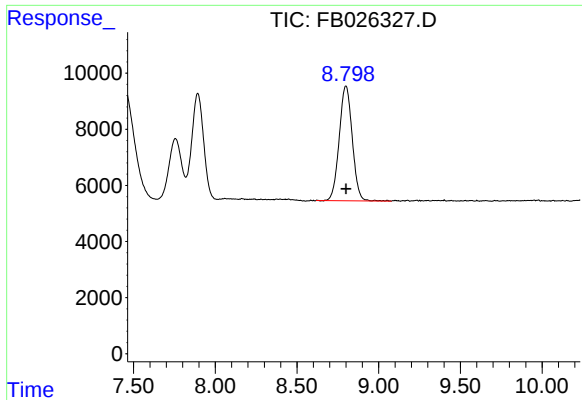

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 226654
Conc: 19.13 ng/ml

Instrument :
FID_B
ClientSampleId :

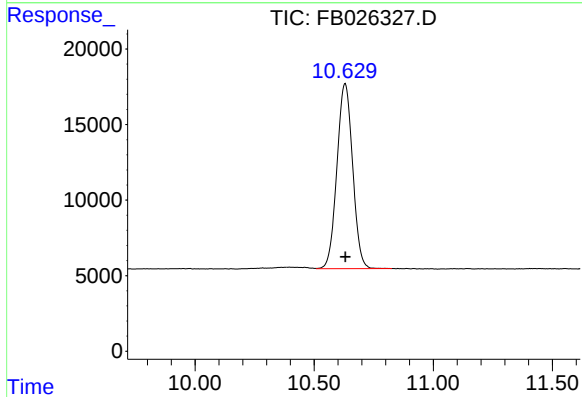


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.001 min
Response: 559831
Conc: 26.99 ng/ml

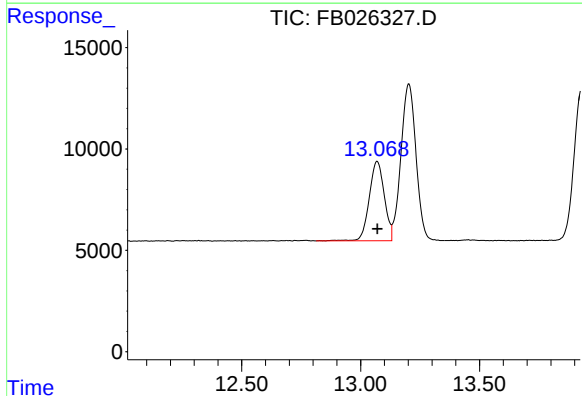


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 172542
Conc: 9.14 ng/ml

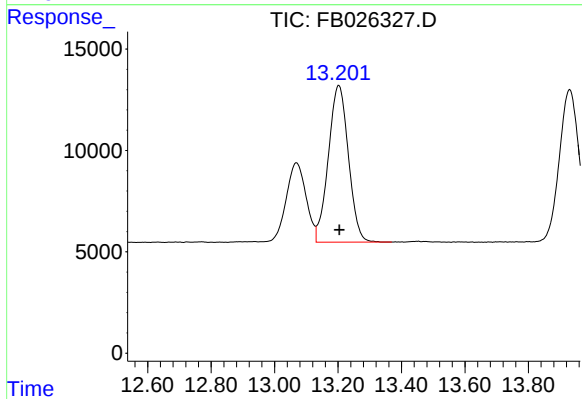

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.002 min
Response: 339795
Conc: 17.87 ng/ml

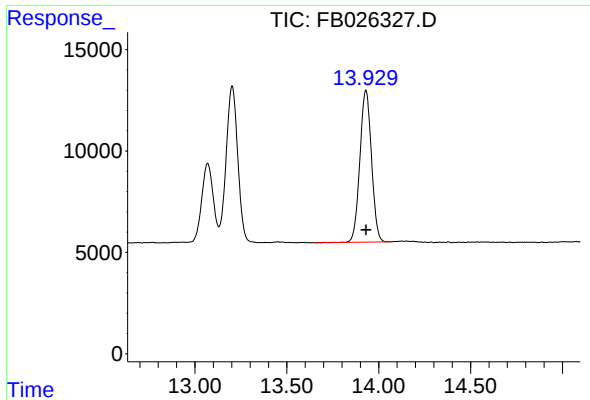

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 328962
Conc: 17.81 ng/ml

Instrument :
FID_B
ClientSampleId :

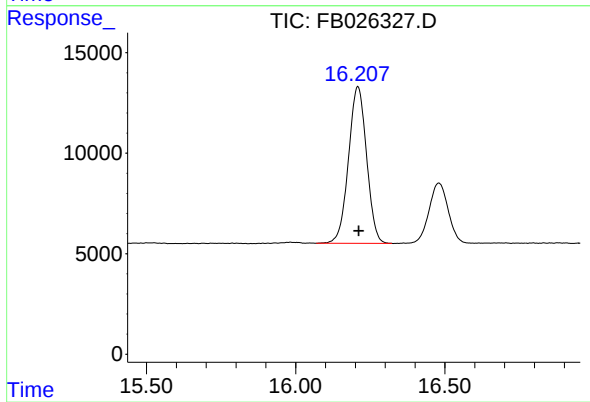

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 328279
Conc: 17.32 ng/ml