

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102821\
 Data File : FB026328.D
 Signal(s) : FID2B.CH
 Acq On : 28 Oct 2021 13:22
 Operator : AJ/MA
 Sample : M4380-01MSD
 Misc : 5.04\5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WASTE-CHAR-(SUSPECT)MSD

Integration File: SAMPLE.e
 Quant Time: Oct 29 07:18:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
 Quant Title :
 QLast Update : Thu Oct 28 05:34:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	216070	18.238 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	365095	21.926 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	301833	15.479 ng/ml
3) t n-Heptane	7.758	97960	5.309 ng/ml
4) t Benzene	7.894	187794	8.614 ng/ml
6) t Toluene	10.630	530681	25.586 ng/ml
7) t Ethylbenzene	13.070	157228	8.326 ng/ml
8) t m-Xylene	13.203	315204	16.572 ng/ml
9) t O-Xylene	13.931	302531	16.380 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	287394	15.159 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB102821\
Data File : FB026328.D
Signal(s) : FID2B.CH
Acq On : 28 Oct 2021 13:22
Operator : AJ/MA
Sample : M4380-01MSD
Misc : 5.04\5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WASTE-CHAR-(SUSPECT)MSD

Integration File: SAMPLE.e
Quant Time: Oct 29 07:18:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102721.M
Quant Title :
QLast Update : Thu Oct 28 05:34:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

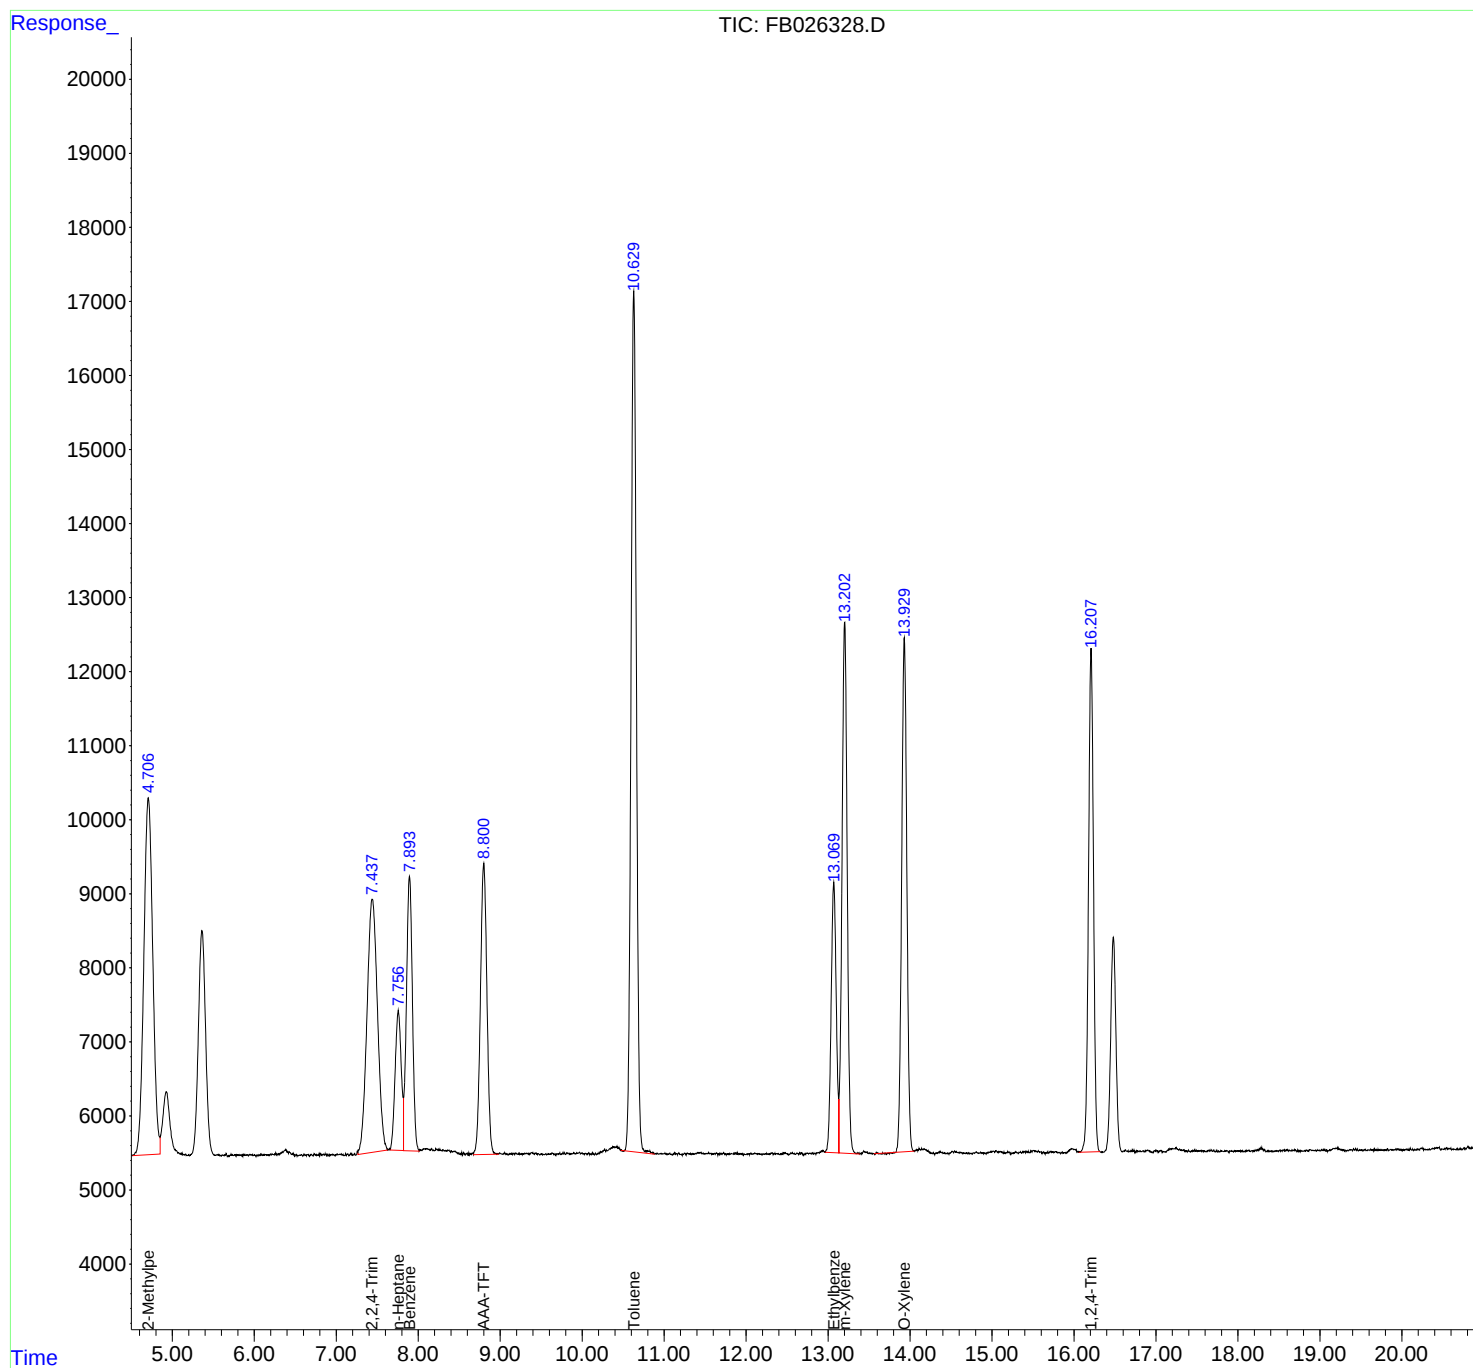


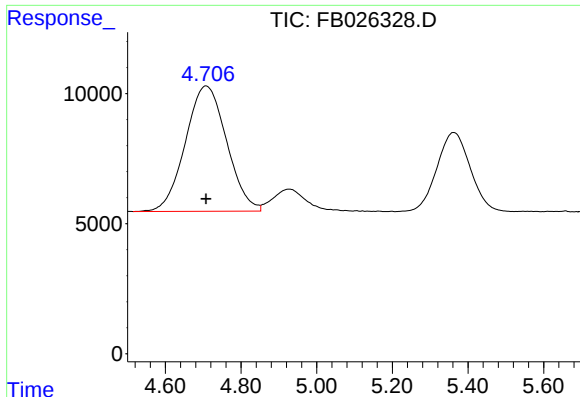

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 365095
Conc: 21.93 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTE-CHAR-(SUSPECT)MSD

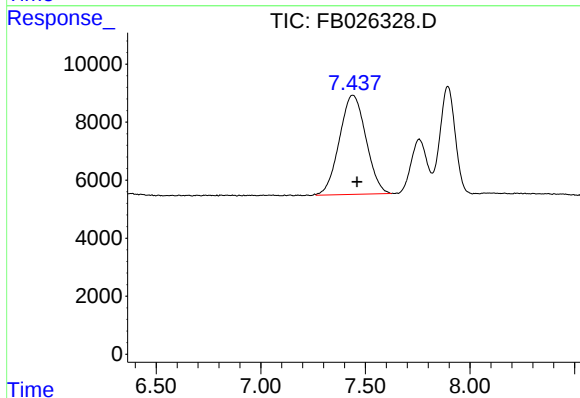


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: -0.021 min
Response: 301833
Conc: 15.48 ng/ml

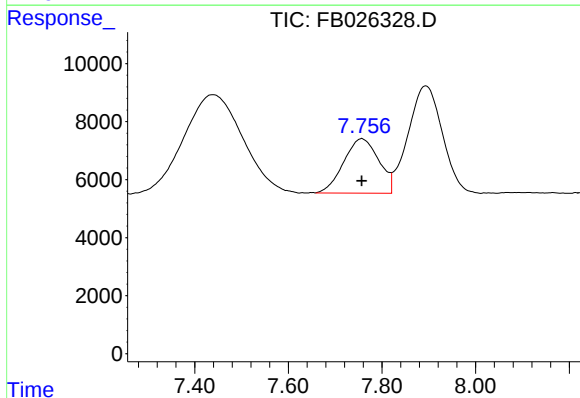


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 97960
Conc: 5.31 ng/ml

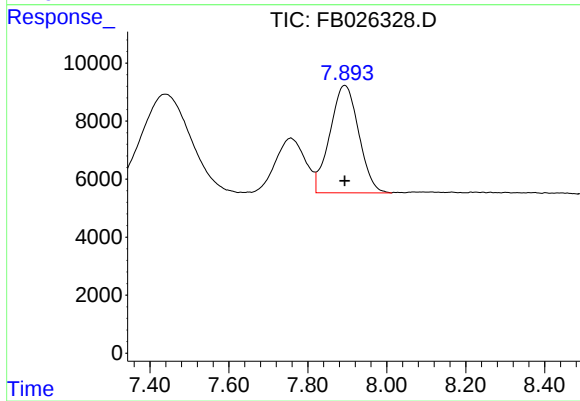

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 187794
Conc: 8.61 ng/ml

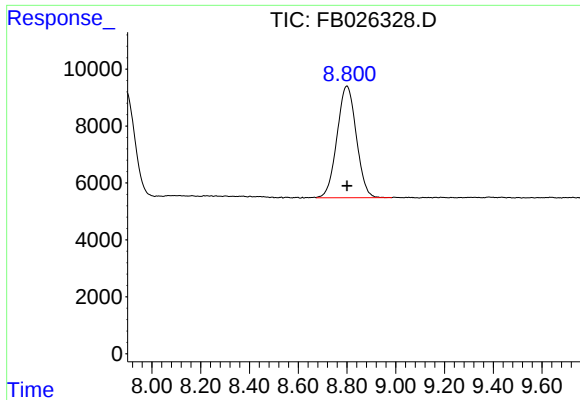

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 216070
Conc: 18.24 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTE-CHAR-(SUSPECT)MSD

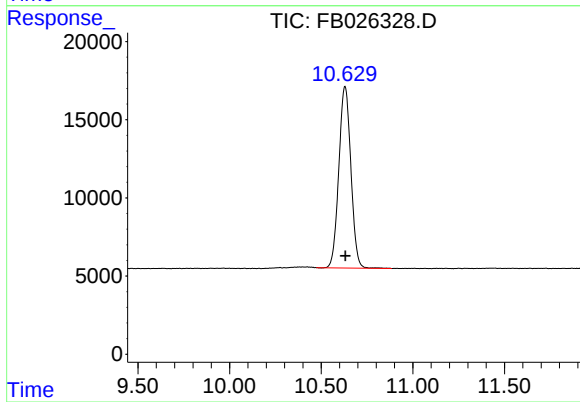


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.001 min
Response: 530681
Conc: 25.59 ng/ml

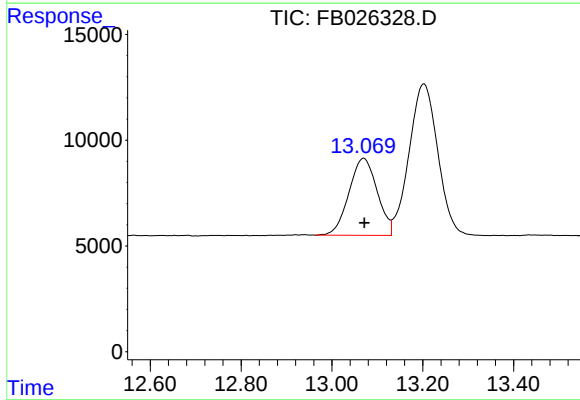


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.001 min
Response: 157228
Conc: 8.33 ng/ml

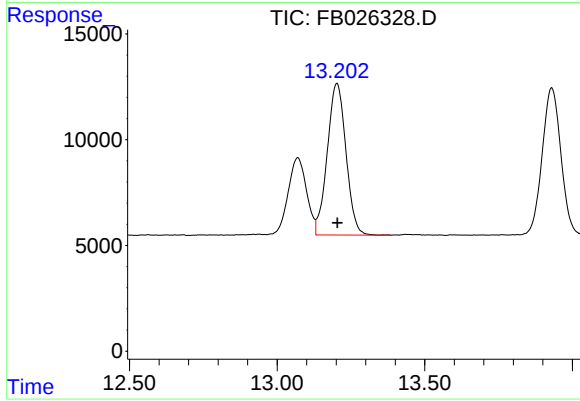

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.002 min
Response: 315204
Conc: 16.57 ng/ml

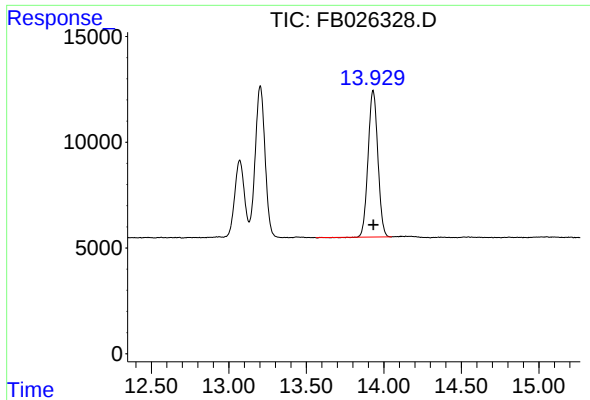

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 302531
Conc: 16.38 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTE-CHAR-(SUSPECT)MSD

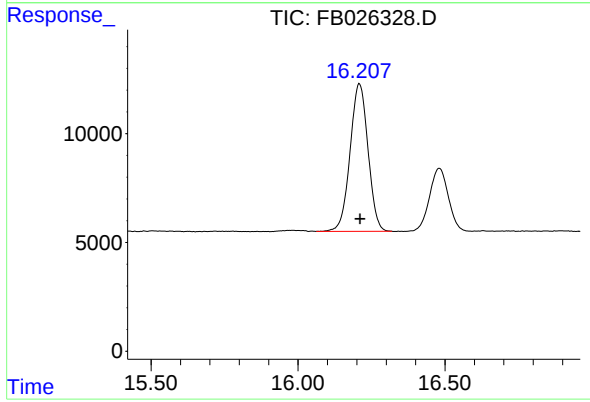

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 287394
Conc: 15.16 ng/ml